
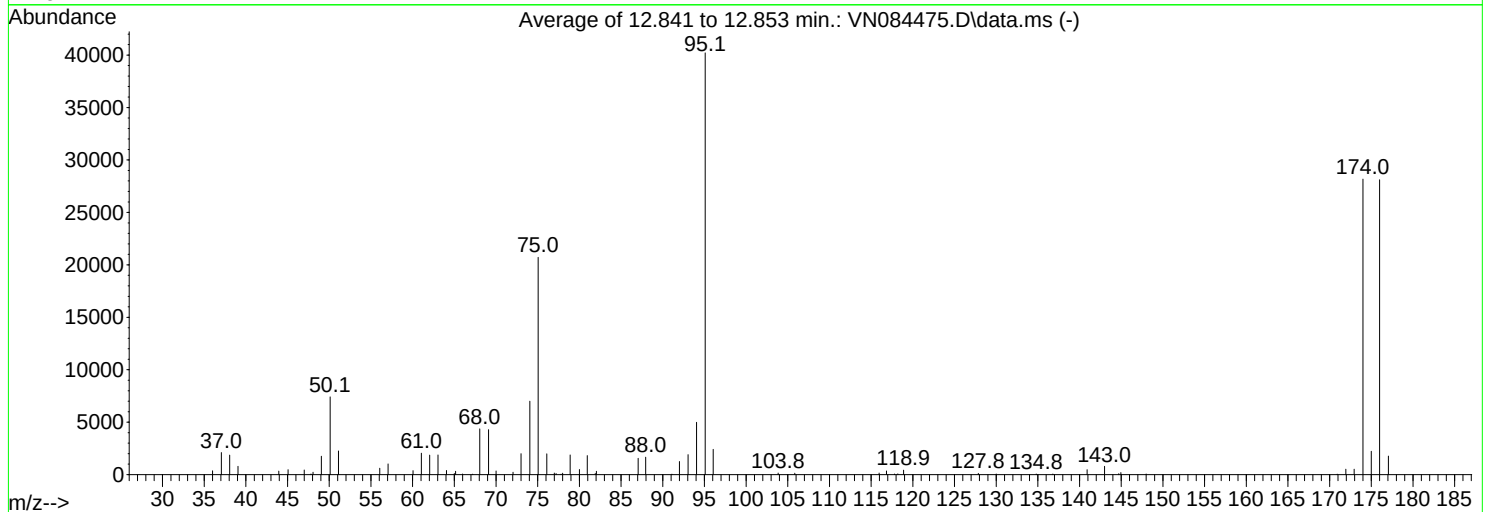


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102424\
Data File : VN084475.D
Acq On : 24 Oct 2024 08:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

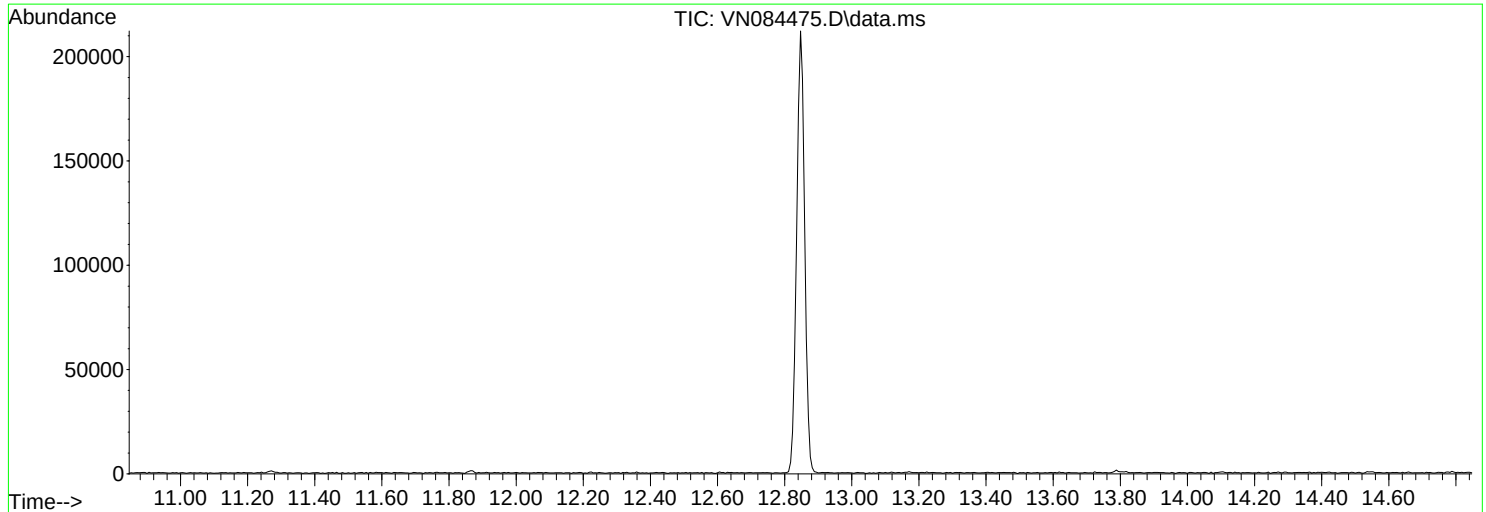

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	7411	PASS
75	95	30	60	51.5	20720	PASS
95	95	100	100	100.0	40213	PASS
96	95	5	9	6.0	2419	PASS
173	174	0.00	2	1.8	513	PASS
174	95	50	100	70.1	28181	PASS
175	174	5	9	7.9	2225	PASS
176	174	95	101	99.8	28120	PASS
177	176	5	9	6.3	1769	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	365	51.10	2262	67.20	53	77.80	51
37.05	2103	56.05	609	68.05	4360	78.00	141
38.05	1867	57.05	1029	69.10	4280	78.90	187
39.05	788	60.05	385	70.00	358	80.00	48
43.95	337	61.05	2053	72.05	233	80.95	1815
45.05	469	62.05	1854	73.00	2006	81.90	102
47.00	440	63.05	1880	74.05	6997	82.05	326
47.80	58	64.05	403	75.05	20720	87.05	1559
48.05	233	65.00	110	76.10	1979	87.95	1671
49.05	1750	65.15	326	77.00	154	91.10	52
50.10	7411	66.00	67	77.20	111	92.00	1247

Average of 12.841 to 12.853 min.: VN084475.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.05	1906	127.85	131	172.95	513		
94.05	4994	130.00	67	174.00	28181		
95.10	40213	134.80	55	175.00	2225		
96.05	2419	136.80	59	176.00	28120		
103.85	155	140.90	476	177.05	1769		
105.85	141	143.00	790				
115.95	153	144.70	91				
116.85	352	144.95	196				
117.80	56	148.00	60				
118.20	73	170.90	53				
118.90	429	171.95	527				

Instrument :
MSVOA_N
ClientSampleId :
BFB