

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102524\
 Data File : VN084521.D
 Acq On : 25 Oct 2024 17:14
 Operator : JC\MD
 Sample : P4528-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 241023068-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
 Title : SW846 8260

Signal : TIC: VN084521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.148	30	33	40	rVB	10033	17644	2.24%	0.335%
2	2.489	85	91	100	rVB2	11806	21419	2.72%	0.406%
3	3.965	334	342	353	rVB	16869	41492	5.28%	0.787%
4	4.448	416	424	436	rVB3	8613	25368	3.23%	0.481%
5	5.524	594	607	618	rBV2	34344	123607	15.72%	2.344%
6	7.430	920	931	944	rBV	100034	279423	35.55%	5.299%
7	7.841	990	1001	1018	rBV2	105877	279850	35.60%	5.307%
8	8.165	1045	1056	1061	rBV	127742	304696	38.76%	5.778%
9	8.224	1061	1066	1079	rVB	205086	447263	56.90%	8.481%
10	8.577	1117	1126	1136	rBV	141054	325210	41.37%	6.167%
11	9.100	1206	1215	1225	rBV	290307	597051	75.95%	11.322%
12	9.694	1307	1316	1326	rVB5	7324	16391	2.09%	0.311%
13	10.565	1456	1464	1473	rBV	428363	786094	100.00%	14.907%
14	11.171	1557	1567	1575	rBV	5058	10691	1.36%	0.203%
15	11.306	1584	1590	1600	rBV2	9537	18350	2.33%	0.348%
16	11.865	1675	1685	1701	rBV	389824	768869	97.81%	14.580%
17	12.847	1845	1852	1861	rVB	290743	495109	62.98%	9.389%
18	13.606	1972	1981	1987	rBV2	8692	13922	1.77%	0.264%
19	13.788	2005	2012	2023	rBV2	354457	677029	86.13%	12.838%
20	14.100	2061	2065	2071	rBV5	5907	8801	1.12%	0.167%
21	15.276	2258	2265	2271	rBV7	8328	15205	1.93%	0.288%




Sum of corrected areas: 5273484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102524\
Data File : VN084521.D
Acq On : 25 Oct 2024 17:14
Operator : JC\MD
Sample : P4528-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
241023068-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

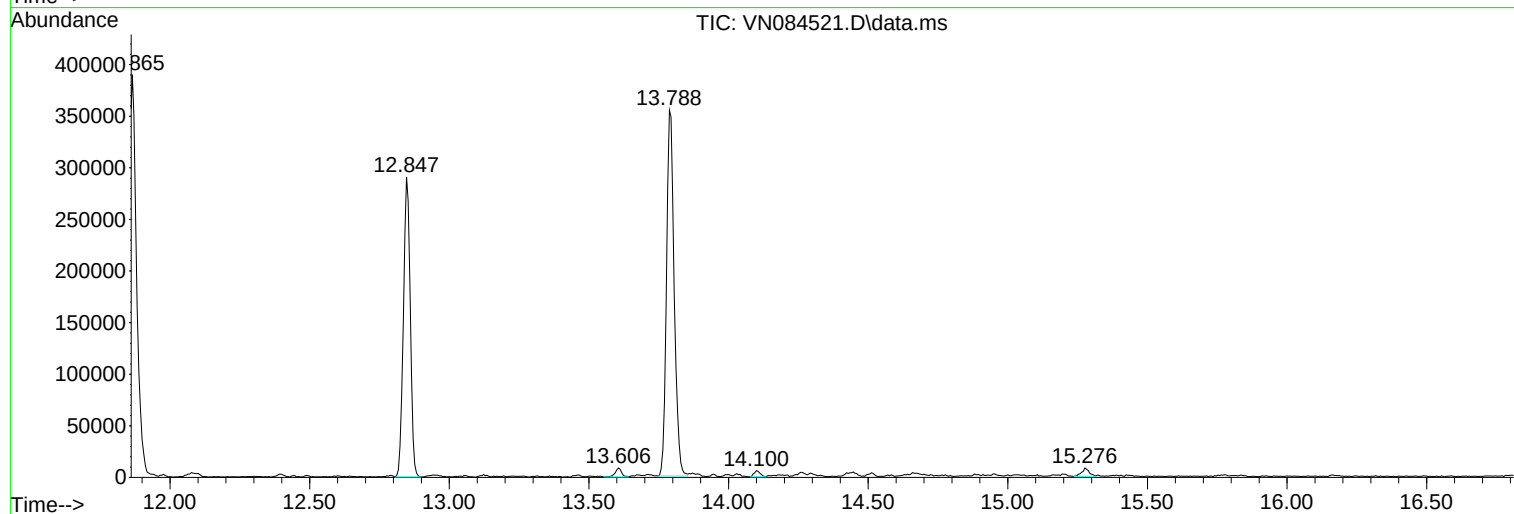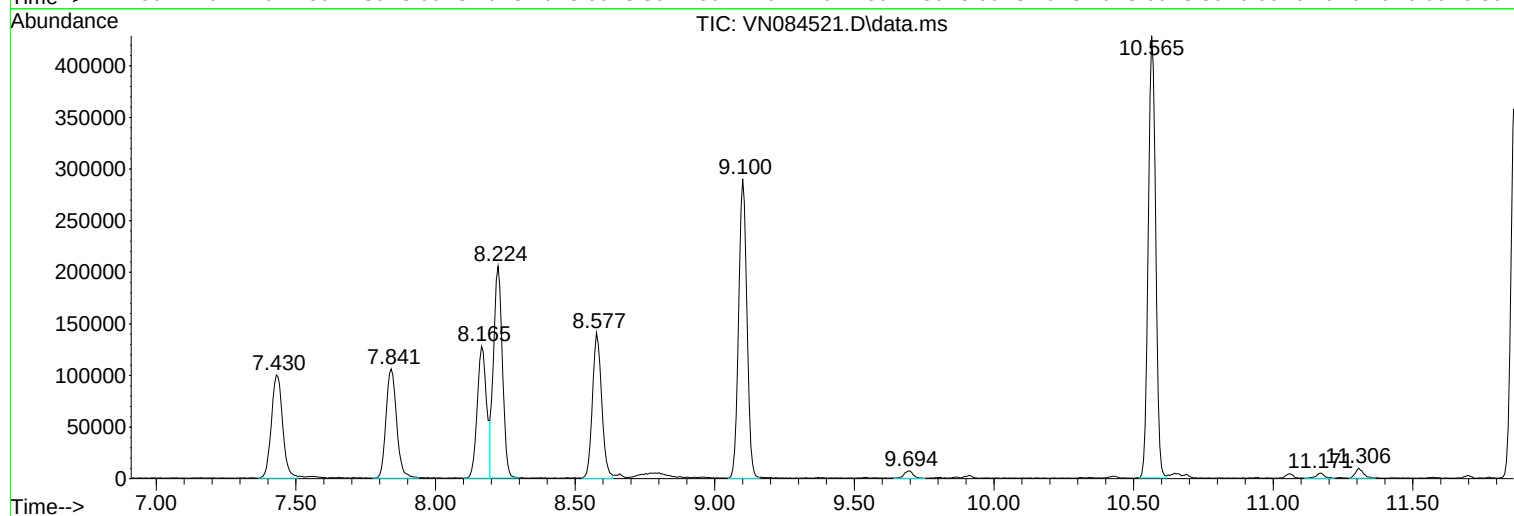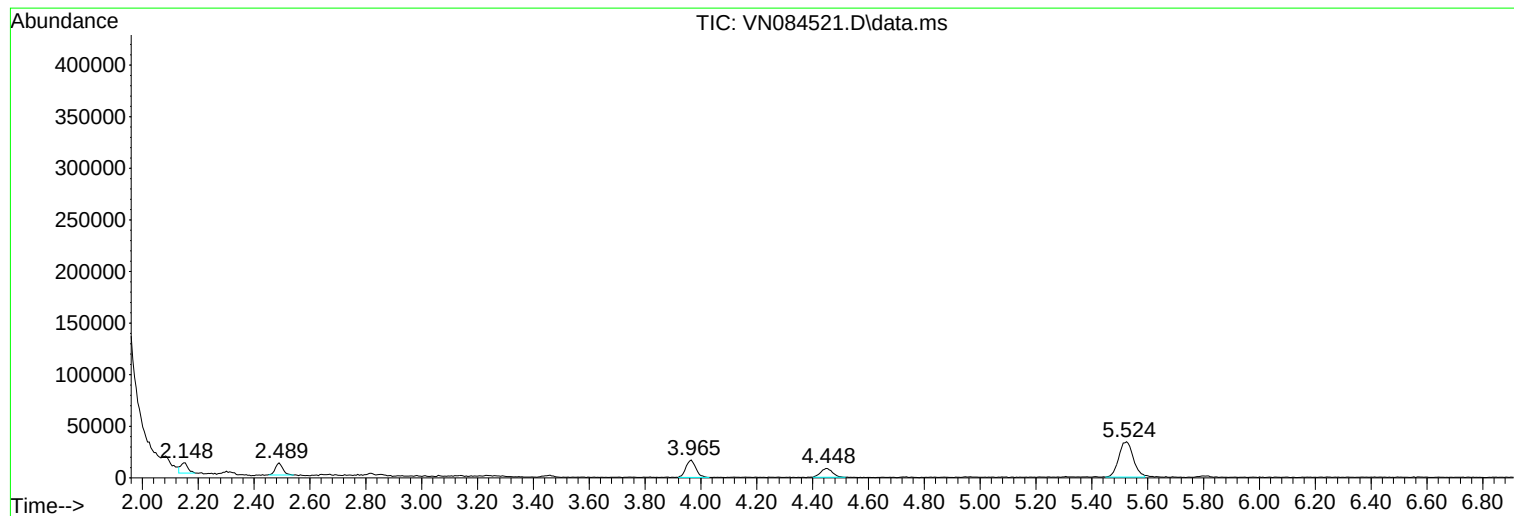

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102524\
Data File : VN084521.D
Acq On : 25 Oct 2024 17:14
Operator : JC\MD
Sample : P4528-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
241023068-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102524\
Data File : VN084521.D
Acq On : 25 Oct 2024 17:14
Operator : JC\MD
Sample : P4528-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
241023068-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
