

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102824\
 Data File : VN084539.D
 Acq On : 28 Oct 2024 15:05
 Operator : JC\MD
 Sample : P4550-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB-190-GW-338-340

Quant Time: Oct 28 18:34:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 01 07:11:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	150803	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	267490	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	231312	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	94475	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	113726	50.863	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 101.720%	
35) Dibromofluoromethane	8.165	113	91484	51.878	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.760%	
50) Toluene-d8	10.565	98	319558	49.254	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 98.500%	
62) 4-Bromofluorobenzene	12.847	95	107270	45.384	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 90.760%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102824\
Data File : VN084539.D
Acq On : 28 Oct 2024 15:05
Operator : JC\MD
Sample : P4550-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-190-GW-338-340

Quant Time: Oct 28 18:34:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 01 07:11:01 2024
Response via : Initial Calibration




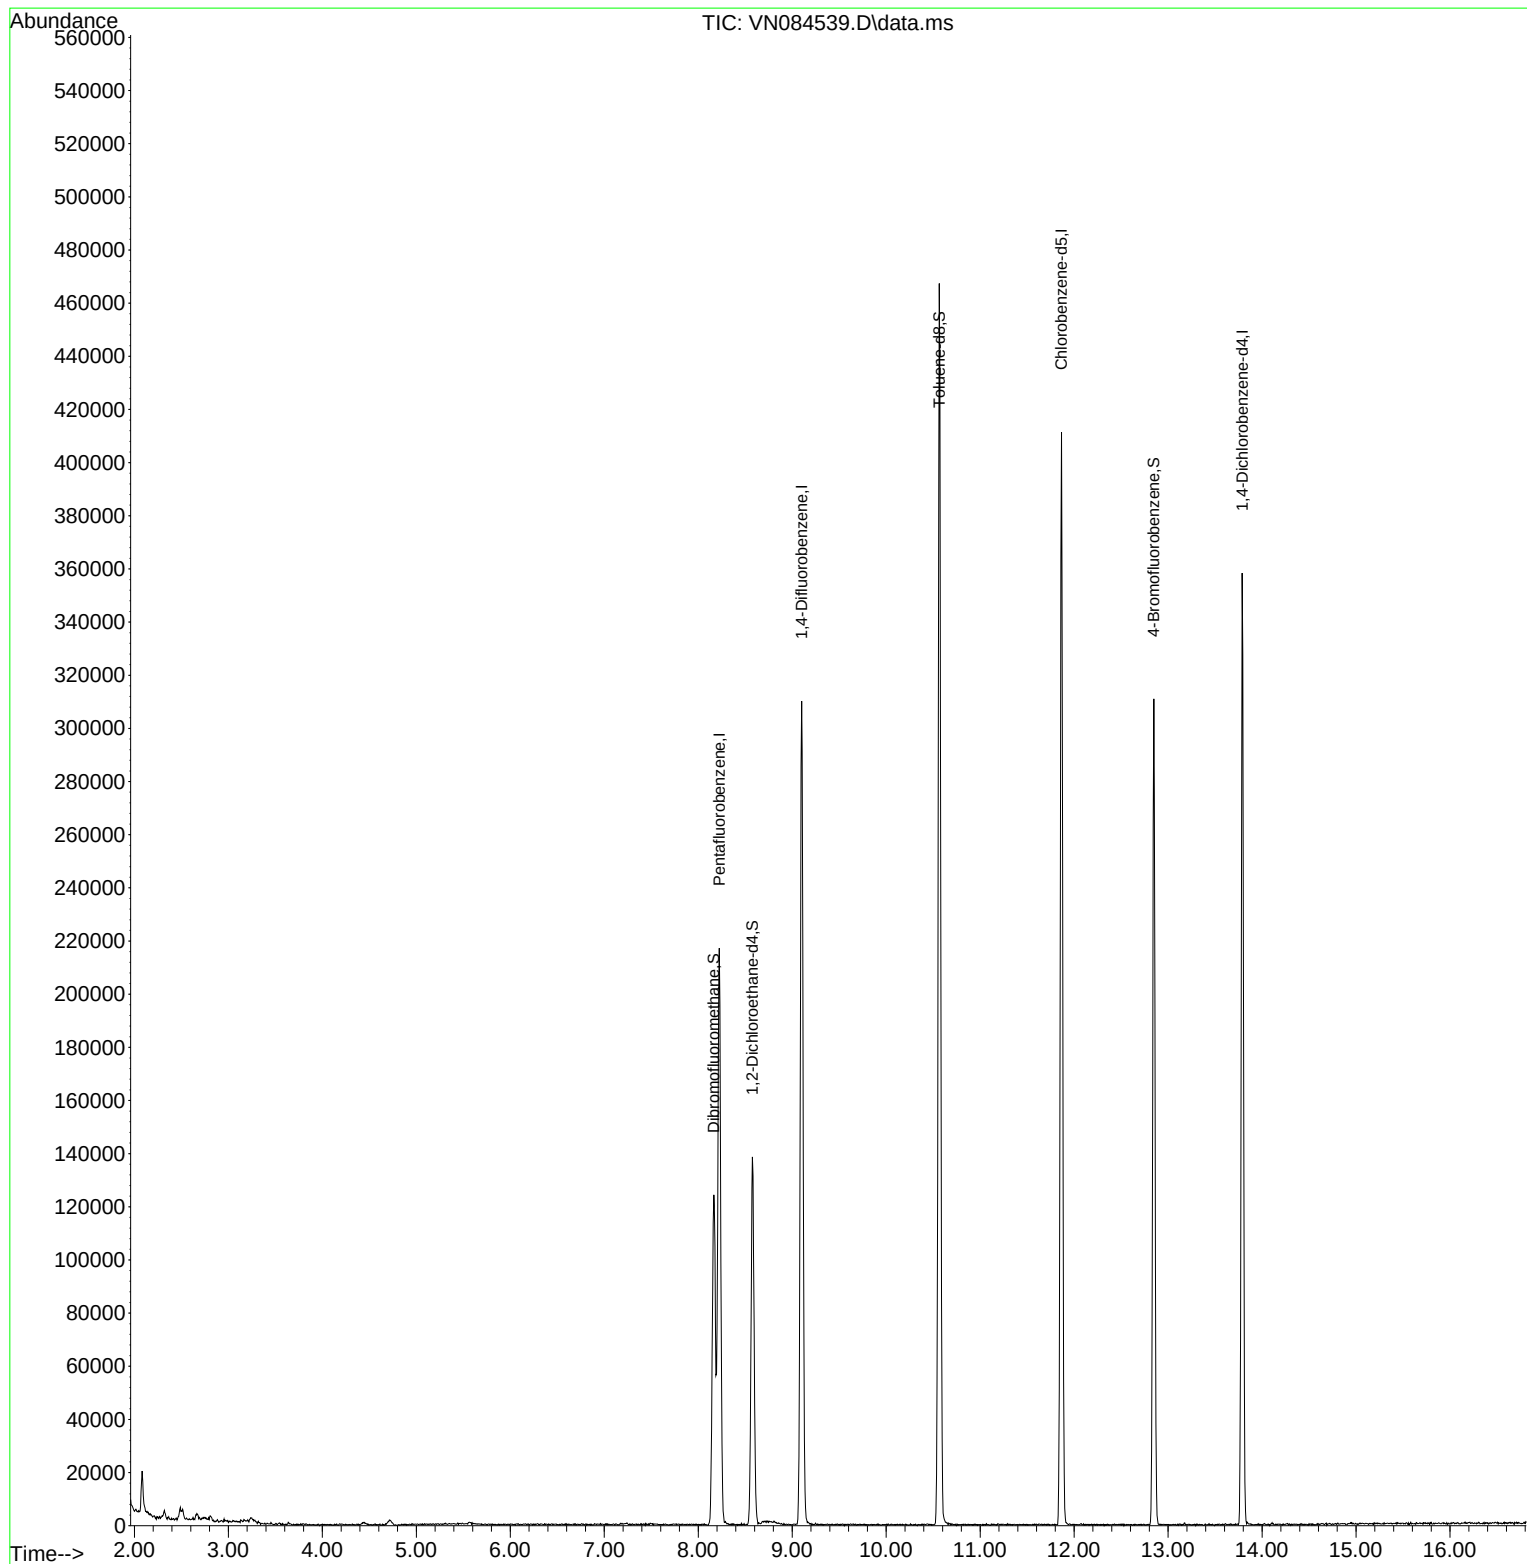


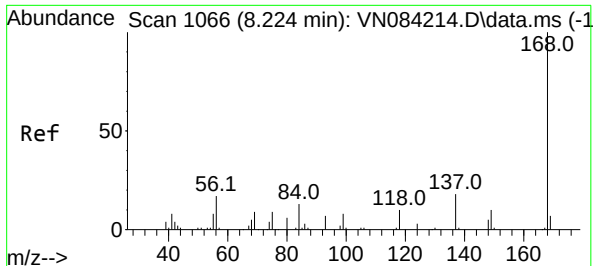

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN084539.D
Acq: 28 Oct 2024 15:05




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-190-GW-338-340


Tgt Ion:168 Resp: 150803
Ion Ratio Lower Upper
168 100
99 63.8 54.2 81.2

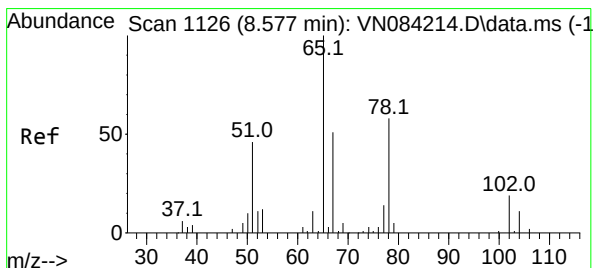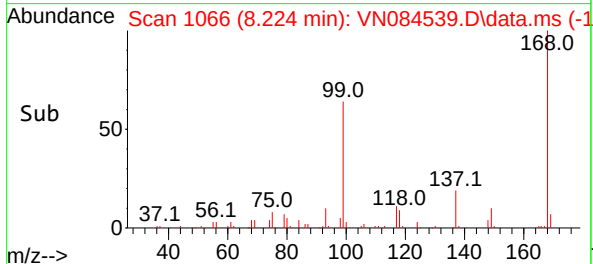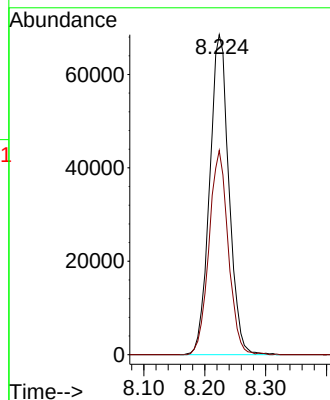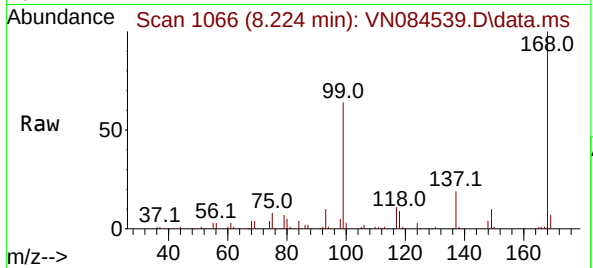

#33
1,2-Dichloroethane-d4
Concen: 50.863 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN084539.D
Acq: 28 Oct 2024 15:05

Tgt Ion: 65 Resp: 113726
Ion Ratio Lower Upper
65 100
67 52.3 0.0 102.0

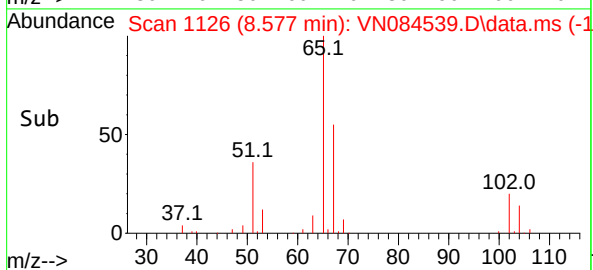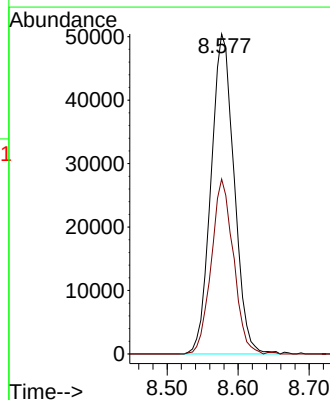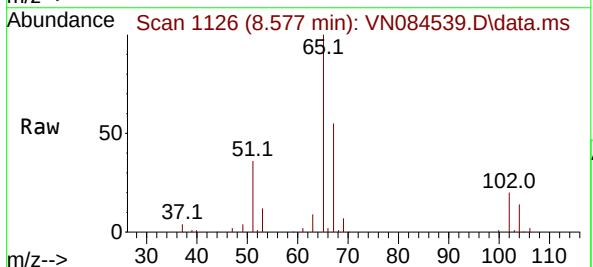

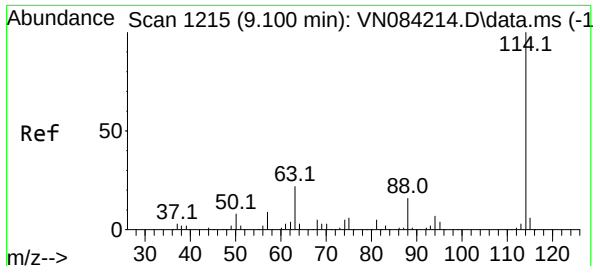

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN084539.D

Acq: 28 Oct 2024 15:05

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB-190-GW-338-340





Tgt Ion:114 Resp: 267490

Ion Ratio Lower Upper

114 100

63 21.8 0.0 43.8

88 16.1 0.0 31.6

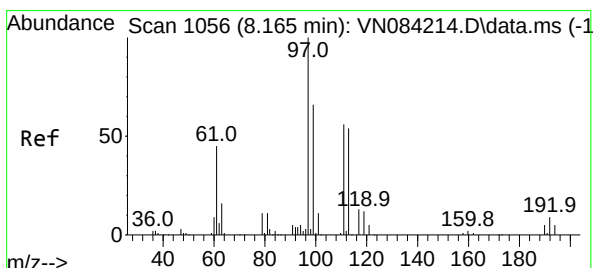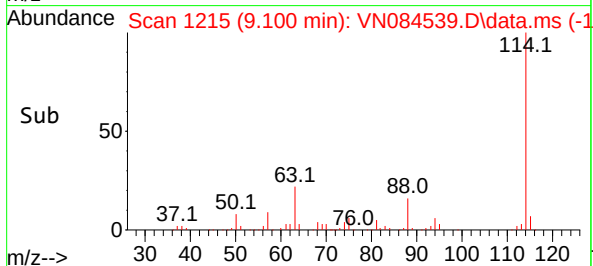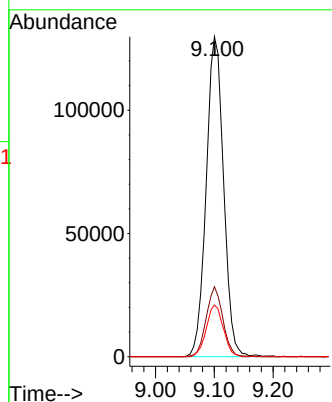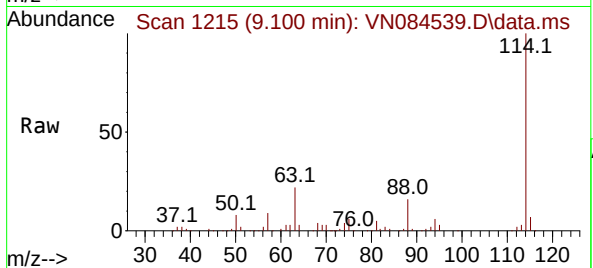

#35

Dibromofluoromethane

Concen: 51.878 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN084539.D

Acq: 28 Oct 2024 15:05




Tgt Ion:113 Resp: 91484


Ion Ratio Lower Upper

113 100

111 103.4 83.3 124.9

192 17.2 13.5 20.3


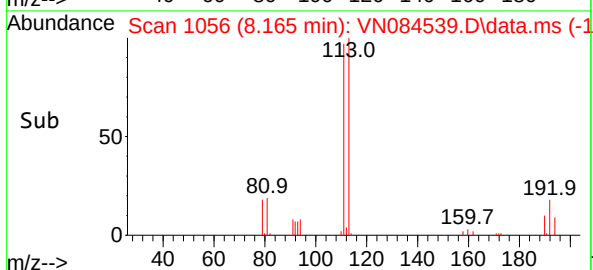
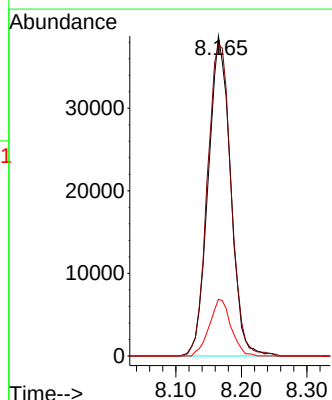
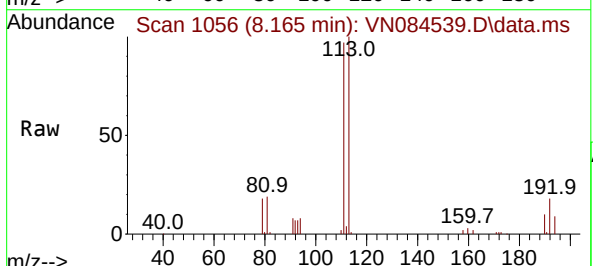


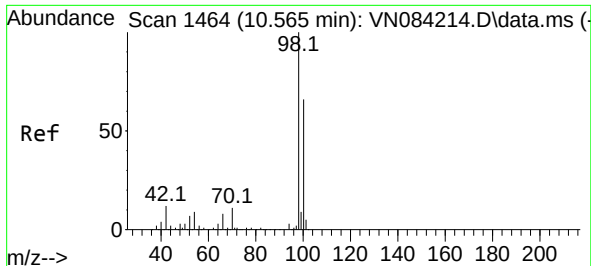

#50
Toluene-d8
Concen: 49.254 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN084539.D
Acq: 28 Oct 2024 15:05




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-190-GW-338-340


Tgt Ion: 98 Resp: 319558
Ion Ratio Lower Upper
98 100
100 64.4 52.7 79.1

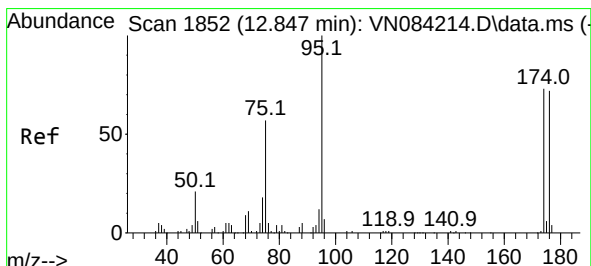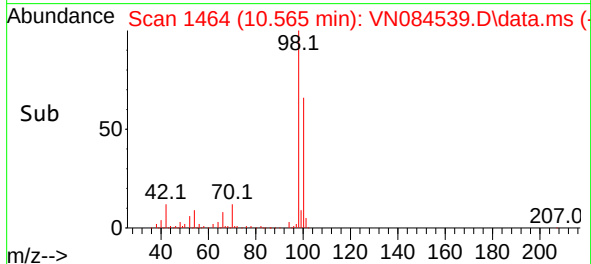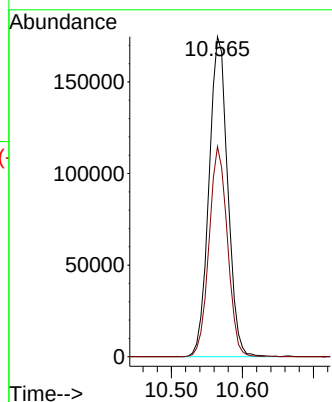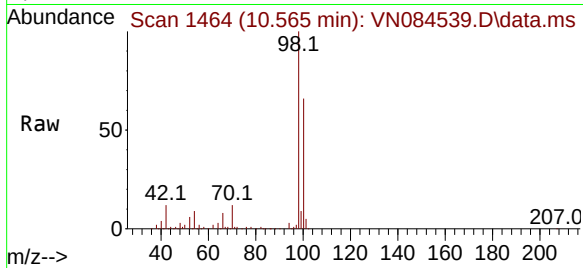

#62
4-Bromofluorobenzene
Concen: 45.384 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN084539.D
Acq: 28 Oct 2024 15:05

Tgt Ion: 95 Resp: 107270
Ion Ratio Lower Upper
95 100
174 76.0 0.0 145.2
176 71.6 0.0 140.0

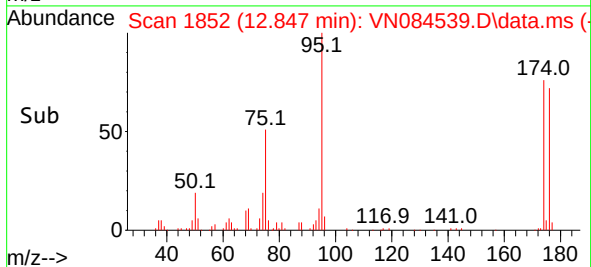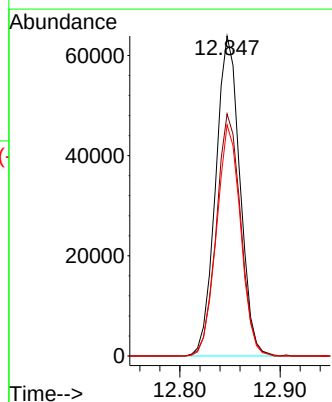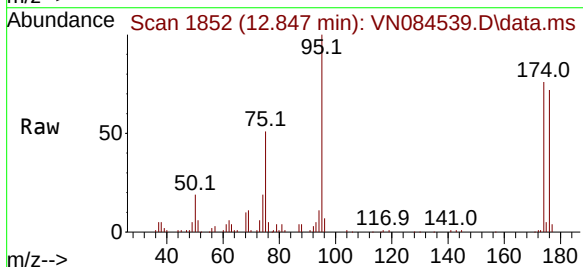

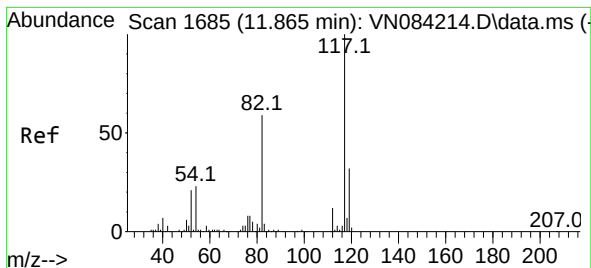

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN084539.D

Acq: 28 Oct 2024 15:05

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB-190-GW-338-340





Tgt Ion:117 Resp: 231312

Ion Ratio Lower Upper

117 100

82 59.0 47.2 70.8

119 31.0 25.4 38.0

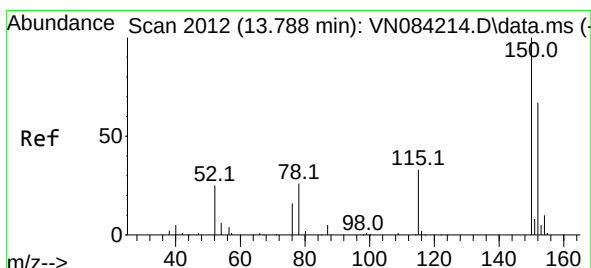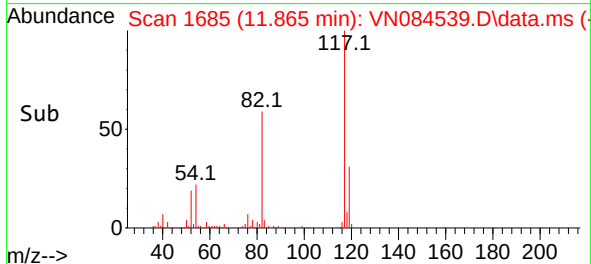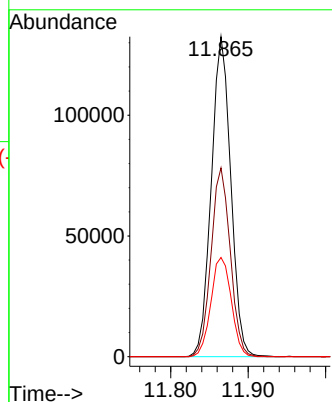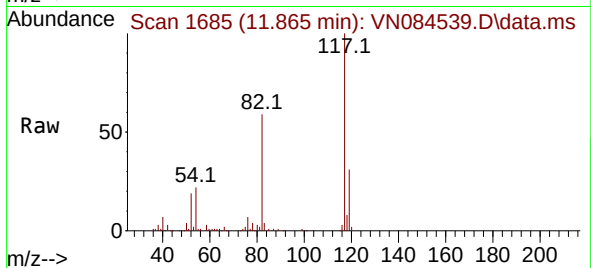

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 2012

Delta R.T. 0.000 min

Lab File: VN084539.D

Acq: 28 Oct 2024 15:05

Tgt Ion:152 Resp: 94475

Ion Ratio Lower Upper

152 100

115 61.2 31.3 93.9

150 158.7 0.0 349.8

