


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102824\
Data File : VN084528.D
Acq On : 28 Oct 2024 09:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

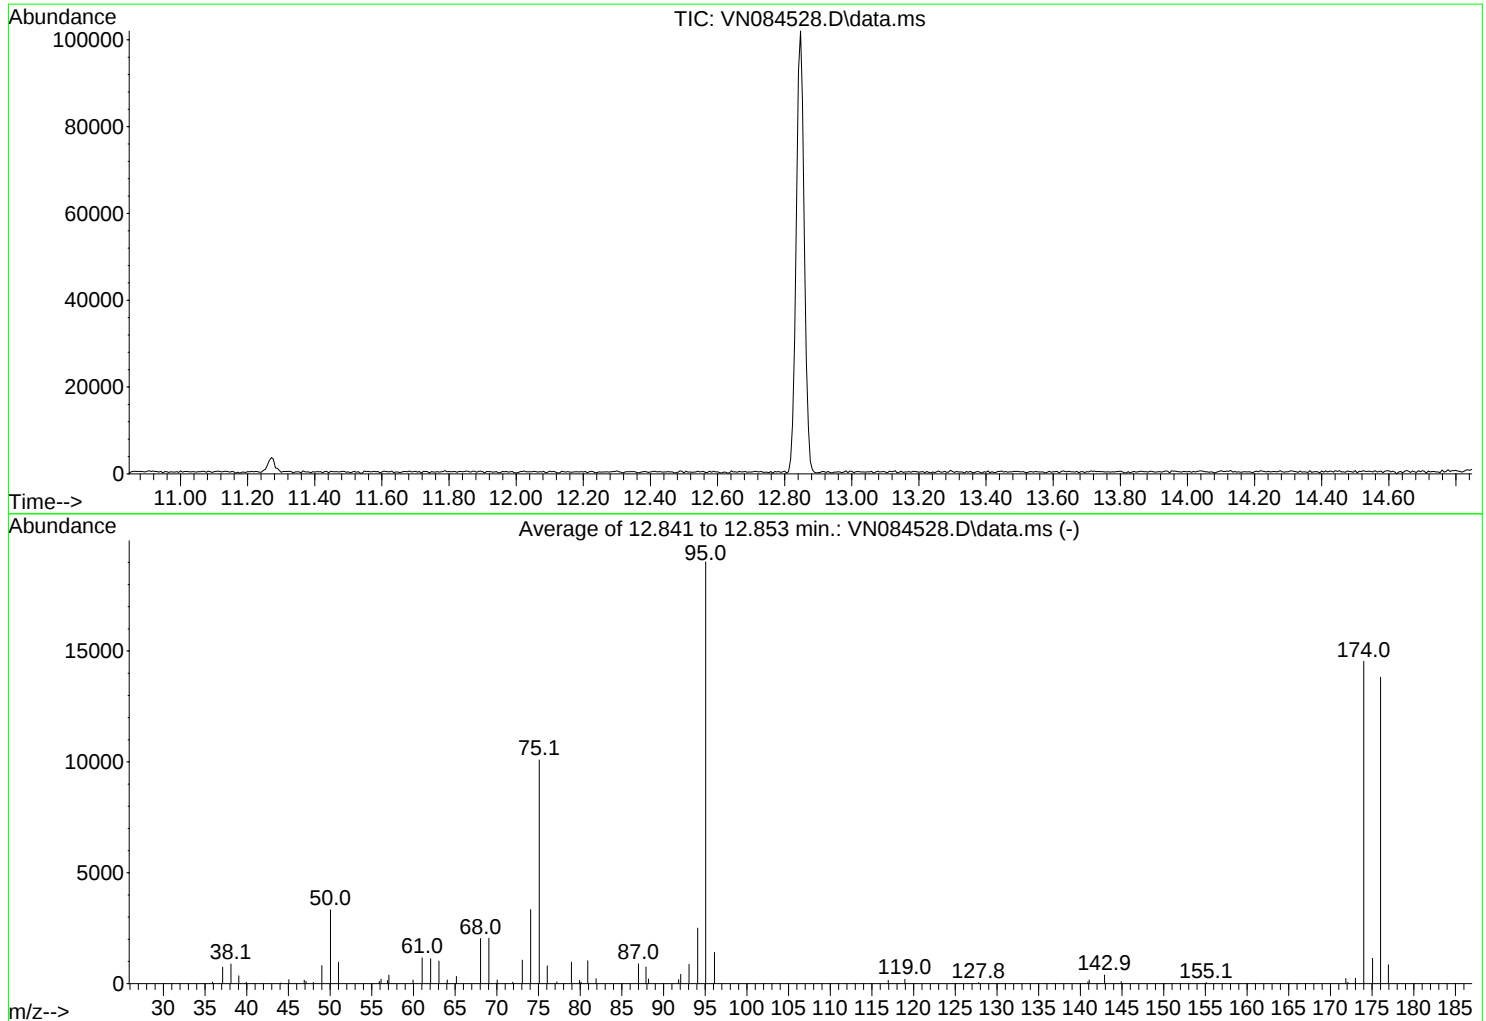

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	3329	PASS
75	95	30	60	53.0	10092	PASS
95	95	100	100	100.0	19024	PASS
96	95	5	9	7.4	1405	PASS
173	174	0.00	2	1.7	248	PASS
174	95	50	100	76.4	14532	PASS
175	174	5	9	7.9	1143	PASS
176	174	95	101	95.1	13817	PASS
177	176	5	9	6.2	850	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	75	50.05	3329	65.15	322	79.90	15
37.10	742	51.00	970	68.05	2038	80.10	7
38.10	886	55.90	98	69.05	2049	80.90	103
39.05	357	56.10	204	70.05	169	81.90	22
39.95	63	56.90	141	71.90	65	87.00	896
44.10	30	57.05	382	73.05	1062	87.90	750
45.05	178	59.95	169	74.05	3335	88.20	213
46.90	162	61.05	1160	75.10	10092	91.80	184
47.10	106	62.05	1123	76.05	799	92.05	419
48.00	59	63.05	1021	77.20	76	93.05	871
49.00	813	64.05	167	78.95	970	94.10	2501

Average of 12.841 to 12.853 min.: VN084528.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	19024	172.10	68				
96.10	1405	173.00	248				
116.95	152	174.00	14532				
118.95	198	175.05	1143				
127.80	52	176.00	13817				
140.90	77	176.95	850				
141.05	163						
142.90	389						
144.90	91						
155.10	52						
171.85	230						

Instrument :

MSVOA_N

ClientSampleId :

BFB