
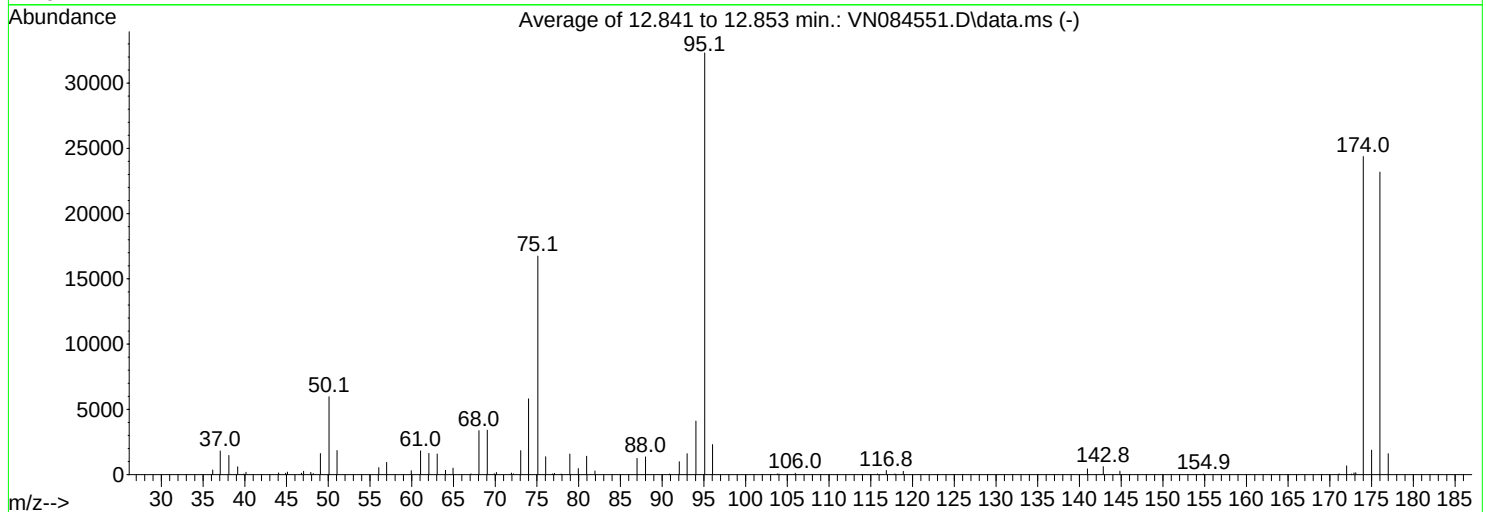


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102924\
Data File : VN084551.D
Acq On : 29 Oct 2024 09:05
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

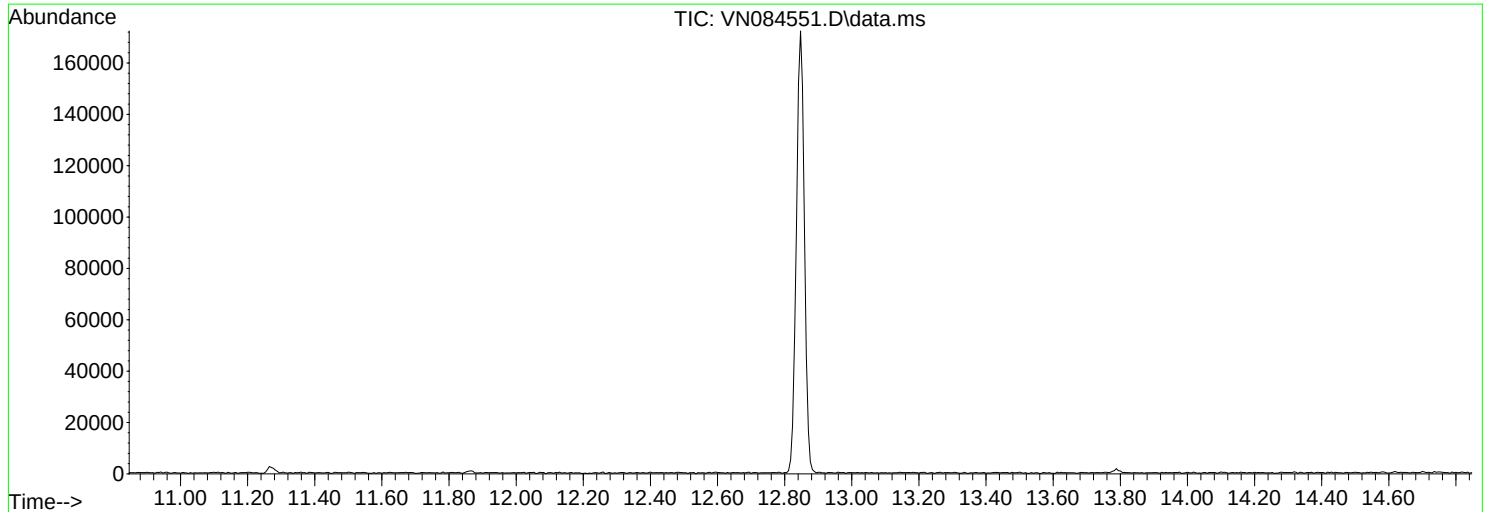

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5973	PASS
75	95	30	60	51.8	16746	PASS
95	95	100	100	100.0	32317	PASS
96	95	5	9	7.1	2302	PASS
173	174	0.00	2	0.6	144	PASS
174	95	50	100	75.4	24368	PASS
175	174	5	9	7.7	1882	PASS
176	174	95	101	95.1	23179	PASS
177	176	5	9	6.9	1610	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.15	351	47.90	173	64.05	330	75.10	1674
37.05	1813	48.20	82	64.95	508	76.05	1371
38.10	1467	49.05	1618	67.10	57	76.90	6
39.15	597	50.10	5973	68.05	3373	77.10	10
39.90	53	51.05	1853	69.05	3404	77.90	52
40.15	180	56.05	540	69.90	64	78.95	1586
44.05	131	57.00	951	70.15	173	79.95	472
44.90	111	59.95	311	71.95	128	80.95	1412
45.10	196	61.05	1830	72.20	63	81.95	288
46.80	106	62.05	1637	73.05	1842	87.00	1252
47.05	262	63.05	1576	74.00	5812	88.00	1359

Average of 12.841 to 12.853 min.: VN084551.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	51	117.90	63	174.00	24368		
92.05	988	118.90	253	175.00	1882		
93.00	1605	140.95	447	176.00	23179		
94.05	4112	142.85	615	177.00	1610		
95.10	32317	144.85	274				
96.05	2302	154.90	52				
103.80	60	171.10	56				
104.00	54	172.00	675				
105.95	106	172.60	55				
115.80	64	172.90	136				
116.85	322	173.10	144				

Instrument :

MSVOA_N

ClientSampleId :

BFB