
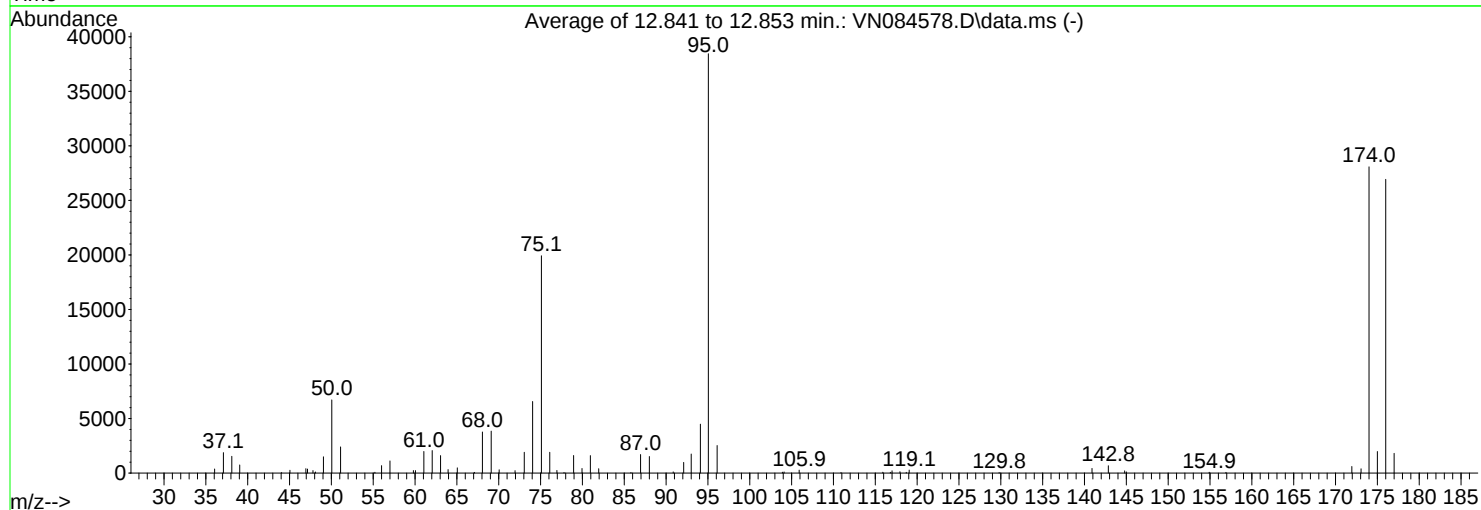


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103024\
Data File : VN084578.D
Acq On : 30 Oct 2024 19:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

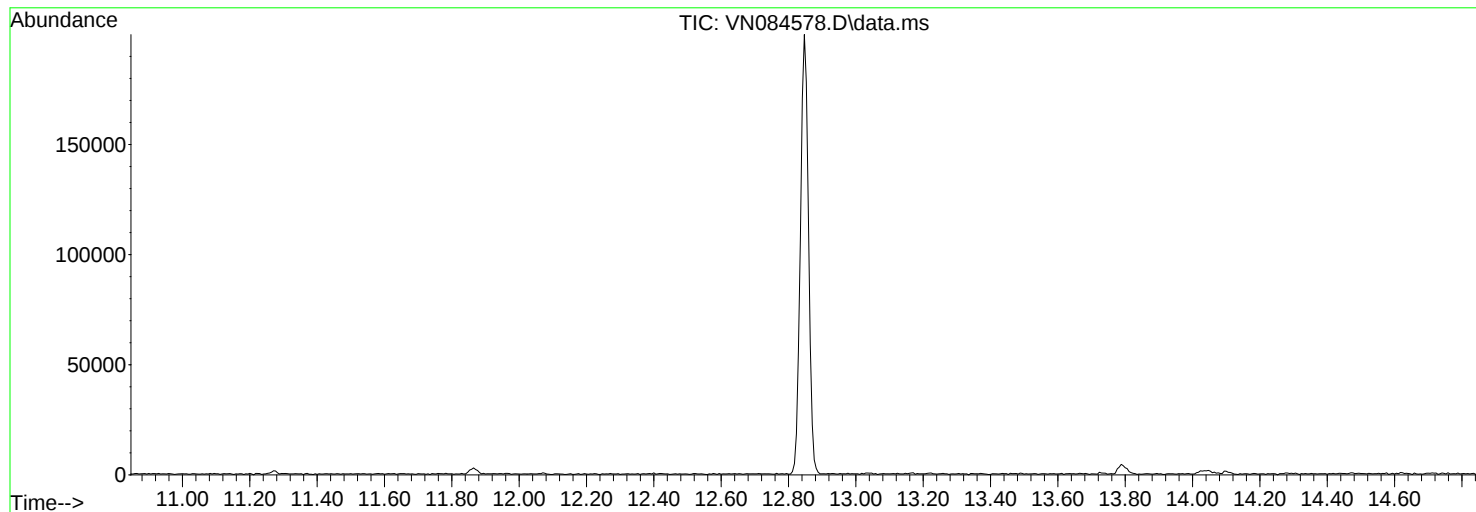

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6709	PASS
75	95	30	60	51.8	19925	PASS
95	95	100	100	100.0	38448	PASS
96	95	5	9	6.6	2529	PASS
173	174	0.00	2	1.4	391	PASS
174	95	50	100	73.0	28080	PASS
175	174	5	9	7.0	1977	PASS
176	174	95	101	95.9	26931	PASS
177	176	5	9	6.7	1809	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	377	50.05	6709	65.05	482	77.80	54
37.10	1875	51.10	2401	67.10	65	78.95	1613
38.10	1535	55.20	76	68.05	3766	79.95	425
39.05	747	56.00	683	69.10	3849	80.95	1603
44.05	47	57.00	1113	70.05	304	81.95	401
45.05	259	59.80	233	71.95	224	85.80	57
46.95	404	60.05	229	73.05	1907	86.95	1699
47.15	371	61.05	1981	74.05	6562	88.00	1520
47.80	233	62.05	2064	75.10	19925	90.85	112
48.10	100	63.05	1601	76.10	1906	92.10	976
49.05	1493	63.95	323	76.95	245	93.00	1749

Average of 12.841 to 12.853 min.: VN084578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	4485	118.70	65	174.00	28080		
95.05	38448	119.05	276	175.00	1977		
96.10	2529	129.80	50	176.00	26931		
103.90	84	140.90	429	177.00	1809		
104.10	105	142.85	674				
105.90	275	144.80	205				
110.90	51	145.00	108				
115.90	78	154.90	74				
116.80	70	156.90	68				
117.00	212	171.95	605				
117.95	128	173.05	391				