
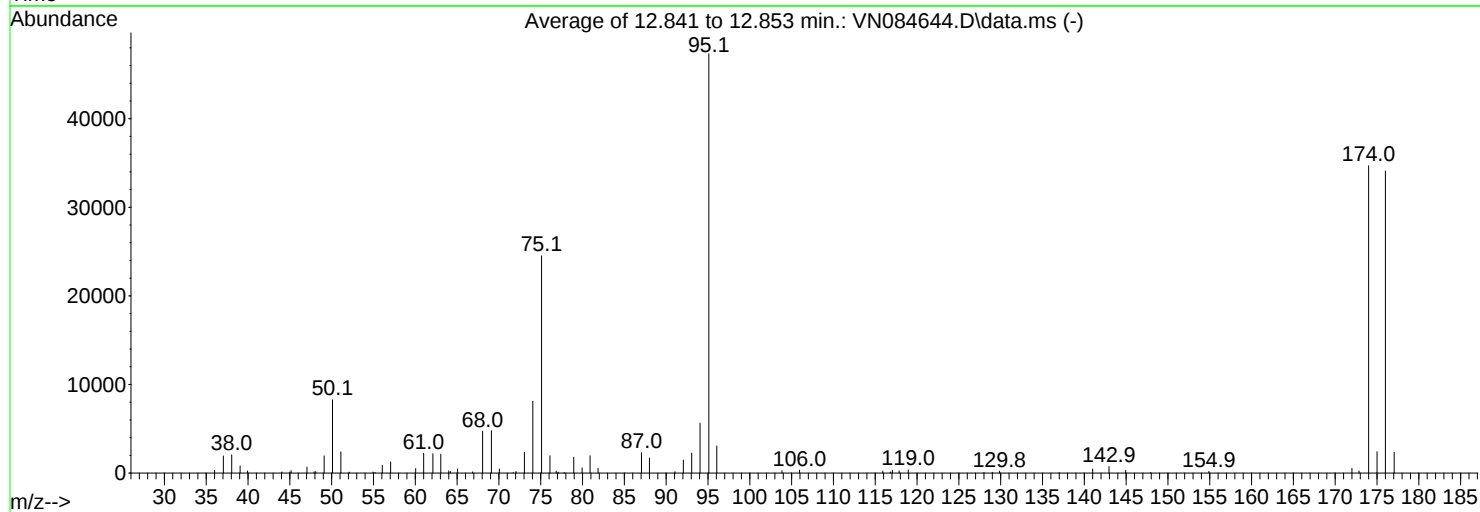


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110424\
Data File : VN084644.D
Acq On : 04 Nov 2024 08:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

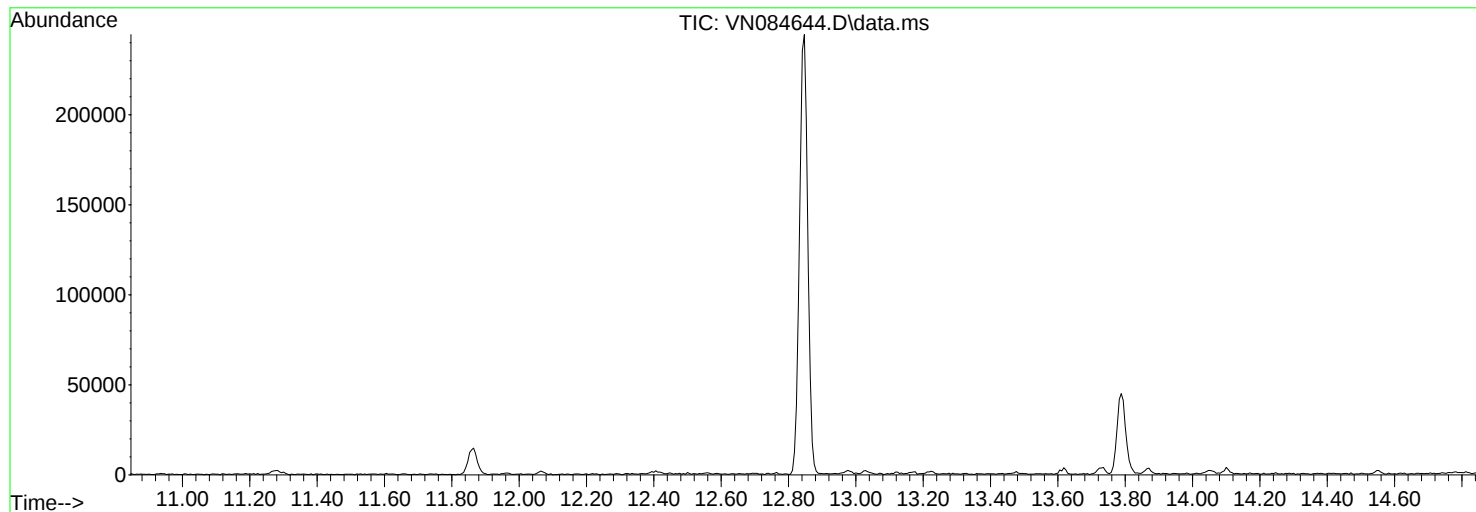

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	8272	PASS
75	95	30	60	51.8	24517	PASS
95	95	100	100	100.0	47333	PASS
96	95	5	9	6.5	3055	PASS
173	174	0.00	2	0.7	242	PASS
174	95	50	100	73.3	34701	PASS
175	174	5	9	7.0	2415	PASS
176	174	95	101	98.3	34101	PASS
177	176	5	9	6.9	2355	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	323	49.10	1944	63.05	2138	74.05	8105
37.05	1940	50.10	8272	64.00	248	75.10	24517
38.05	2052	51.10	2396	64.20	178	76.10	1963
39.05	804	52.10	117	65.05	463	76.85	231
39.95	239	54.95	125	66.85	137	77.10	106
44.05	137	55.20	57	68.05	4730	77.80	79
45.00	124	56.05	860	69.10	4780	78.95	1793
45.15	281	57.05	1262	70.05	452	79.95	584
47.05	678	60.05	505	71.70	57	80.90	1956
47.90	144	61.00	2241	72.05	192	81.85	549
48.10	172	62.10	2185	73.05	2344	87.05	2305

Average of 12.841 to 12.853 min.: VN084644.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.00	1699	117.05	324	154.90	195		
91.05	159	117.85	251	172.00	543		
92.05	1471	118.95	351	172.85	242		
93.05	2257	128.00	59	174.00	34701		
94.05	5638	129.00	88	175.00	2415		
95.10	47333	129.85	222	176.00	34101		
96.05	3055	137.00	51	177.05	2355		
103.85	276	141.00	467				
105.95	337	142.95	743				
115.90	220	144.95	322				
116.80	138	147.90	57				