
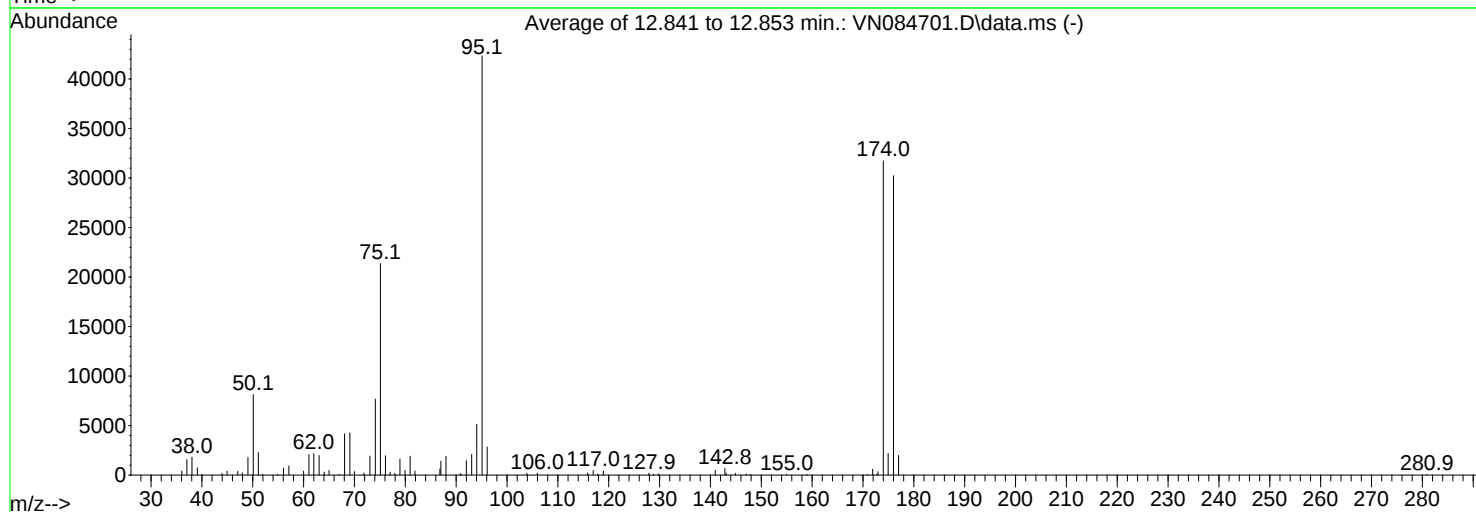


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN110624\  
Data File : VN084701.D  
Acq On : 06 Nov 2024 09:44  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N103024W.M  
Title : SW846 8260  
Last Update : Thu Oct 31 18:45:38 2024

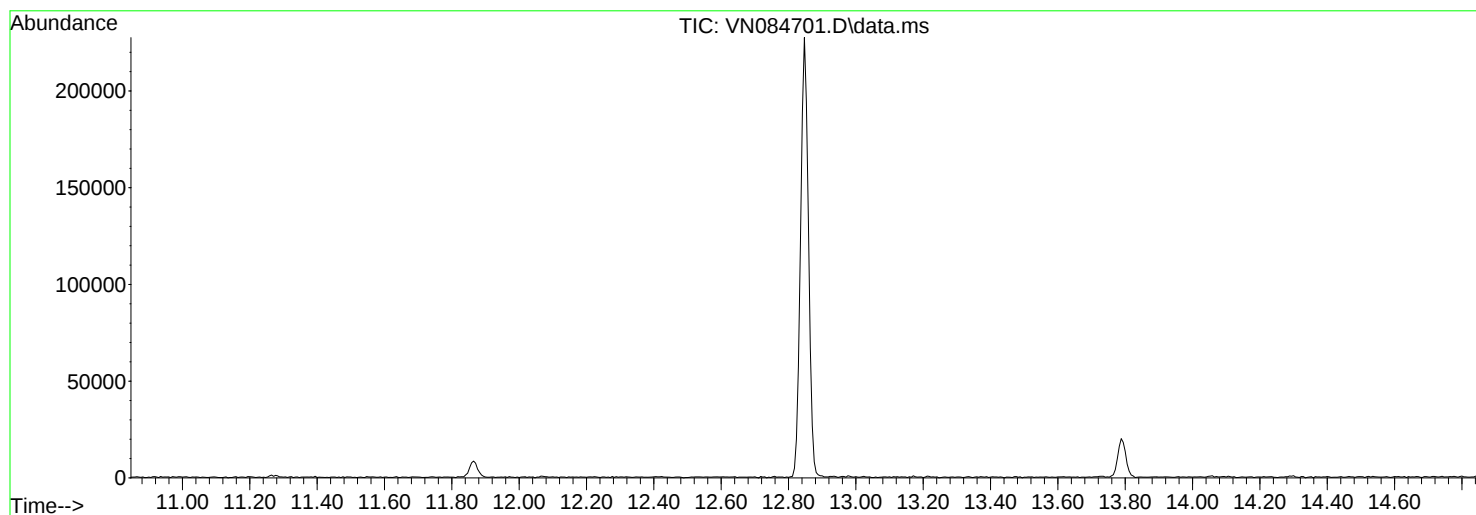

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.2         | 8130       | PASS                |
| 75             | 95              | 30              | 60              | 50.5         | 21371      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 42349      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 2839       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 345        | PASS                |
| 174            | 95              | 50              | 100             | 74.9         | 31739      | PASS                |
| 175            | 174             | 5               | 9               | 6.9          | 2186       | PASS                |
| 176            | 174             | 95              | 101             | 95.3         | 30237      | PASS                |
| 177            | 176             | 5               | 9               | 6.6          | 1988       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.05 | 407    | 51.10 | 2276   | 67.00 | 53     | 78.95 | 1625   |
| 37.05 | 1569   | 51.90 | 72     | 68.05 | 4167   | 79.95 | 476    |
| 38.05 | 1807   | 54.90 | 64     | 69.10 | 4261   | 80.95 | 1908   |
| 39.10 | 742    | 56.05 | 704    | 70.00 | 349    | 81.90 | 414    |
| 40.00 | 53     | 57.10 | 939    | 71.85 | 212    | 86.80 | 603    |
| 43.95 | 163    | 60.00 | 399    | 73.05 | 1926   | 87.00 | 1410   |
| 44.95 | 397    | 61.05 | 2074   | 74.10 | 7673   | 88.00 | 1888   |
| 47.05 | 386    | 62.00 | 2157   | 75.10 | 21371  | 90.80 | 153    |
| 47.95 | 234    | 63.05 | 1981   | 76.10 | 1955   | 91.00 | 56     |
| 49.05 | 1791   | 64.05 | 309    | 77.00 | 300    | 92.00 | 1450   |
| 50.10 | 8130   | 65.00 | 471    | 77.95 | 184    | 93.05 | 2090   |

Average of 12.841 to 12.853 min.: VN084701.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 94.05  | 5141   | 129.75 | 125    | 172.70 | 96     |     |        |
| 95.10  | 42349  | 140.95 | 499    | 172.95 | 345    |     |        |
| 96.10  | 2839   | 142.85 | 661    | 174.00 | 31739  |     |        |
| 103.90 | 199    | 143.10 | 195    | 174.95 | 2186   |     |        |
| 105.95 | 194    | 144.90 | 188    | 176.00 | 30237  |     |        |
| 115.85 | 211    | 147.05 | 111    | 177.00 | 1988   |     |        |
| 116.95 | 457    | 147.80 | 72     | 280.90 | 51     |     |        |
| 117.80 | 104    | 155.00 | 81     |        |        |     |        |
| 118.95 | 405    | 159.00 | 54     |        |        |     |        |
| 127.90 | 198    | 170.90 | 70     |        |        |     |        |
| 128.80 | 72     | 171.90 | 590    |        |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB