

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110724\
 Data File : VN084725.D
 Acq On : 07 Nov 2024 16:45
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M

Title : SW846 8260

Signal : TIC: VN084725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.289	51	57	66	rBV2	21556	45877	4.56%	0.757%
2	2.912	138	163	170	rBV10	19922	101738	10.11%	1.680%
3	8.165	1044	1056	1060	rBV	141413	335256	33.33%	5.535%
4	8.218	1060	1065	1075	rVB	252186	564945	56.16%	9.328%
5	8.577	1116	1126	1136	rBV	154421	342553	34.05%	5.656%
6	8.765	1147	1158	1160	rBV3	3902	10502	1.04%	0.173%
7	9.100	1203	1215	1229	rBV	367140	760332	75.58%	12.554%
8	10.565	1455	1464	1479	rBV	556191	1005972	100.00%	16.609%
9	11.865	1677	1685	1693	rBV	513656	911518	90.61%	15.050%
10	11.959	1696	1701	1706	rVV	14056	23227	2.31%	0.383%
11	12.847	1845	1852	1859	rVB	425404	709362	70.52%	11.712%
12	13.035	1878	1884	1889	rVB	20654	34067	3.39%	0.562%
13	13.170	1903	1907	1912	rVB4	9284	11496	1.14%	0.190%
14	13.612	1976	1982	1984	rBV6	6202	10809	1.07%	0.178%
15	13.788	2004	2012	2026	rBV	532174	917290	91.18%	15.145%
16	13.953	2034	2040	2043	rBV6	7878	16007	1.59%	0.264%
17	14.000	2043	2048	2049	rBV3	20509	29755	2.96%	0.491%
18	14.329	2095	2104	2110	rBV	21519	38376	3.81%	0.634%
19	14.564	2139	2144	2151	rVB10	7976	16890	1.68%	0.279%
20	14.653	2153	2159	2163	rBV3	9898	18090	1.80%	0.299%
21	14.688	2163	2165	2169	rVV3	9400	12951	1.29%	0.214%
22	14.929	2201	2206	2217	rVB6	9906	26465	2.63%	0.437%
23	15.053	2217	2227	2231	rBV8	13295	37388	3.72%	0.617%
24	15.441	2288	2293	2298	rVB7	6924	14326	1.42%	0.237%
25	15.635	2321	2326	2334	rVB2	13095	27152	2.70%	0.448%
26	15.947	2374	2379	2383	rVB6	5450	10629	1.06%	0.175%
27	16.782	2514	2521	2522	rBV3	13302	23664	2.35%	0.391%




Sum of corrected areas: 6056637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110724\
Data File : VN084725.D
Acq On : 07 Nov 2024 16:45
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

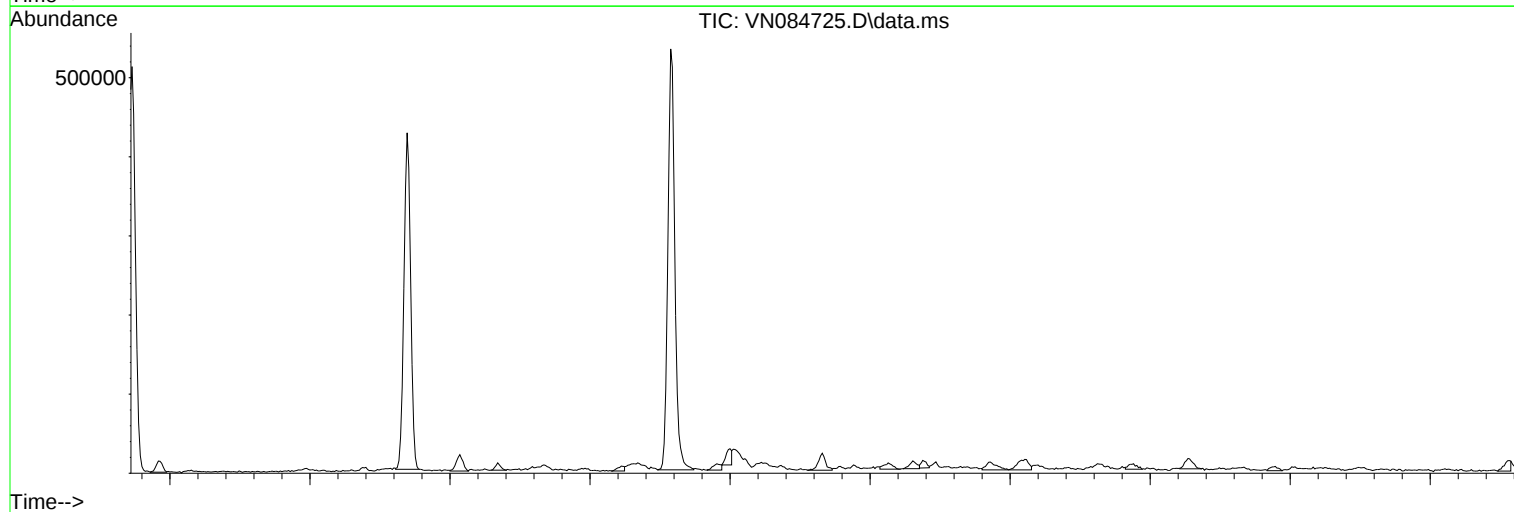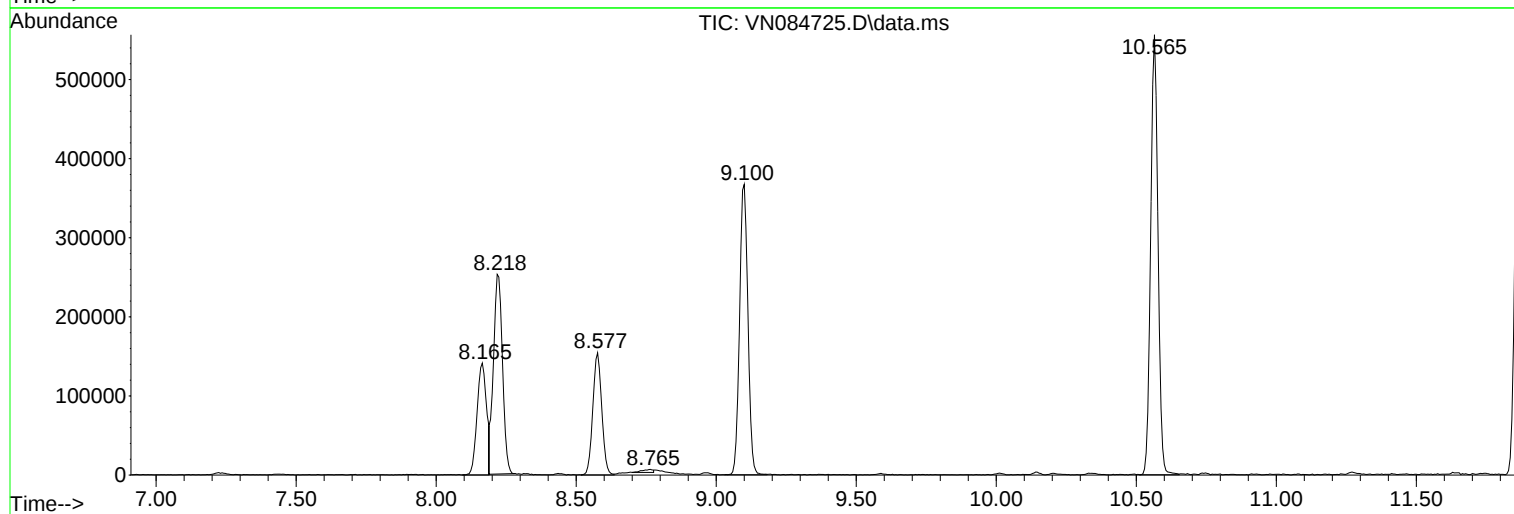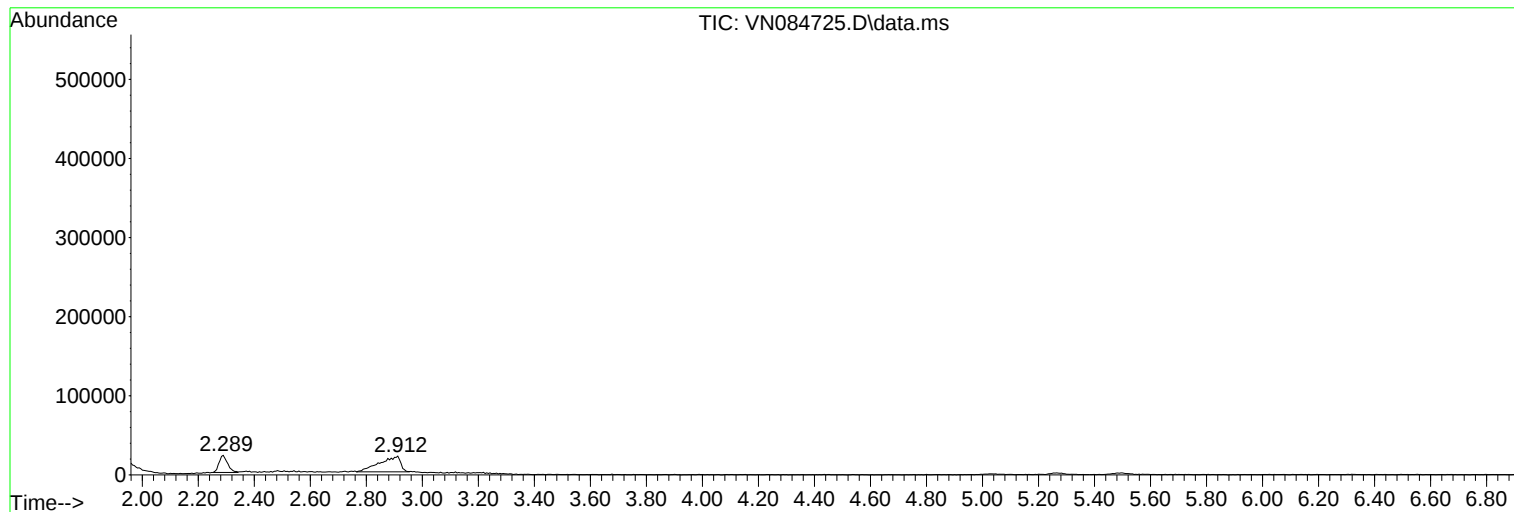

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110724\
Data File : VN084725.D
Acq On : 07 Nov 2024 16:45
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110724\
Data File : VN084725.D
Acq On : 07 Nov 2024 16:45
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------