
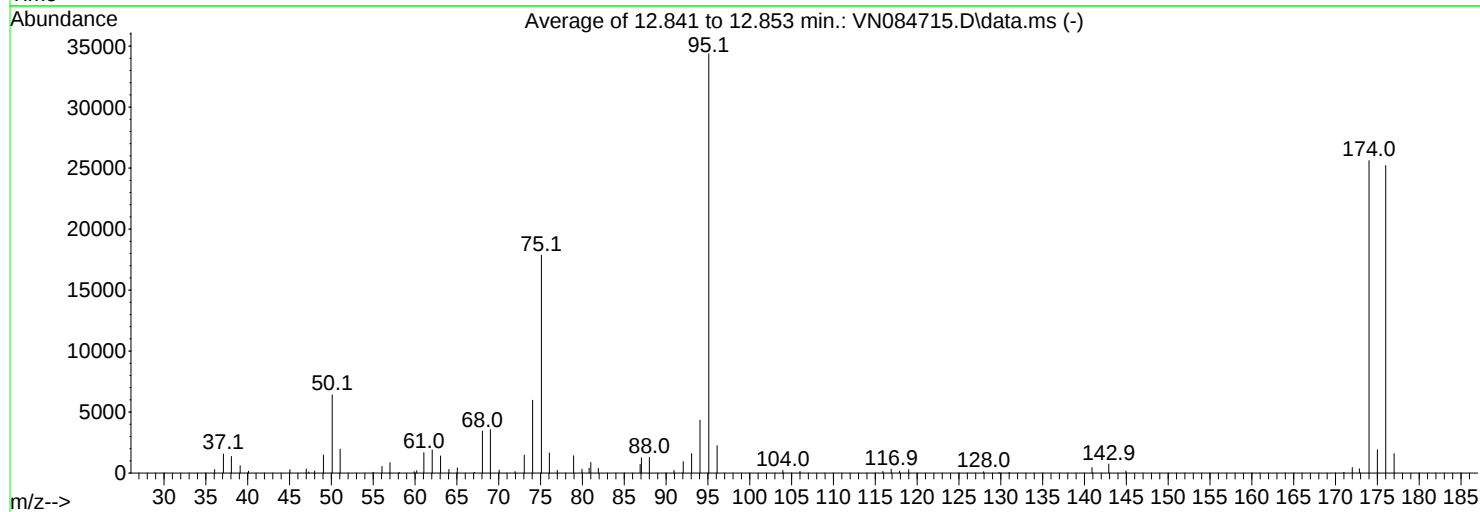


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110724\
Data File : VN084715.D
Acq On : 07 Nov 2024 10:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

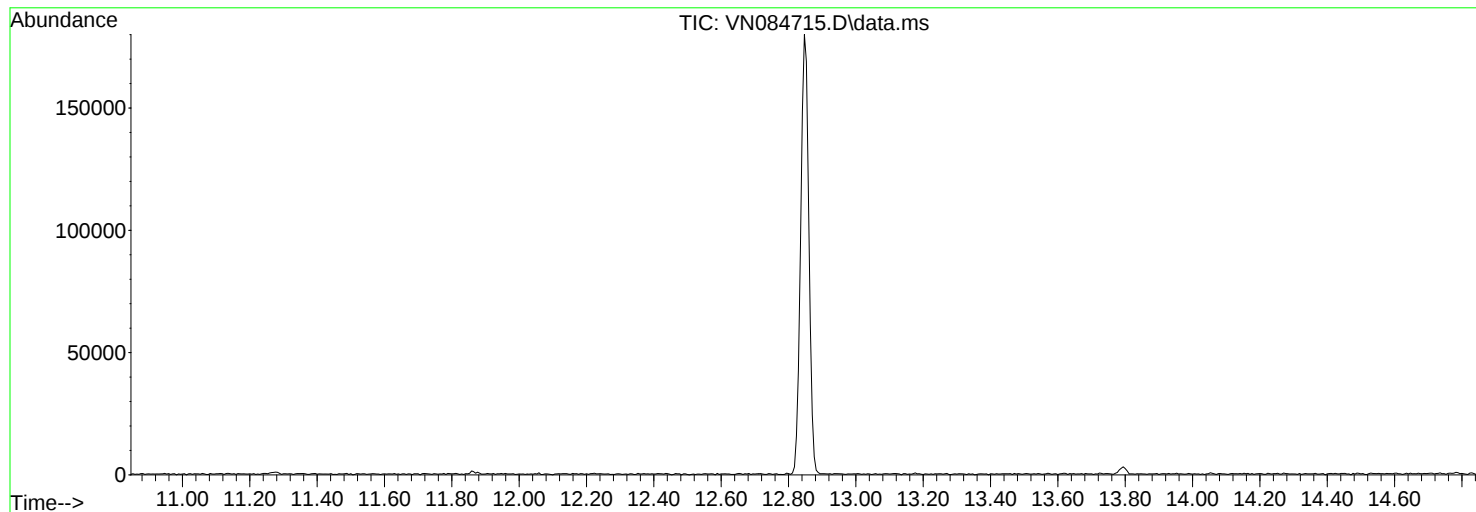

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	6416	PASS
75	95	30	60	51.9	17856	PASS
95	95	100	100	100.0	34376	PASS
96	95	5	9	6.5	2250	PASS
173	174	0.00	2	1.4	356	PASS
174	95	50	100	74.5	25611	PASS
175	174	5	9	7.5	1919	PASS
176	174	95	101	98.4	25213	PASS
177	176	5	9	6.3	1601	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	292	51.05	1958	65.05	424	78.95	1422
37.10	1572	55.00	68	67.10	60	79.95	318
38.05	1364	56.05	552	68.05	3439	80.80	400
39.10	609	57.00	851	69.00	3566	81.00	877
40.10	158	58.10	56	70.05	249	81.90	381
45.05	290	59.90	120	71.95	131	86.90	711
47.00	336	60.20	207	73.05	1471	87.05	1254
47.30	101	61.05	1677	74.05	5975	88.00	1290
48.00	183	62.05	1896	75.10	17856	90.95	226
49.05	1475	63.05	1405	76.05	1654	92.05	939
50.10	6416	64.05	302	77.00	224	93.05	1602

Average of 12.841 to 12.853 min.: VN084715.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	4340	131.00	53				
95.10	34376	140.90	457				
96.10	2250	142.90	729				
103.95	233	144.95	164				
106.00	143	171.00	65				
115.90	137	172.00	457				
116.90	327	172.85	356				
117.90	159	174.00	25611				
119.00	287	175.00	1919				
127.95	122	176.00	25213				
129.80	60	177.00	1601				

Instrument :

MSVOA_N

ClientSampleId :

BFB