

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120622\
 Data File : VN075578.D
 Acq On : 06 Dec 2022 12:13
 Operator : JC\MD
 Sample : VN1206MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1206MBL01

Quant Time: Dec 07 00:11:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	129964	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	217572	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	188987	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	78499	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	38003	54.475	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.940%
35) Dibromofluoromethane	8.171	113	46982	54.969	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.940%
50) Toluene-d8	10.571	98	93681	48.665	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.340%
62) 4-Bromofluorobenzene	12.853	95	63138	44.436	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120622\
Data File : VN075578.D
Acq On : 06 Dec 2022 12:13
Operator : JC\MD
Sample : VN1206MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1206MBL01

Quant Time: Dec 07 00:11:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




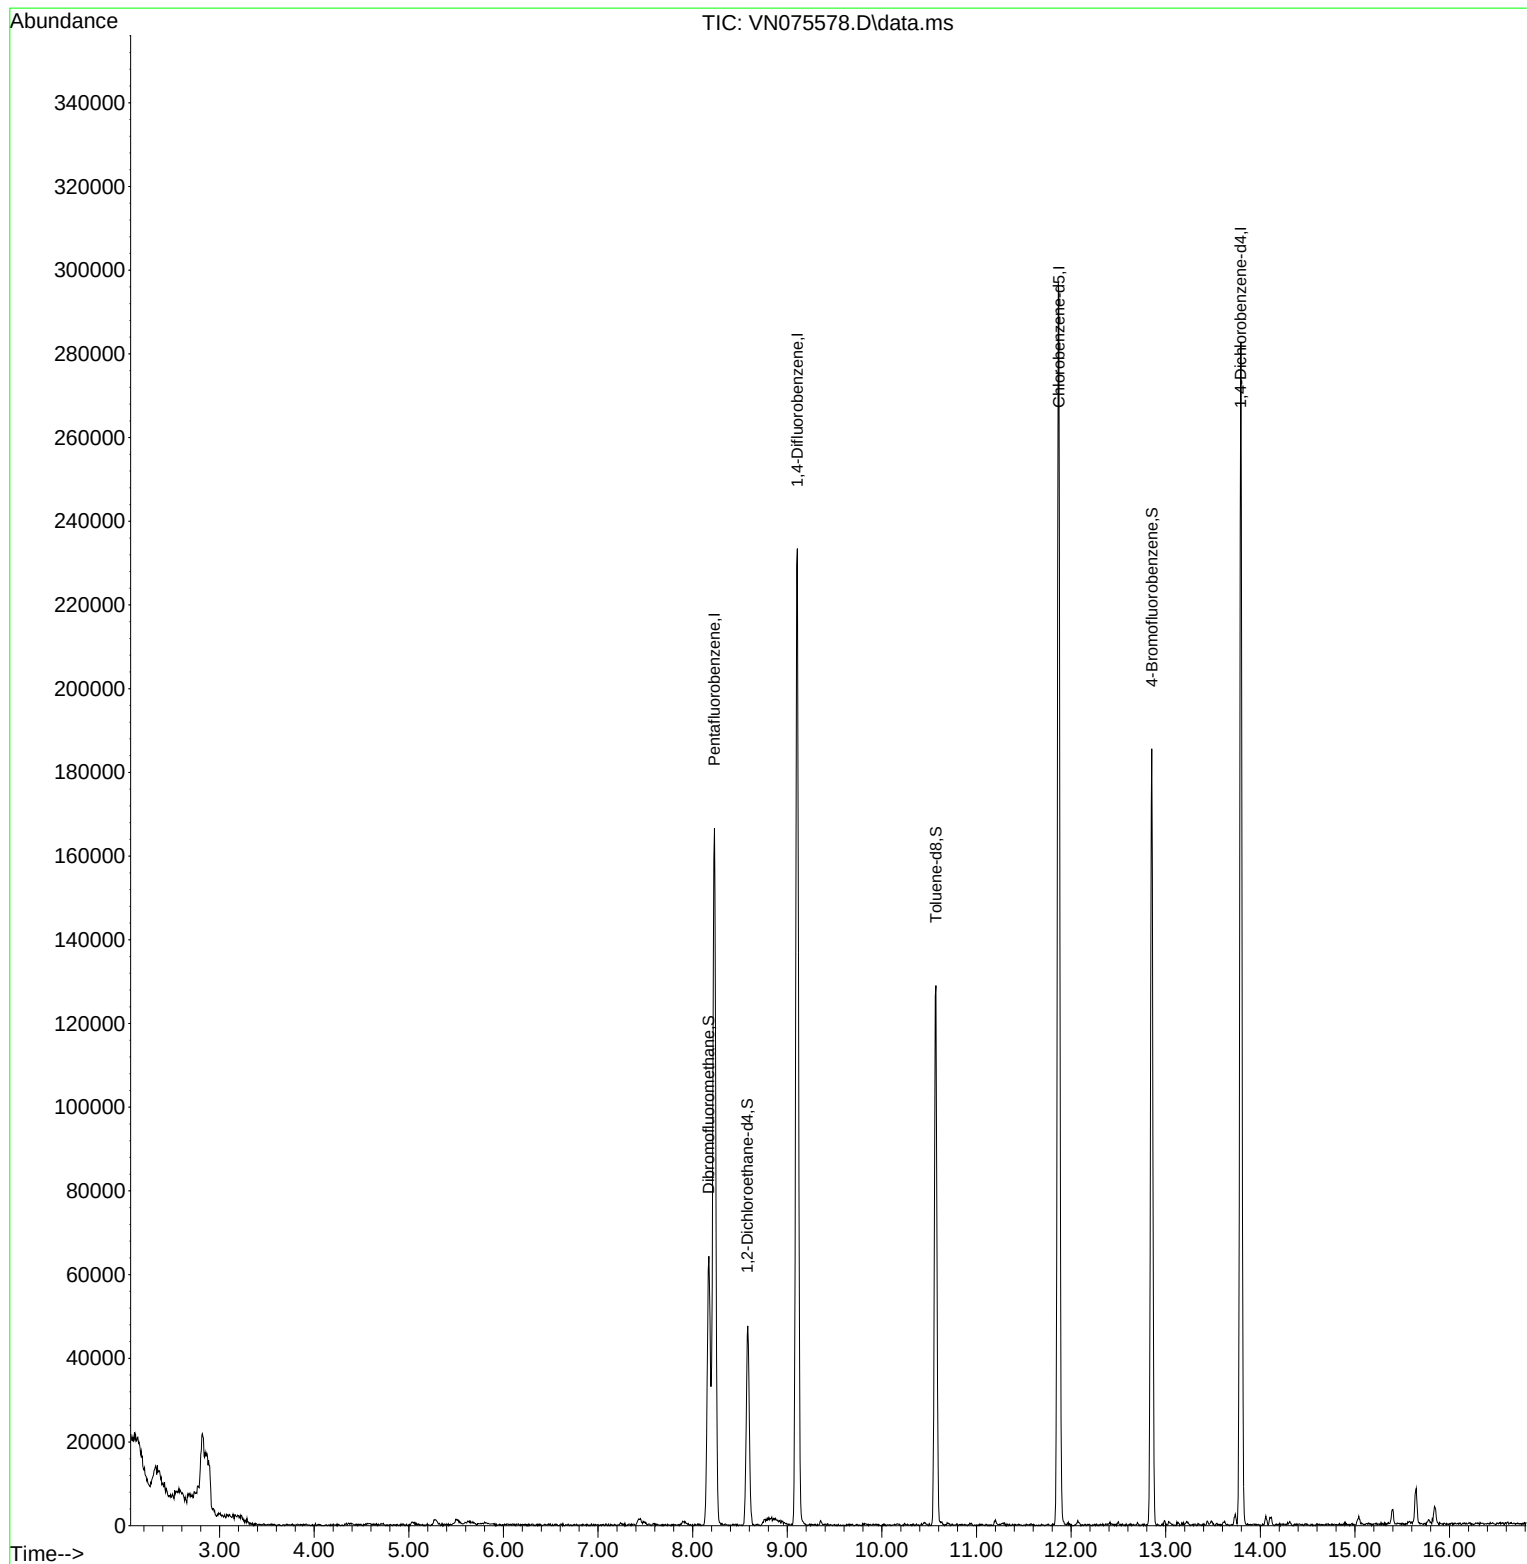


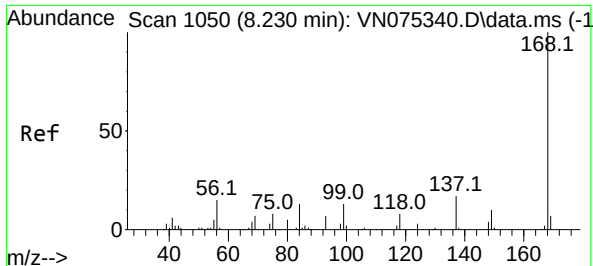

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1109
Delta R.T. -0.000 min
Lab File: VN075578.D
Acq: 06 Dec 2022 12:13




Instrument :
MSVOA_N
ClientSampleId :
VN1206MBL01


Tgt Ion:168 Resp: 129964
Ion Ratio Lower Upper
168 100
99 55.7 51.6 77.4

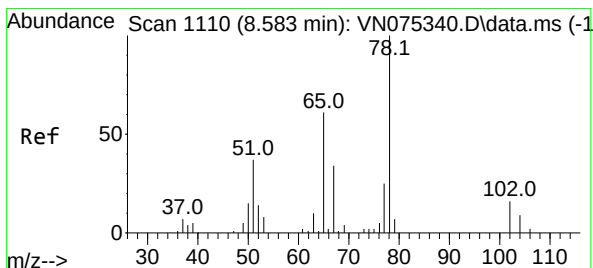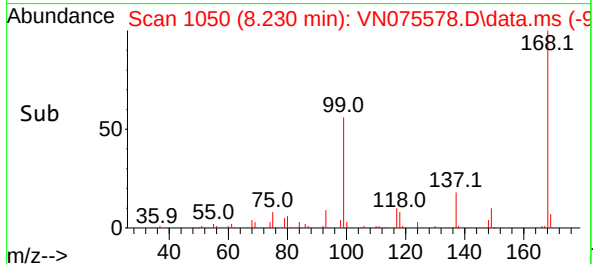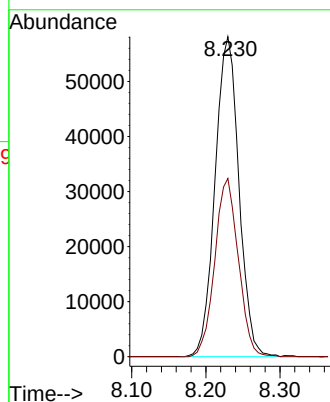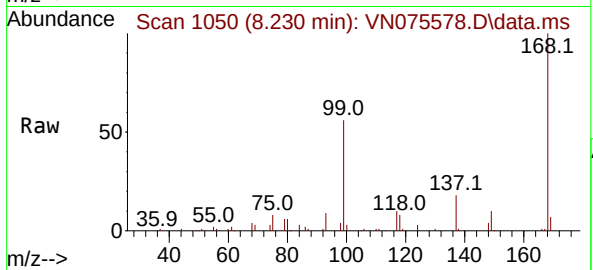

#33
1,2-Dichloroethane-d4
Concen: 54.475 ug/l
RT: 8.577 min Scan# 1109
Delta R.T. -0.006 min
Lab File: VN075578.D
Acq: 06 Dec 2022 12:13

Tgt Ion: 65 Resp: 38003
Ion Ratio Lower Upper
65 100
67 52.4 0.0 102.0

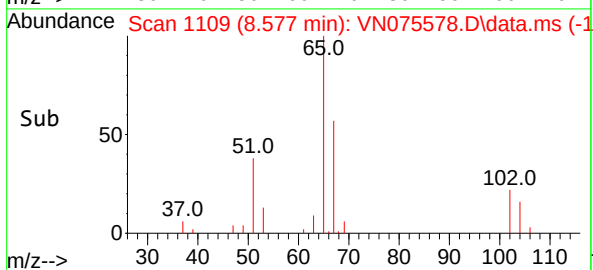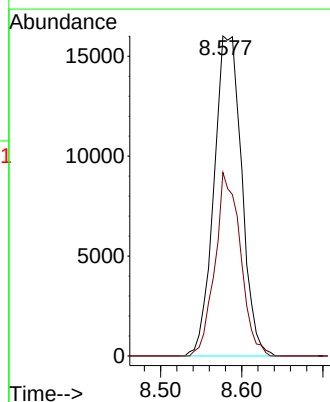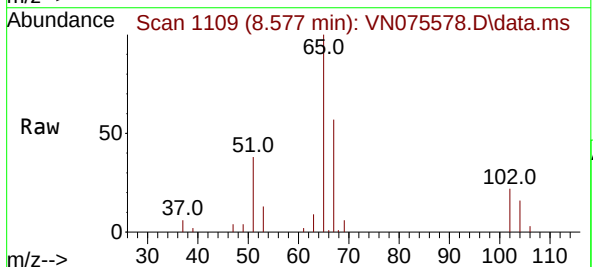

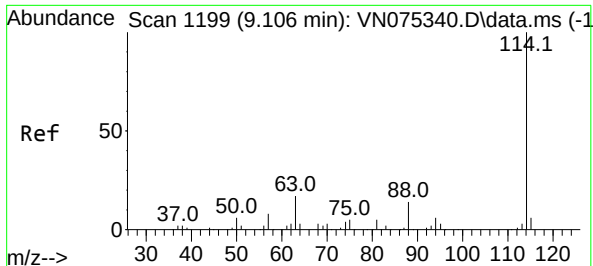

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN075578.D

Acq: 06 Dec 2022 12:13

Instrument :

MSVOA_N

ClientSampleId :

VN1206MBL01





Tgt Ion:114 Resp: 217572

Ion Ratio Lower Upper

114 100

63 16.6 0.0 39.6

88 14.2 0.0 29.0

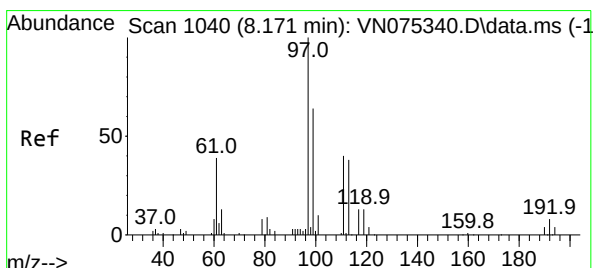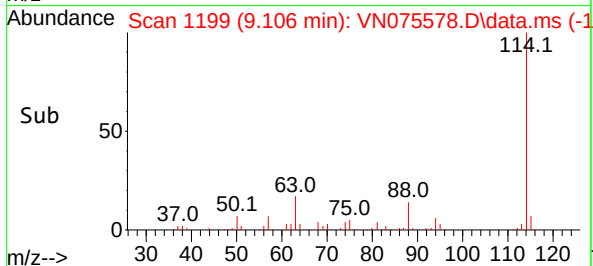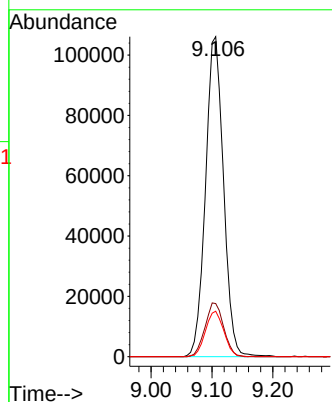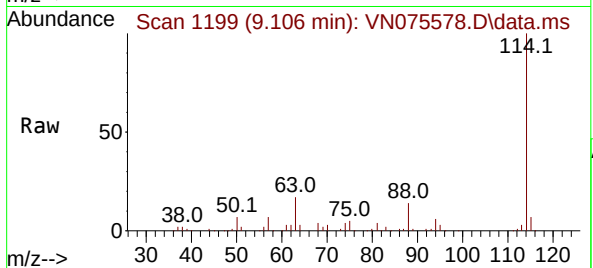

#35

Dibromofluoromethane

Concen: 54.969 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN075578.D

Acq: 06 Dec 2022 12:13




Tgt Ion:113 Resp: 46982


Ion Ratio Lower Upper

113 100

111 103.0 80.5 120.7

192 19.2 13.2 19.8


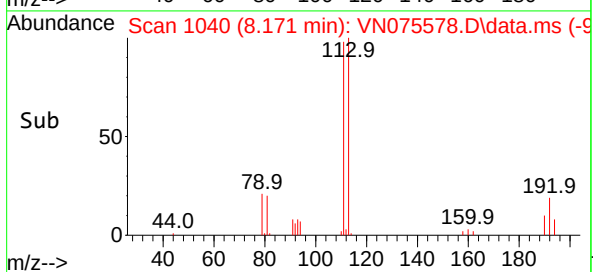
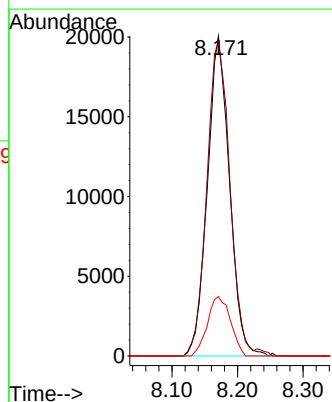
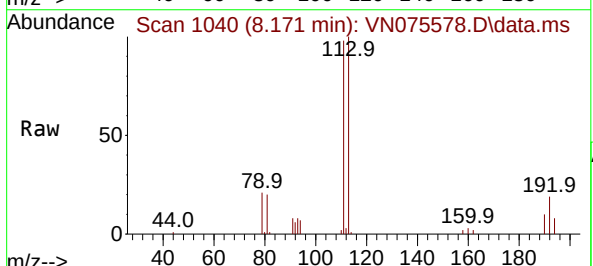


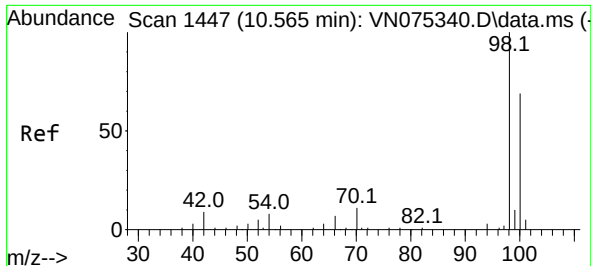

#50
Toluene-d8
Concen: 48.665 ug/l
RT: 10.571 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN075578.D
Acq: 06 Dec 2022 12:13




Instrument :
MSVOA_N
ClientSampleId :
VN1206MBL01


Tgt Ion: 98 Resp: 93681
Ion Ratio Lower Upper
98 100
100 65.6 53.0 79.6

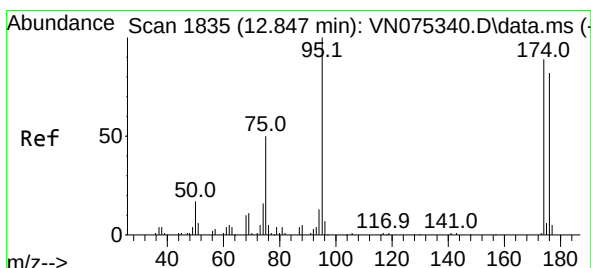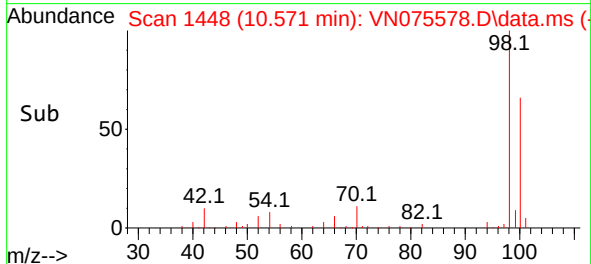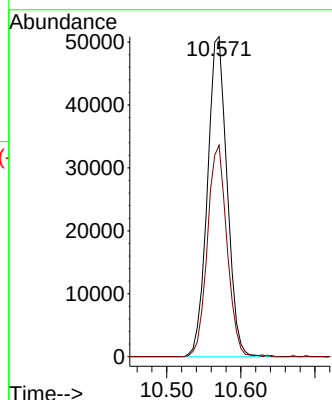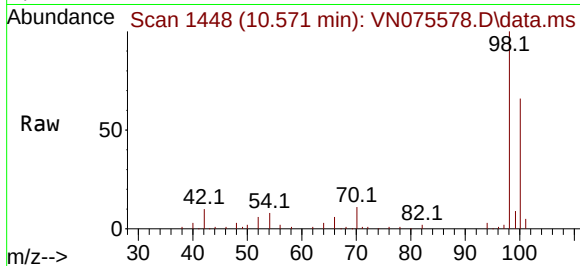

#62
4-Bromofluorobenzene
Concen: 44.436 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075578.D
Acq: 06 Dec 2022 12:13

Tgt Ion: 95 Resp: 63138
Ion Ratio Lower Upper
95 100
174 86.1 0.0 147.4
176 83.4 0.0 142.2


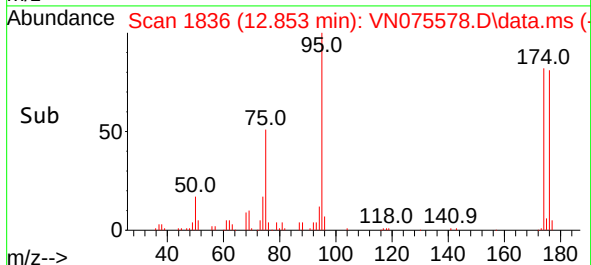
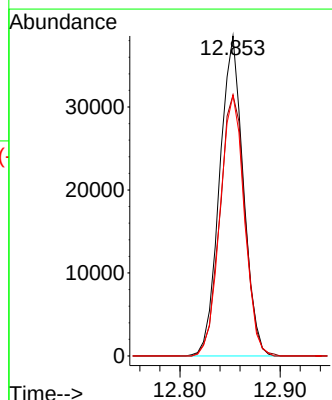
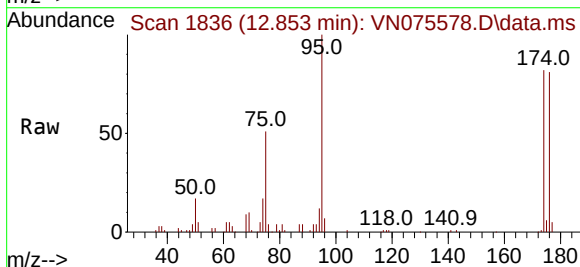


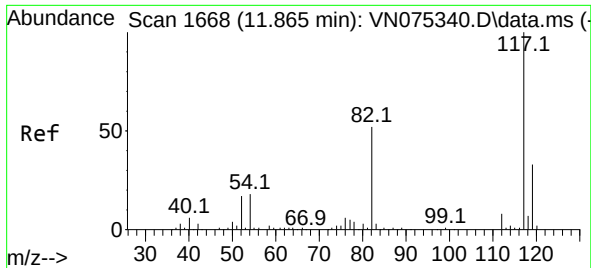

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN075578.D
Acq: 06 Dec 2022 12:13

Instrument :
MSVOA_N
ClientSampleId :
VN1206MBL01

Tgt Ion:117 Resp: 188987
Ion Ratio Lower Upper
117 100
82 52.4 43.1 64.7
119 31.0 25.5 38.3

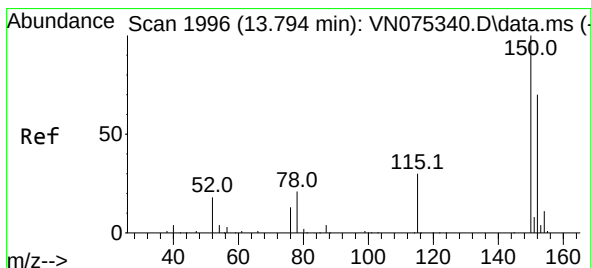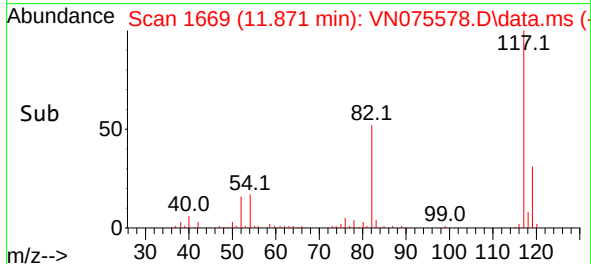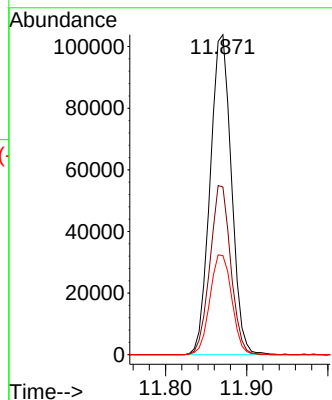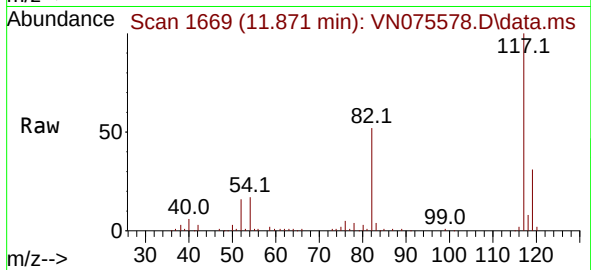

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN075578.D
Acq: 06 Dec 2022 12:13

Tgt Ion:152 Resp: 78499
Ion Ratio Lower Upper
152 100
115 57.8 30.2 90.6
150 157.0 0.0 348.4

