
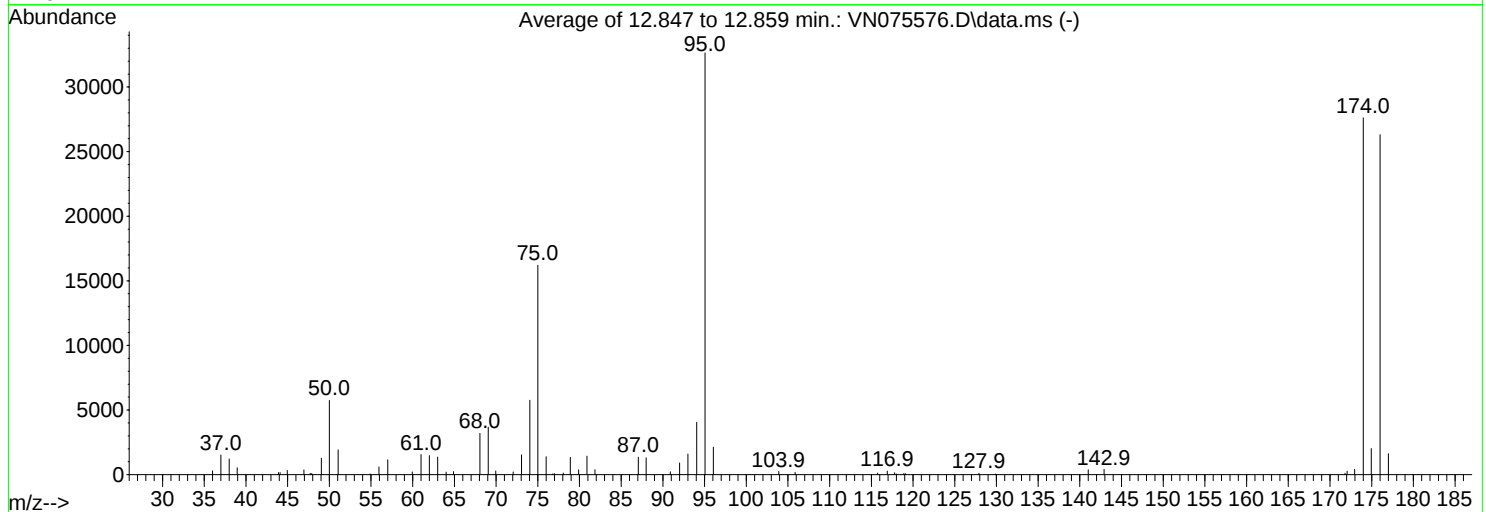


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120622\
Data File : VN075576.D
Acq On : 06 Dec 2022 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Title : SW846 8260
Last Update : Wed Nov 23 00:18:03 2022

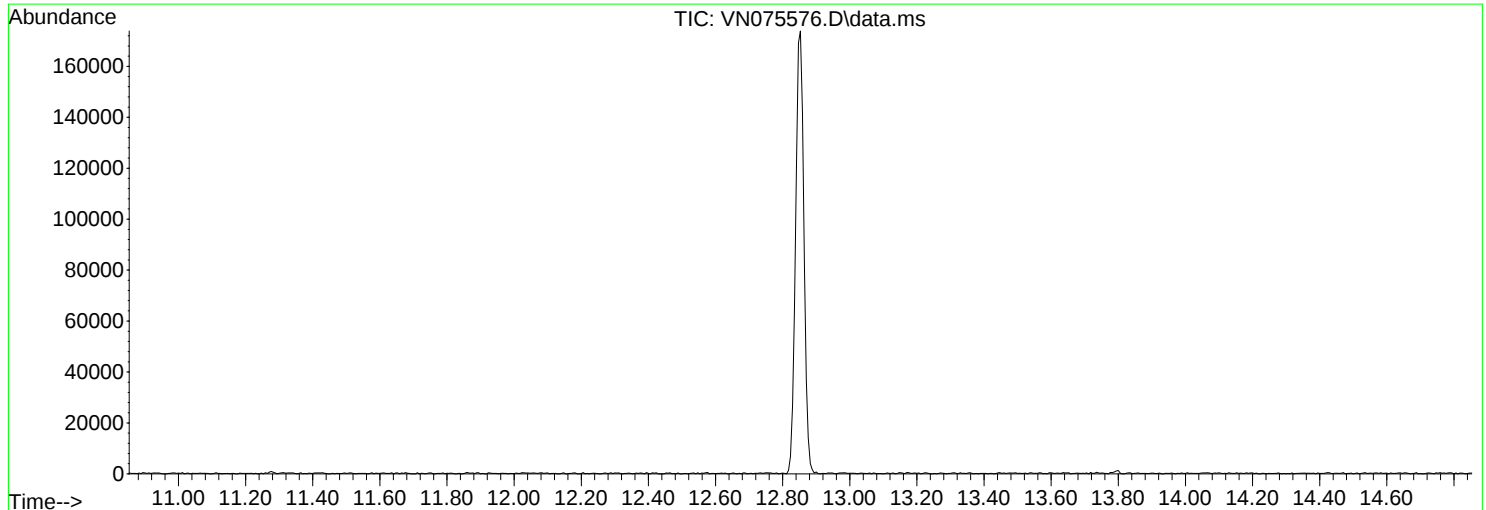

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	5752	PASS
75	95	30	60	49.6	16206	PASS
95	95	100	100	100.0	32645	PASS
96	95	5	9	6.5	2129	PASS
173	174	0.00	2	1.5	413	PASS
174	95	50	100	84.6	27613	PASS
175	174	5	9	7.3	2014	PASS
176	174	95	101	95.3	26309	PASS
177	176	5	9	6.2	1629	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	296	50.00	5752	68.05	3199	78.90	1331
37.00	1523	51.05	1916	69.05	3675	79.90	371
38.00	1221	54.90	51	69.95	281	80.90	143
38.95	528	55.95	601	72.05	215	81.85	382
43.90	167	57.00	1148	73.05	1532	87.05	1347
44.10	167	59.95	210	74.05	5756	88.00	1304
44.95	325	61.00	1560	75.00	16206	90.90	219
46.95	372	62.00	1468	76.00	1384	92.00	906
47.70	95	63.00	1358	76.80	67	93.00	1592
47.90	97	64.00	197	77.00	73	94.05	4046
49.05	1271	64.90	240	78.05	127	95.05	32645

Average of 12.847 to 12.859 min.: VN075576.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2129	141.00	380				
103.90	245	142.90	407				
105.85	190	171.80	116				
115.75	127	172.05	269				
116.90	278	172.95	413				
117.80	149	174.00	27613				
118.00	50	174.95	2014				
118.90	103	176.00	26309				
119.10	79	177.00	1629				
127.90	109						
129.90	54						

Instrument :

MSVOA_N

ClientSampleId :

BFB