
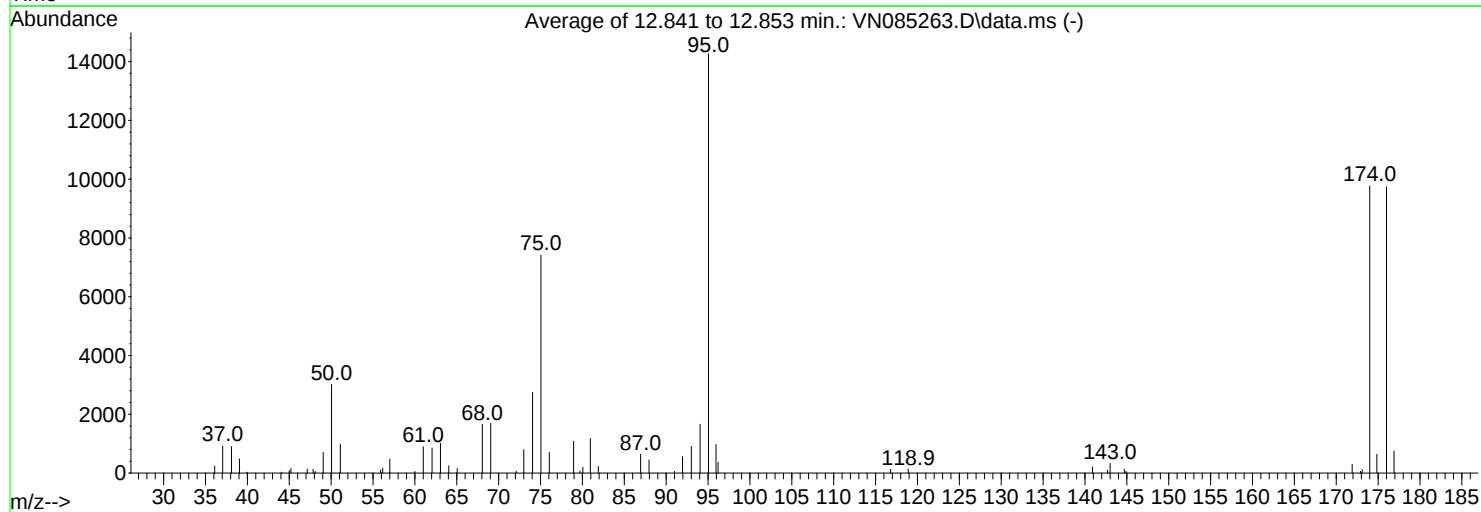


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121924\
Data File : VN085263.D
Acq On : 19 Dec 2024 11:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N120624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Dec 06 22:50:42 2024

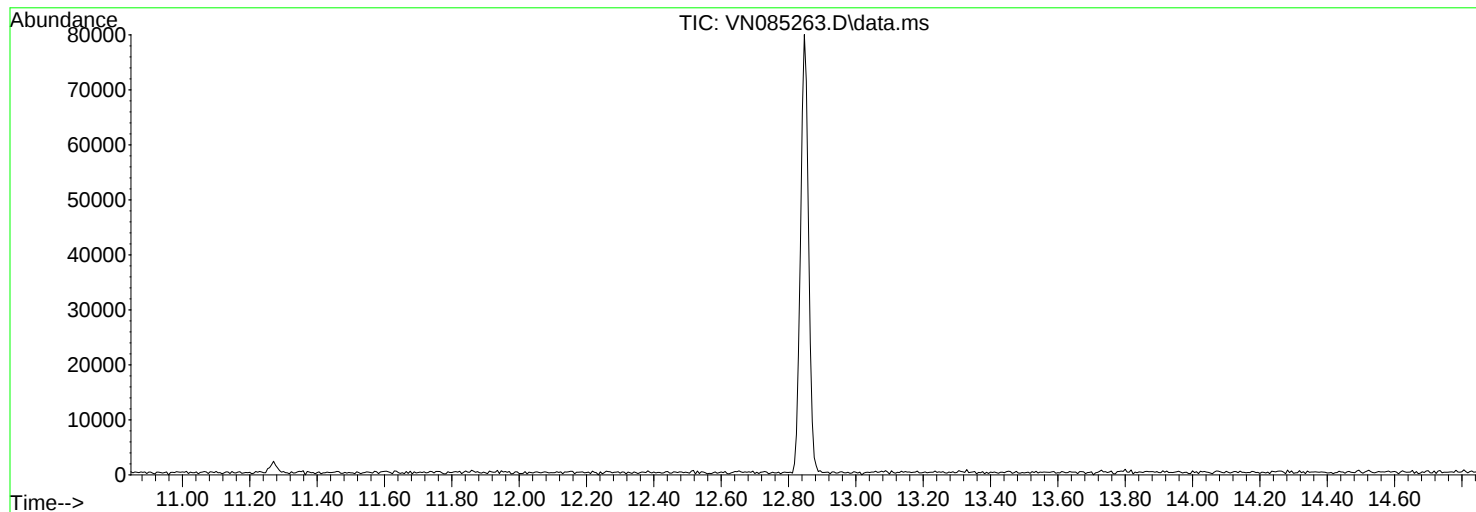

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	3021	PASS
75	95	30	60	52.0	7419	PASS
95	95	100	100	100.0	14269	PASS
96	95	5	9	6.8	971	PASS
173	174	0.00	2	1.2	115	PASS
174	95	50	100	68.4	9767	PASS
175	174	5	9	6.6	640	PASS
176	174	95	101	99.7	9741	PASS
177	176	5	9	7.7	752	PASS