


1,1,2,2-Tetrachloroethane


Response Ratio

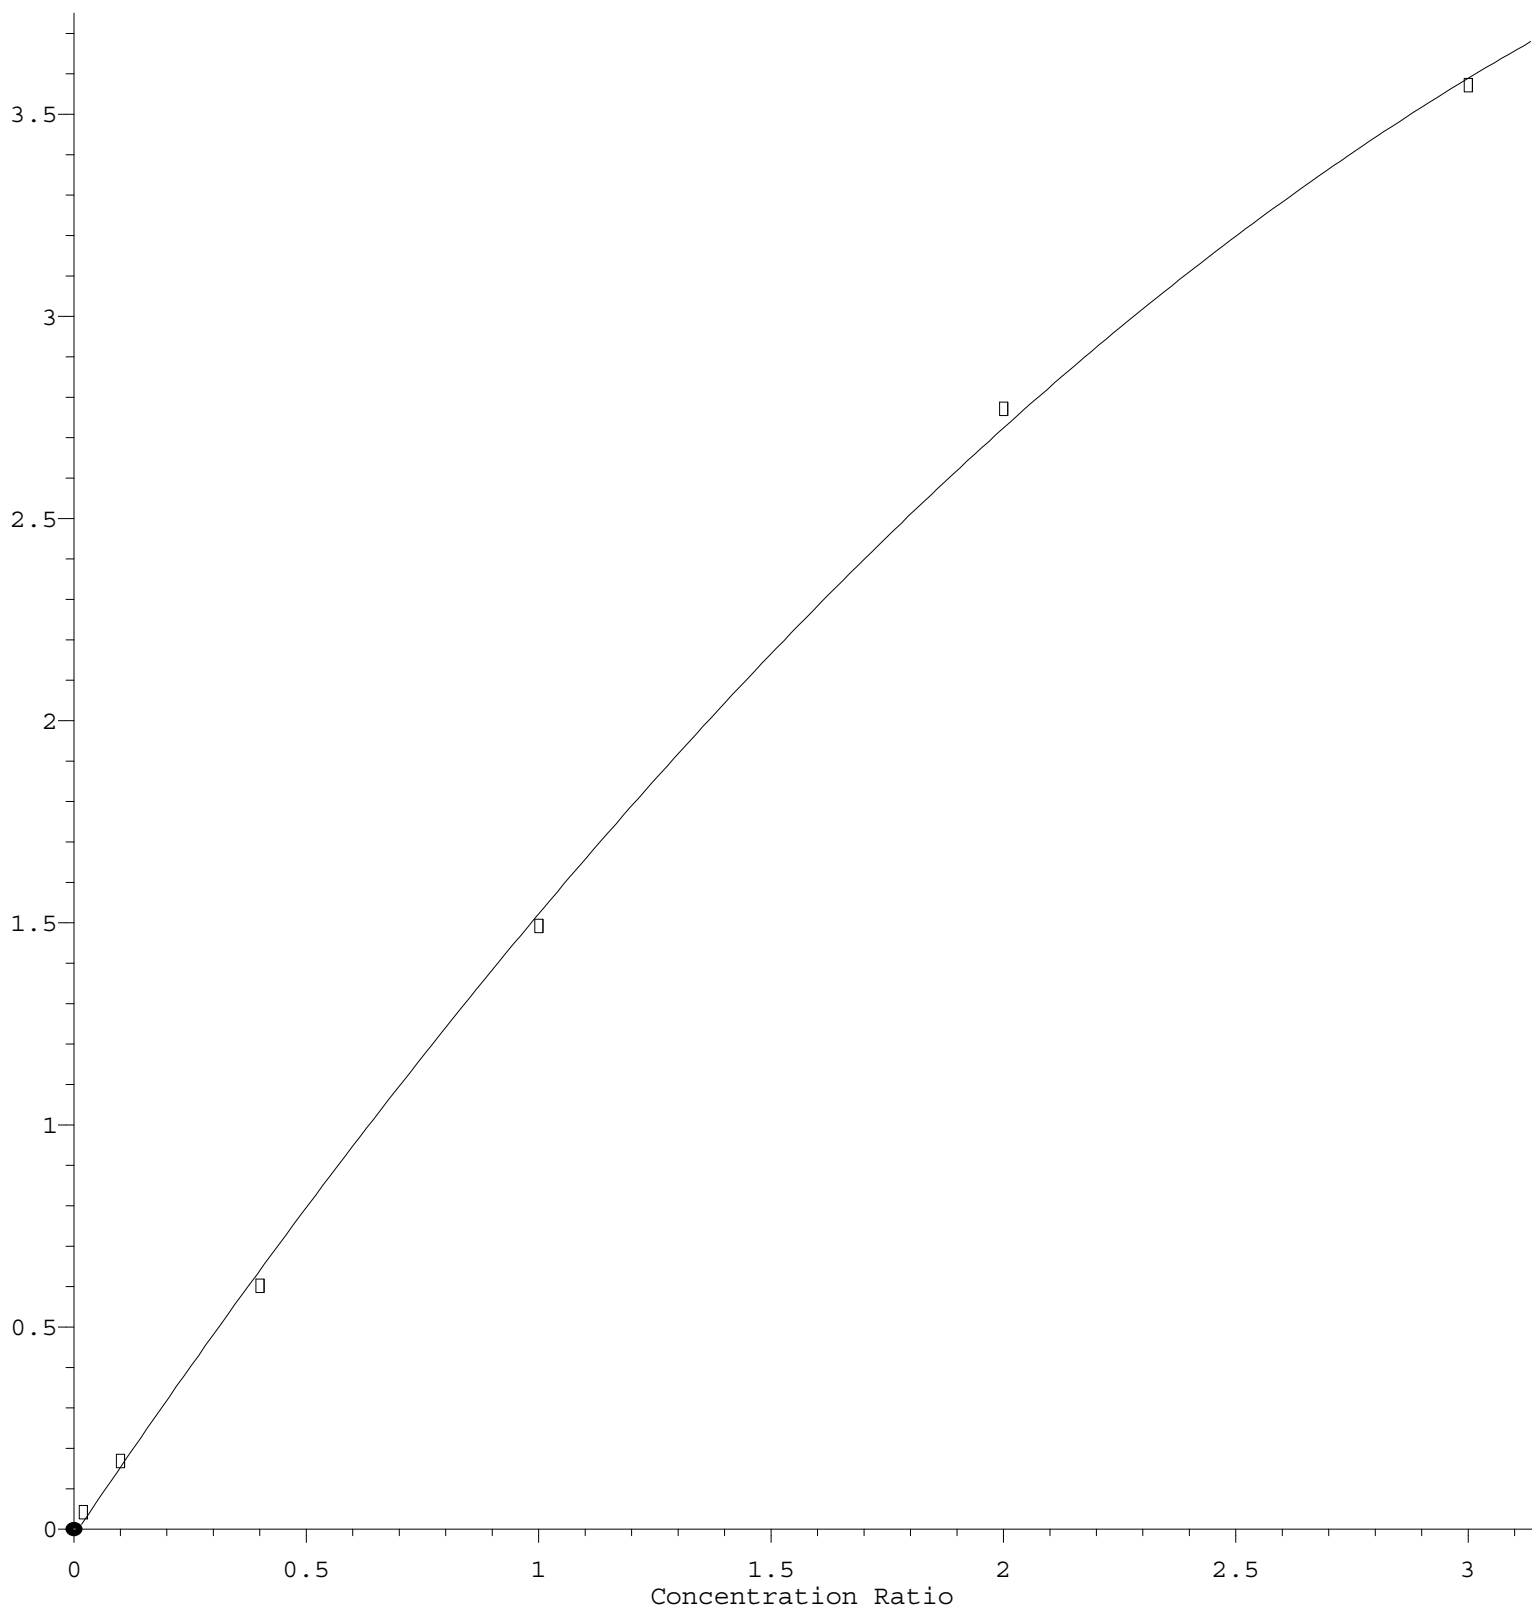

$R = -1.681e-001 A^2 + 1.706e+000 A - 1.524e-002$
 Coef of Det (r^2) = 0.999465 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N122721W.M
 Calibration Table Last Updated: Mon Dec 27 18:47:12 2021

1,2,3-Trichloropropane

Response Ratio

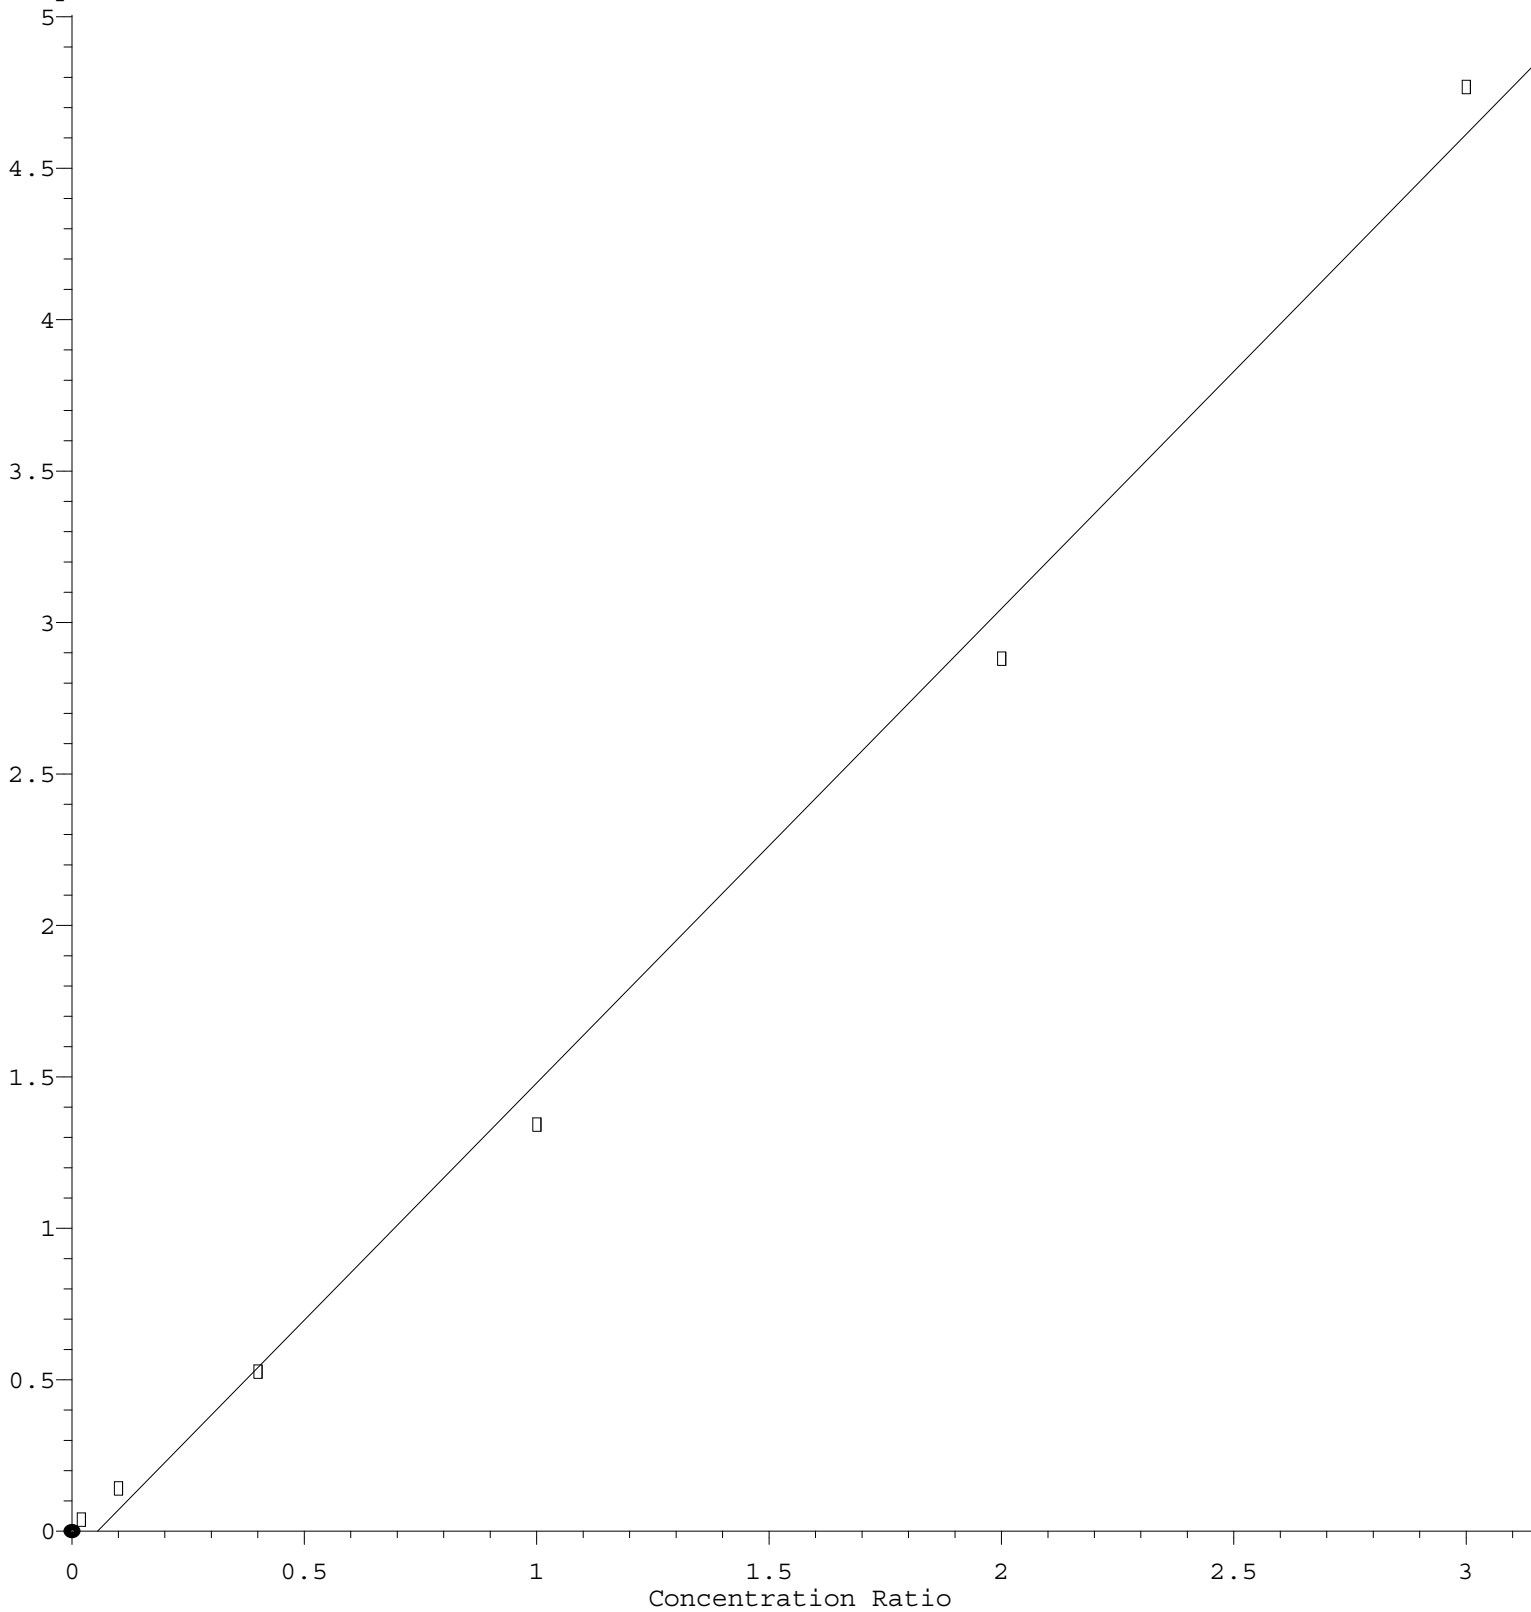

$$\text{Response} = 1.566\text{e}+000 * \text{Amt} - 8.562\text{e}-002$$


Coef of Det (r^2) = 0.995158 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N122721W.M

Calibration Table Last Updated: Mon Dec 27 18:47:12 2021

Naphthalene


Response Ratio

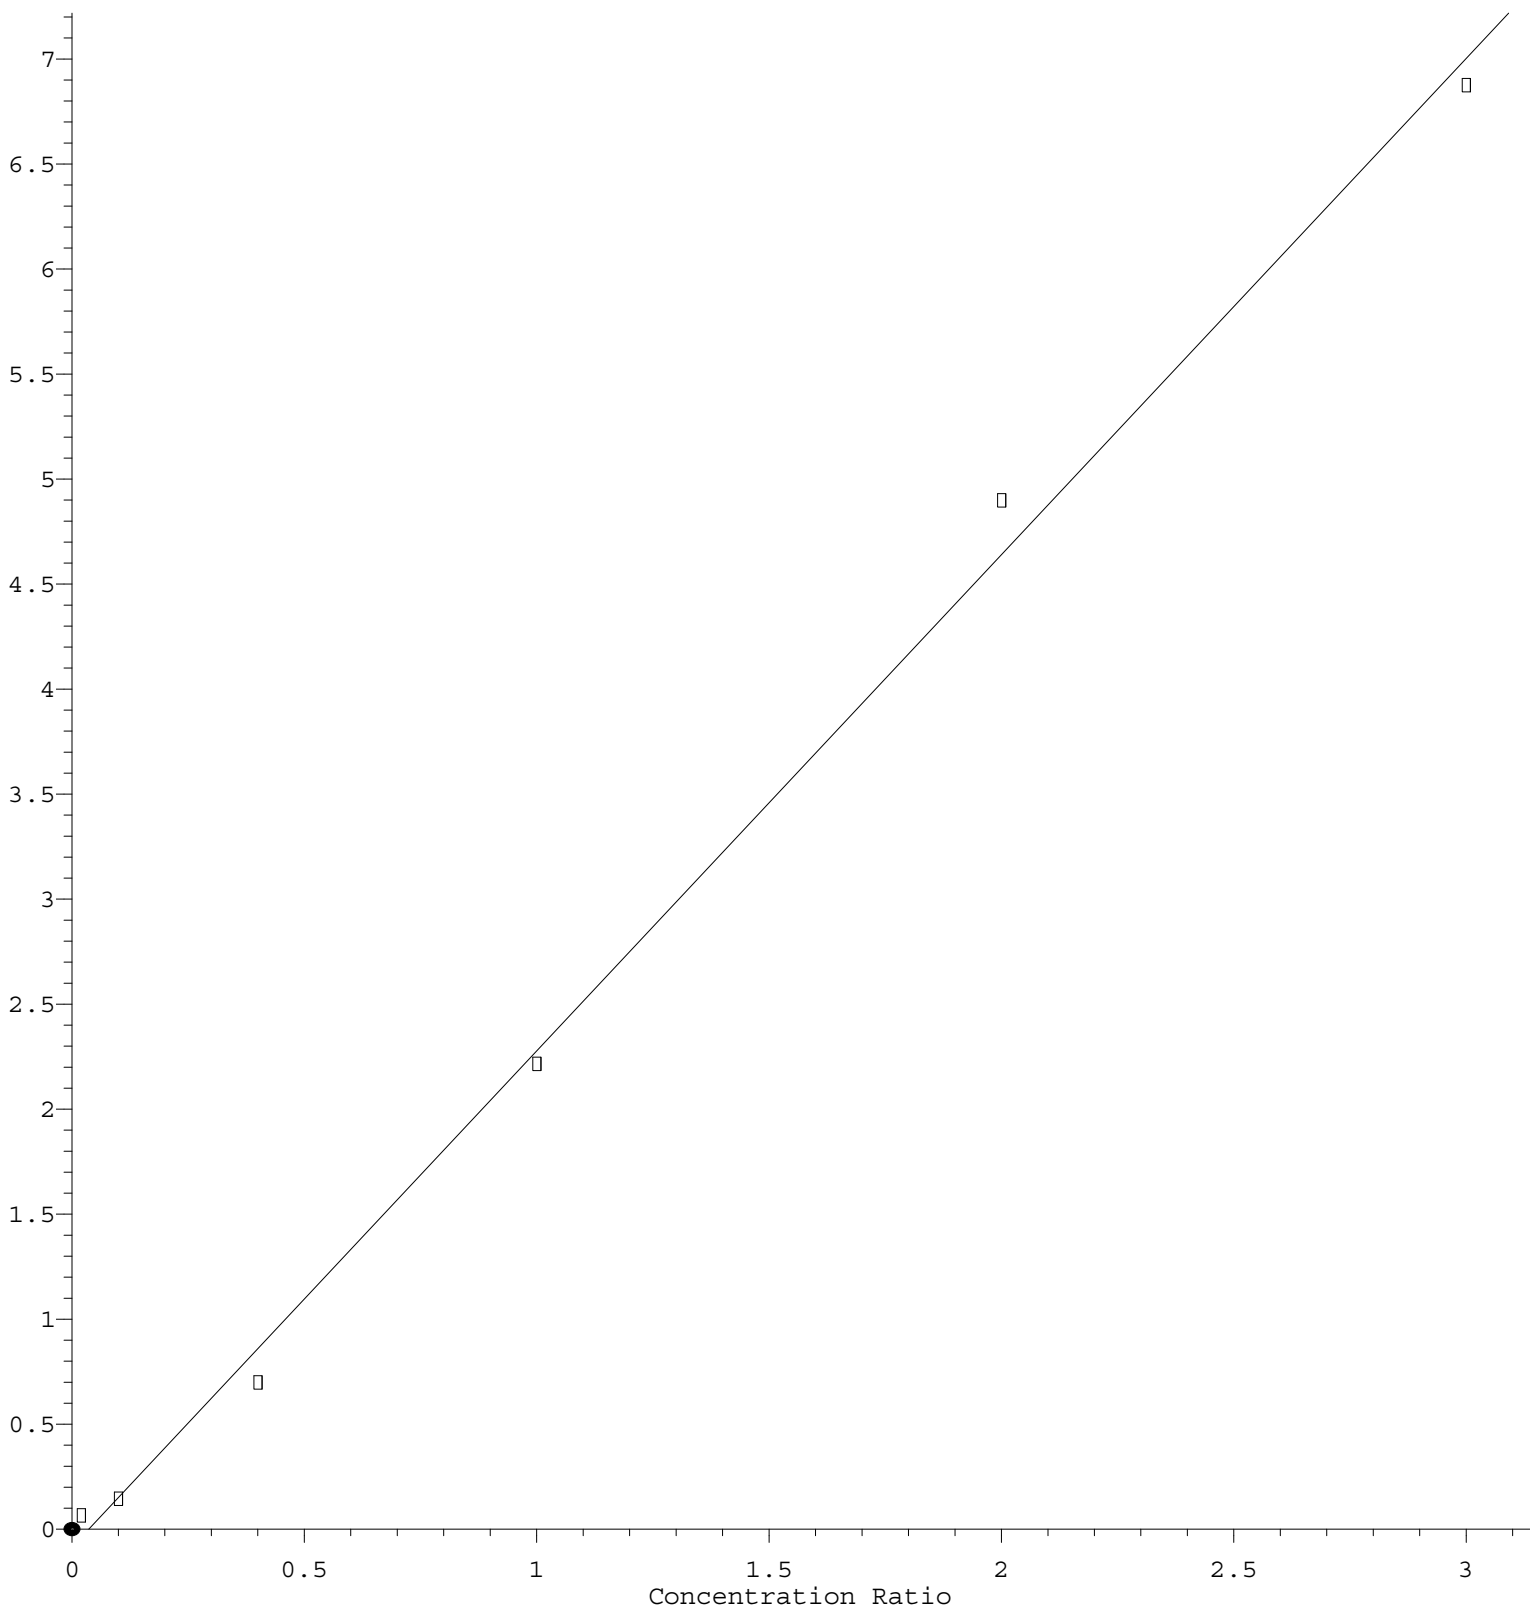

Response = 2.363e+000 * Amt - 8.492e-002
 Coef of Det (r^2) = 0.996888 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N122721W.M
 Calibration Table Last Updated: Mon Dec 27 18:47:12 2021

1,2,3-Trichlorobenzene

Response Ratio

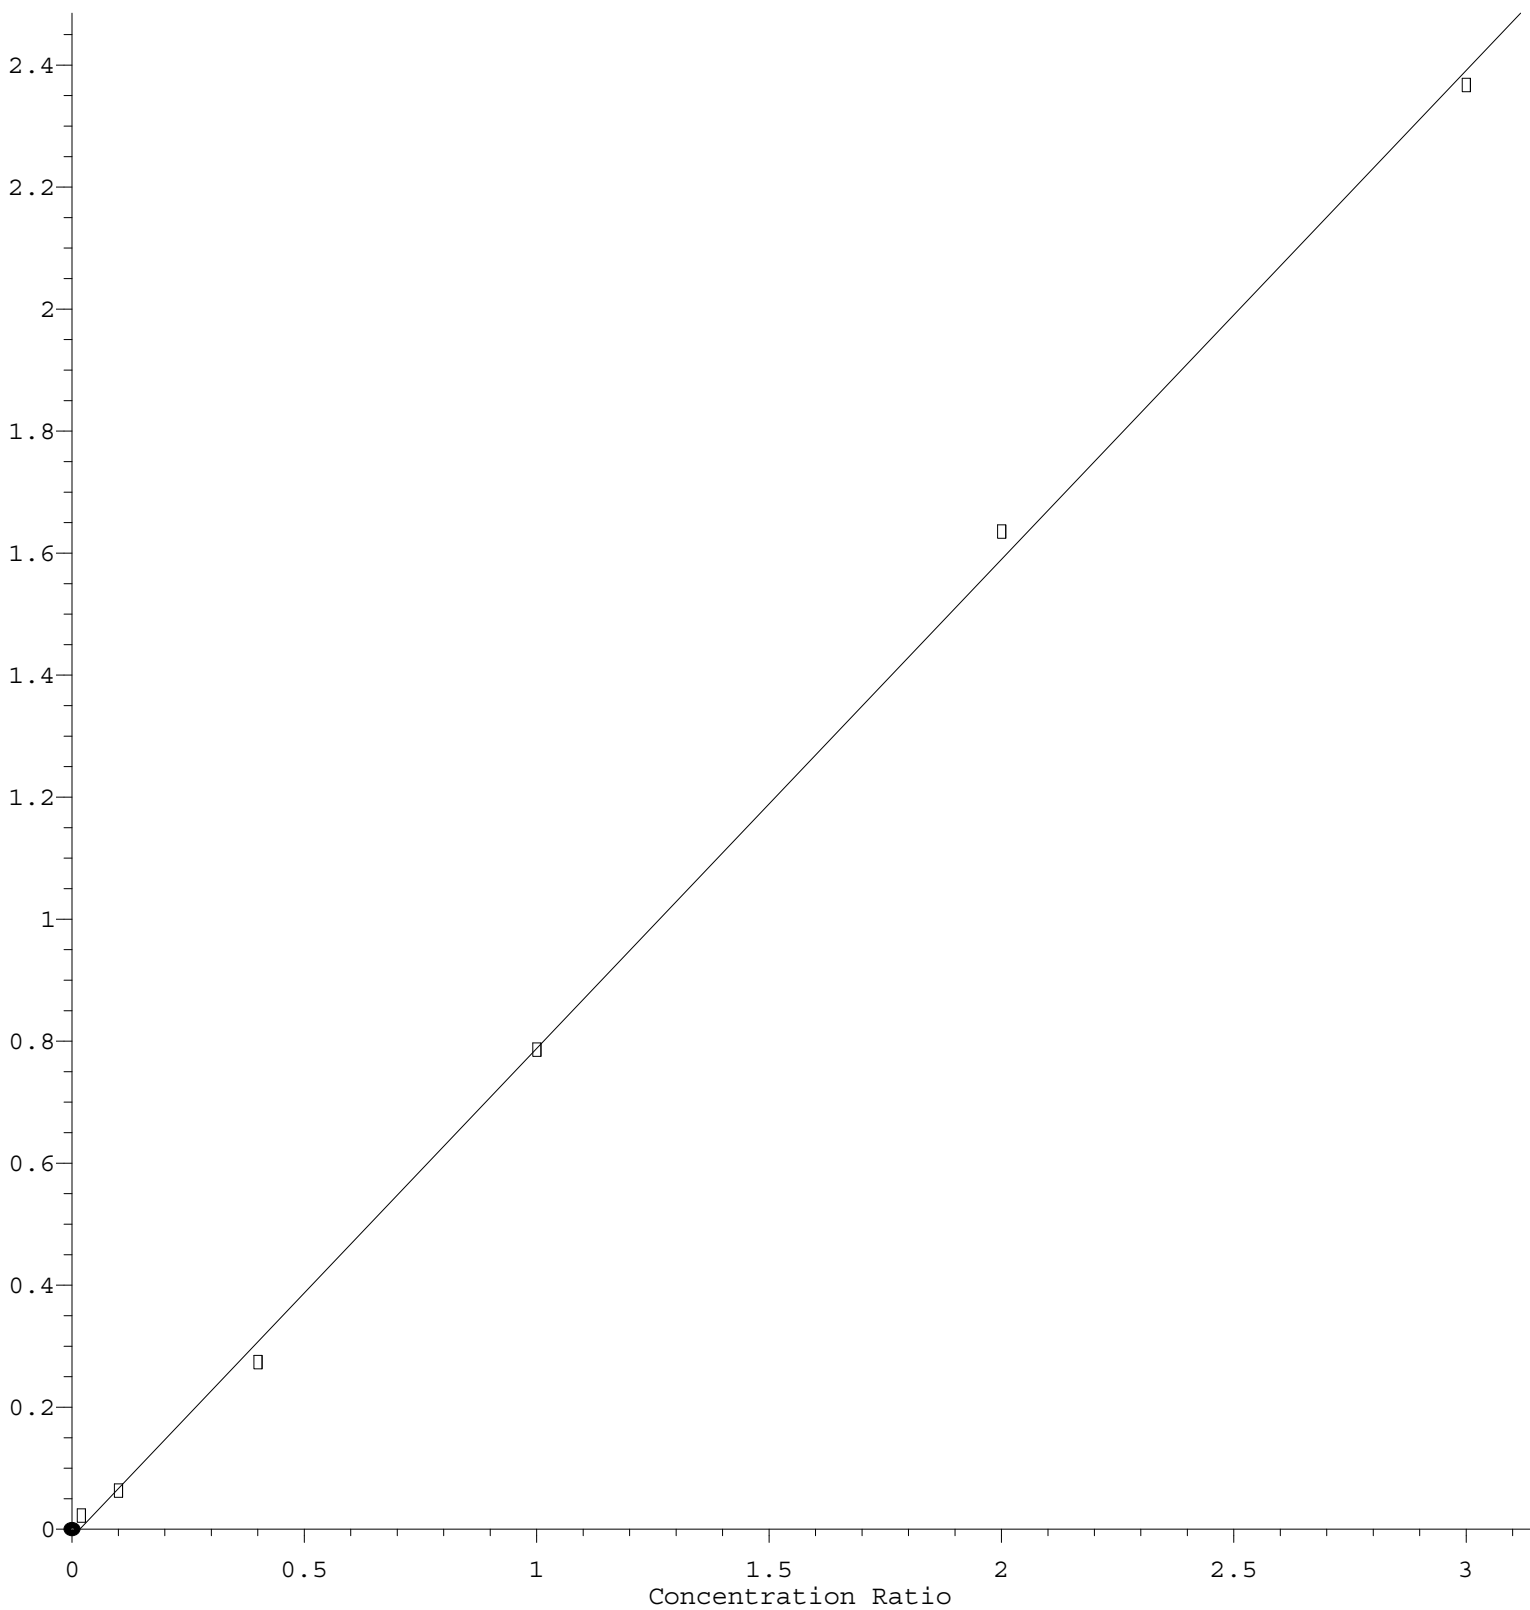

$$\text{Response} = 8.017\text{e-}001 * \text{Amt} - 1.325\text{e-}002$$


Coef of Det (r^2) = 0.999084 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N122721W.M

Calibration Table Last Updated: Mon Dec 27 18:47:12 2021

2-Chloroethyl Vinyl ether

Response Ratio

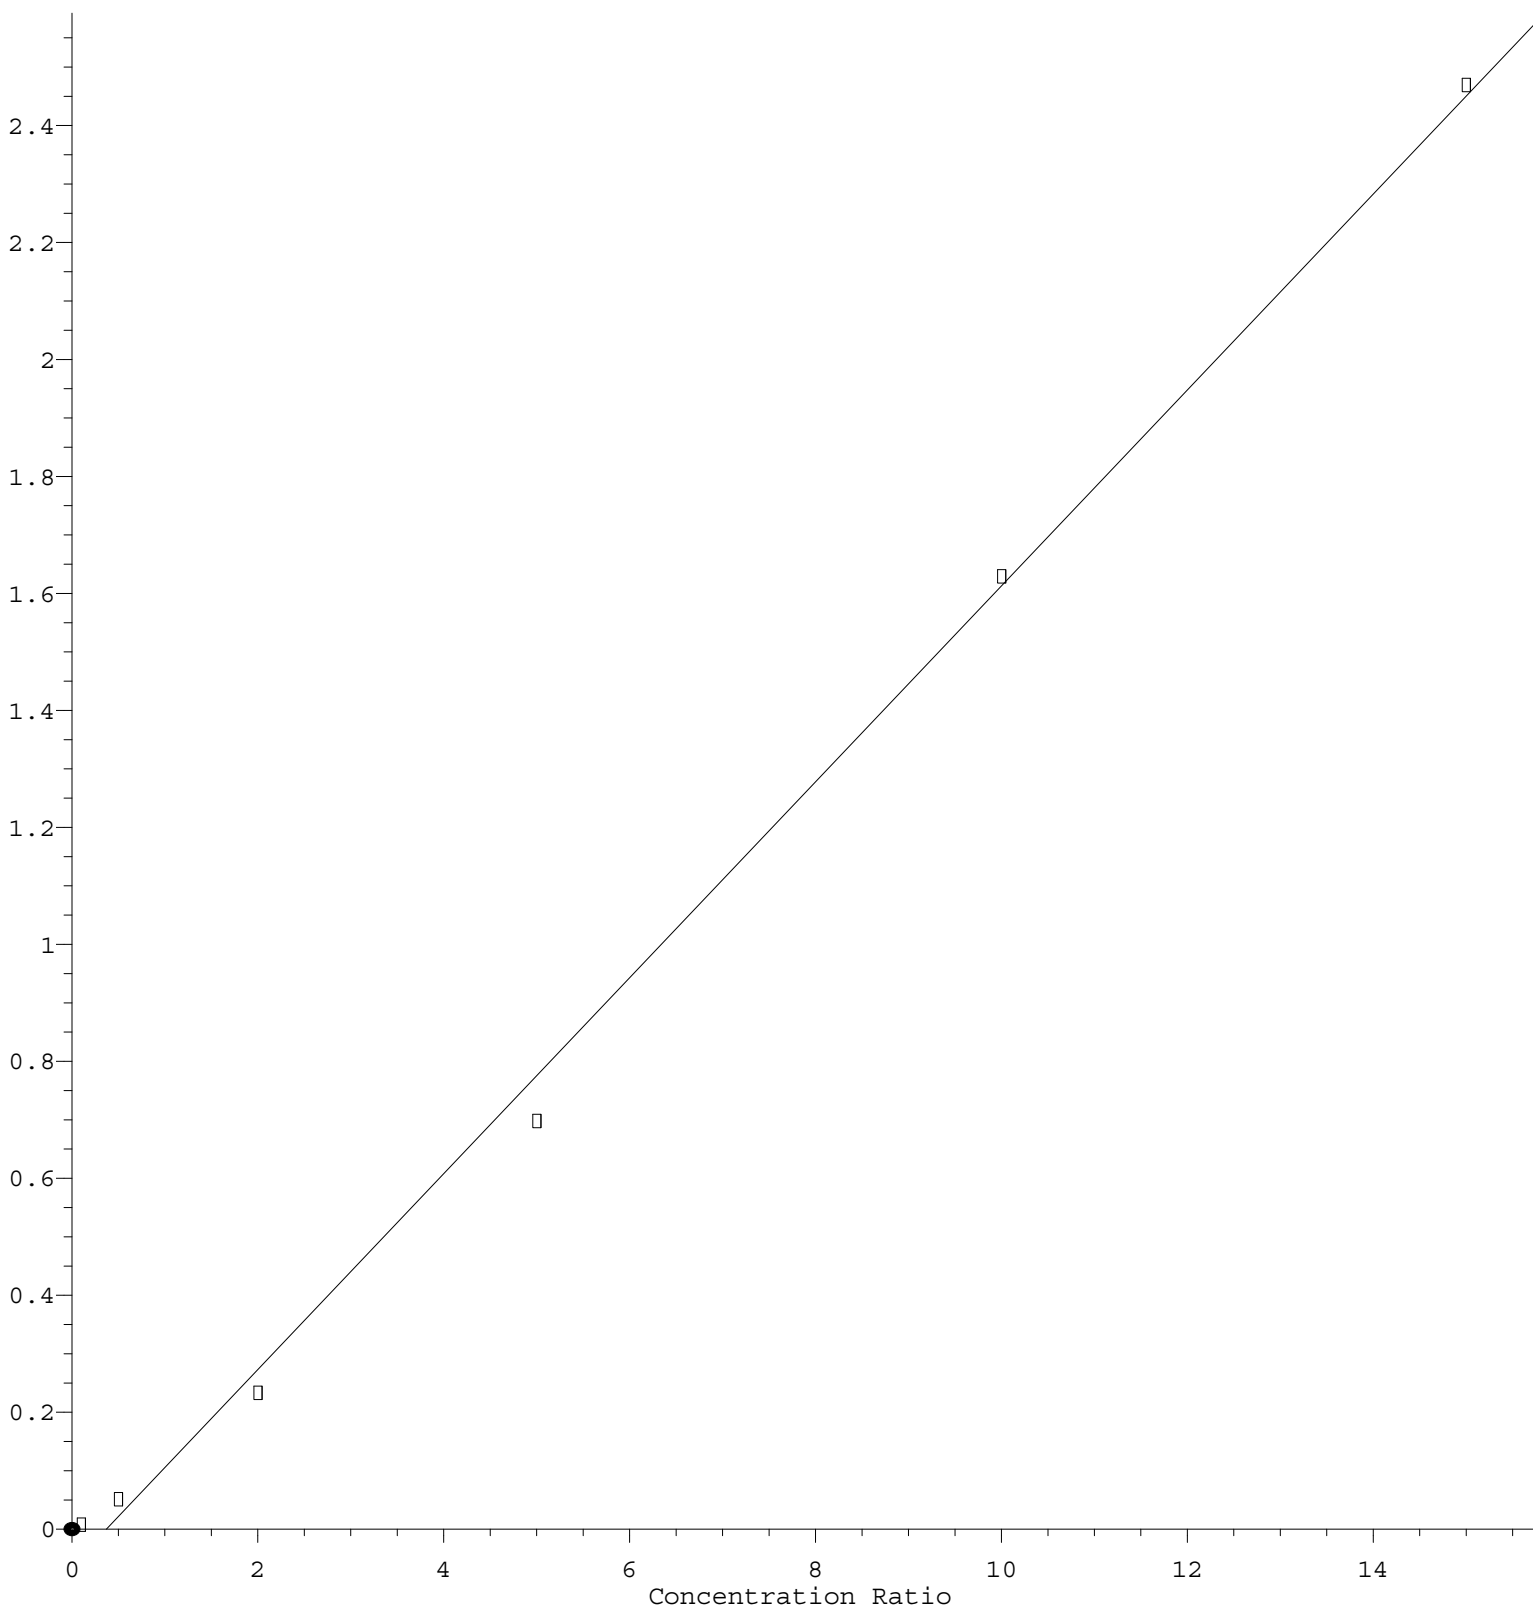

$$\text{Response} = 1.675\text{e-}001 * \text{Amt} - 6.201\text{e-}002$$

Coef of Det (r^2) = 0.997611 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N122721W.M

Calibration Table Last Updated: Mon Dec 27 18:47:12 2021