

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122922\
 Data File : VN076053.D
 Acq On : 29 Dec 2022 16:54
 Operator : JC\MD
 Sample : N6213-03DL 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-3DL

Quant Time: Dec 30 05:35:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	347933	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	549529	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	474445	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	209951	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	174598	46.127	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.260%
35) Dibromofluoromethane	8.171	113	162301	47.691	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.380%
50) Toluene-d8	10.570	98	617330	48.517	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.040%
62) 4-Bromofluorobenzene	12.847	95	198797	47.172	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.340%


Target Compounds						Qvalue
11) Tert butyl alcohol	5.530	59	277	0.517	ug/l #	72
16) Acetone	4.465	43	3481	2.668	ug/l	90
18) Methyl Acetate	5.030	43	1047	0.271	ug/l #	45
20) Methylene Chloride	5.288	84	1239	Below Cal	#	56
25) 2-Butanone	7.482	43	378	0.207	ug/l #	40
31) Cyclohexane	8.235	56	6850	1.264	ug/l #	1
36) 1,1-Dichloropropene	8.229	75	24029	5.315	ug/l #	50
37) Ethyl Acetate	7.577	43	2406	0.663	ug/l #	73
38) Carbon Tetrachloride	8.235	117	32960	6.514	ug/l #	17
40) Benzene	8.612	78	451553	32.374	ug/l	100
42) 1,2-Dichloroethane	8.612	62	4008	0.864	ug/l	76
43) Isopropyl Acetate	8.706	43	6392	1.067	ug/l #	66
51) 4-Methyl-2-Pentanone	10.447	43	1980	0.547	ug/l #	72
52) Toluene	10.635	92	218726	24.078	ug/l	98
53) t-1,3-Dichloropropene	10.629	75	2558	0.529	ug/l #	1
55) 1,1,2-Trichloroethane	10.888	97	1311	0.368	ug/l #	16
59) 2-Hexanone	11.176	43	2137	0.809	ug/l #	20
67) Ethyl Benzene	11.970	91	28242	1.718	ug/l	92
68) m/p-Xylenes	12.070	106	65008	9.994	ug/l	100
69) o-Xylene	12.400	106	58729	9.123	ug/l	99
70) Styrene	12.412	104	14170	1.384	ug/l #	40
71) Bromoform	12.853	173	1698	0.647	ug/l #	1
76) 1,2,3-Trichloropropane	12.847	75	99475	23.505	ug/l #	1
78) n-propylbenzene	13.041	91	4022	0.240	ug/l	82
79) 2-Chlorotoluene	13.094	91	2359	0.226	ug/l #	40
80) 1,3,5-Trimethylbenzene	13.176	105	13257	1.044	ug/l	84
81) trans-1,4-Dichloro-2-b...	12.847	75	99475	84.606	ug/l #	12
82) 4-Chlorotoluene	13.094	91	2359	0.226	ug/l #	40
83) tert-Butylbenzene	13.488	119	6017	0.537	ug/l #	68
84) 1,2,4-Trimethylbenzene	13.488	105	42911	3.406	ug/l	99
85) sec-Butylbenzene	13.488	105	42911	2.777	ug/l #	56
95) Naphthalene	15.647	128	201899	19.078	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122922\
Data File : VN076053.D
Acq On : 29 Dec 2022 16:54
Operator : JC\MD
Sample : N6213-03DL 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-3DL

Quant Time: Dec 30 05:35:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




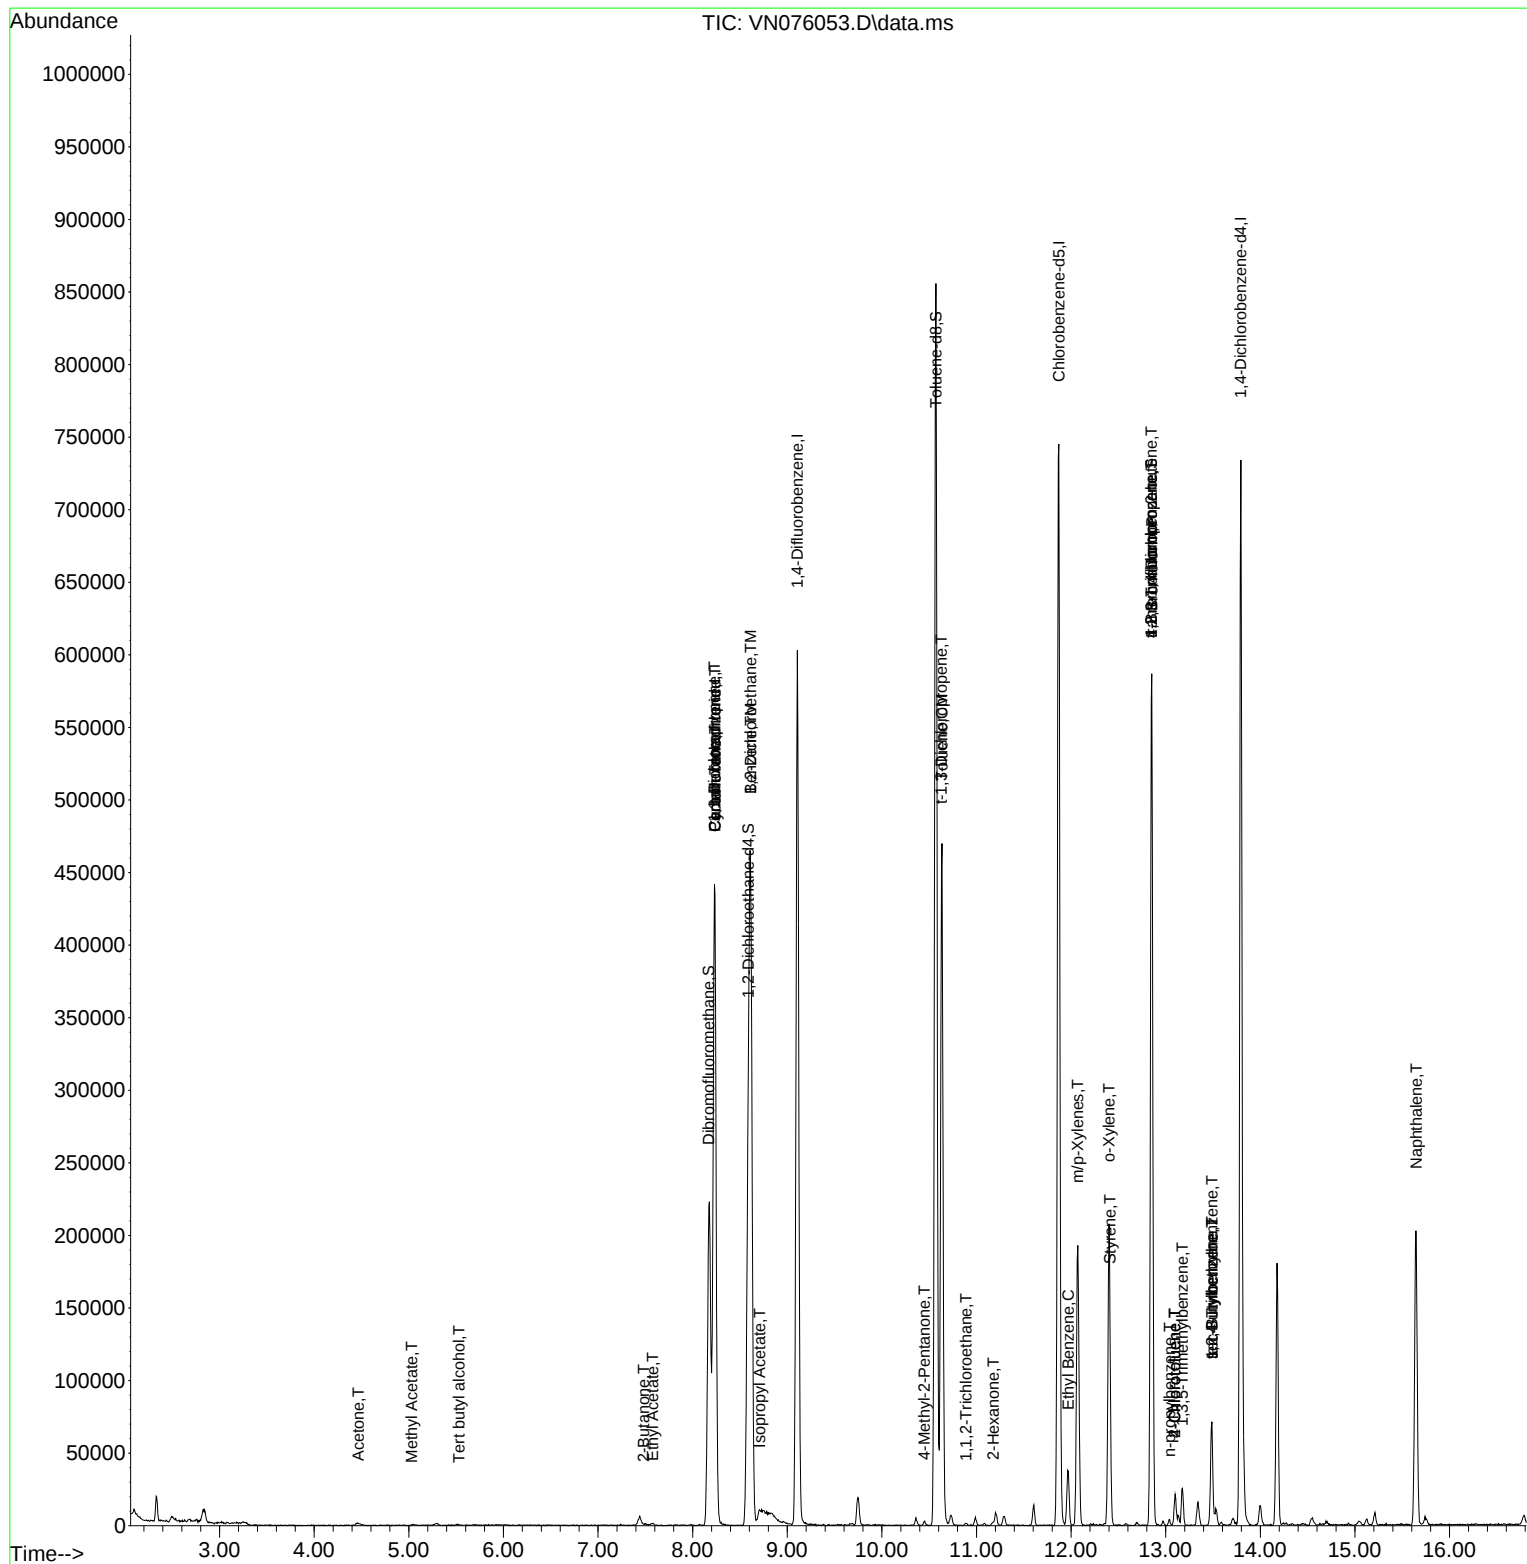




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1050
Delta R.T. 0.005 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion:168 Resp: 347933
Ion Ratio Lower Upper
168 100
99 53.0 44.2 66.4

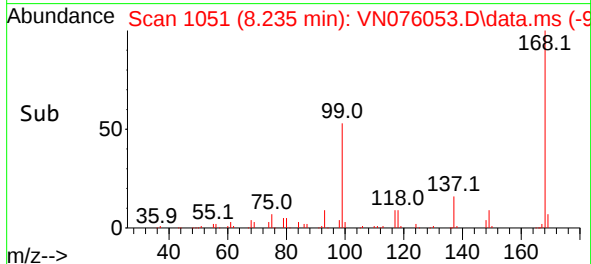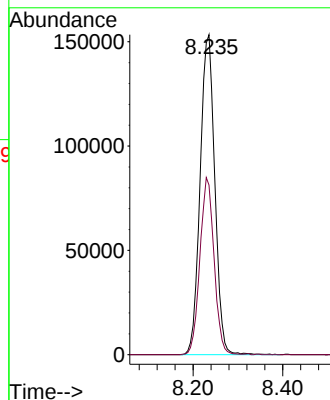

#11
Tert butyl alcohol
Concen: 0.517 ug/l
RT: 5.530 min Scan# 591
Delta R.T. -0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 59 Resp: 277
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#


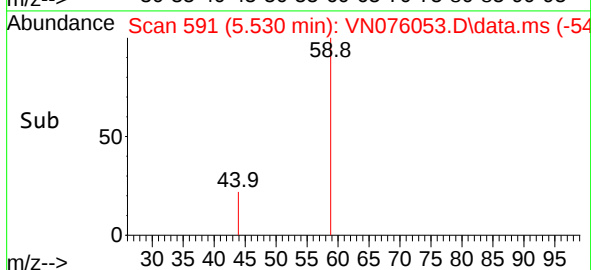
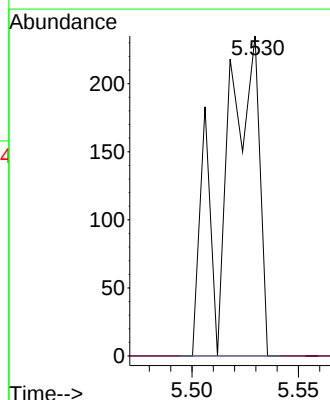





#16
Acetone
Concen: 2.668 ug/l
RT: 4.465 min Scan# 41
Delta R.T. 0.023 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL

Tgt Ion: 43 Resp: 3481
Ion Ratio Lower Upper
43 100
58 29.7 28.6 43.0

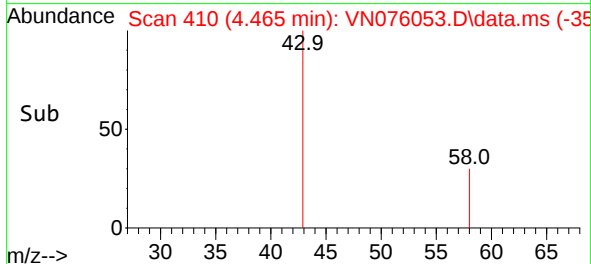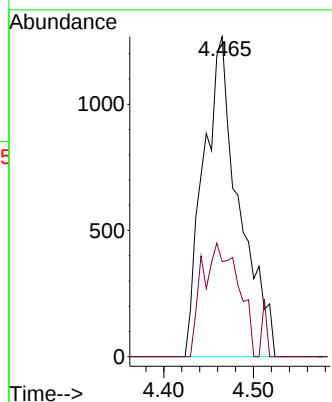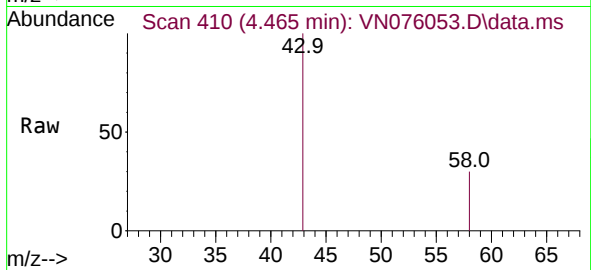

#18
Methyl Acetate
Concen: 0.271 ug/l
RT: 5.030 min Scan# 506
Delta R.T. -0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54


Tgt Ion: 43 Resp: 1047
Ion Ratio Lower Upper
43 100
74 0.0 23.6 35.4#

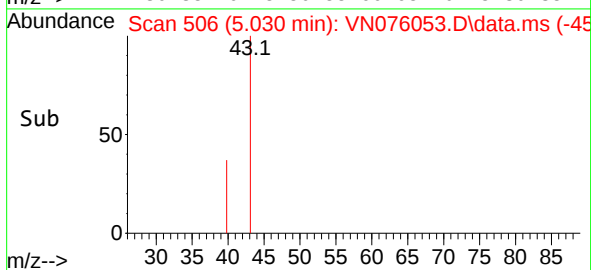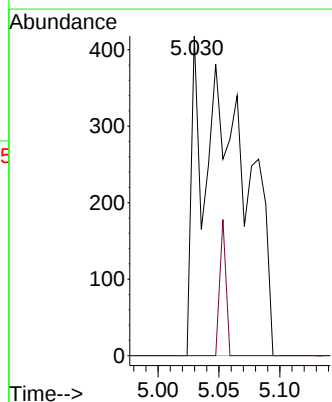





#20
Methylene Chloride
Concen: Below Cal
RT: 5.288 min Scan# 511
Delta R.T. -0.001 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Instrument :
MSVOA_N
ClientSampleId :
SB-3DL







Tgt Ion	84	Resp:	1239
Ion	Ratio	Lower	Upper
84	100		
49	50.5	81.8	122.6#
51	0.0	26.7	40.1#
86	44.8	51.5	77.3#



#25
2-Butanone
Concen: 0.207 ug/l
RT: 7.482 min Scan# 923
Delta R.T. -0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion	43	Resp:	378
Ion	Ratio	Lower	Upper
43	100		
72	0.0	28.0	42.0#

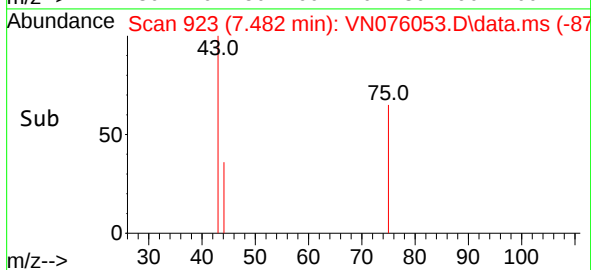

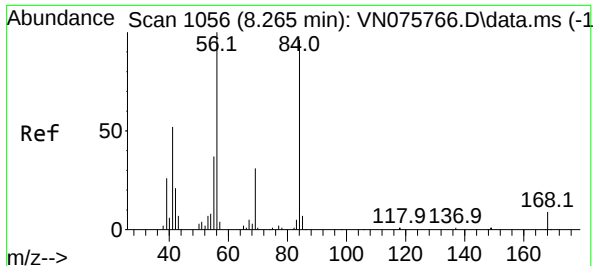

#31

Cyclohexane

Concen: 1.264 ug/l

RT: 8.235 min Scan# 1105

Delta R.T. -0.030 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54

Instrument :

MSVOA_N

ClientSampleId :

SB-3DL





Tgt Ion: 56 Resp: 6850

Ion Ratio Lower Upper

56 100

69 161.3 24.7 37.1#

84 148.1 76.5 114.7#

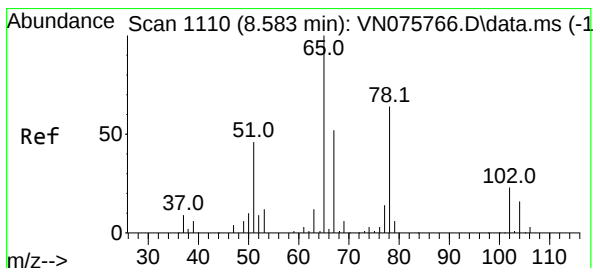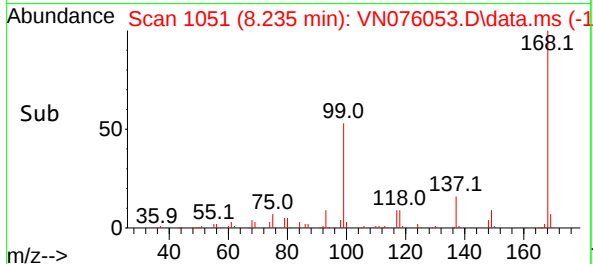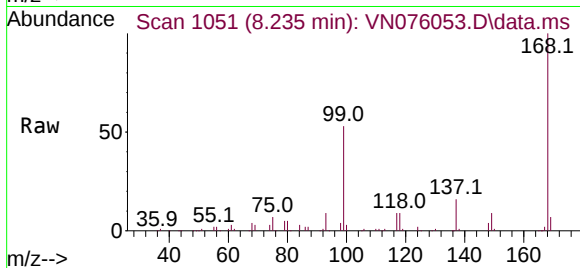

#33

1,2-Dichloroethane-d4

Concen: 46.127 ug/l

RT: 8.588 min Scan# 1111

Delta R.T. 0.006 min

Lab File: VN076053.D




Acq: 29 Dec 2022 16:54


Tgt Ion: 65 Resp: 174598

Ion Ratio Lower Upper

65 100

67 52.1 0.0 103.4

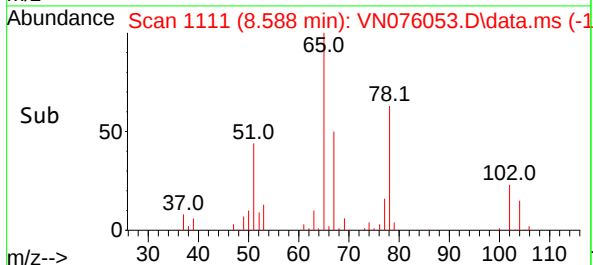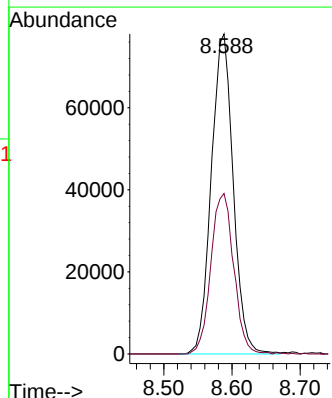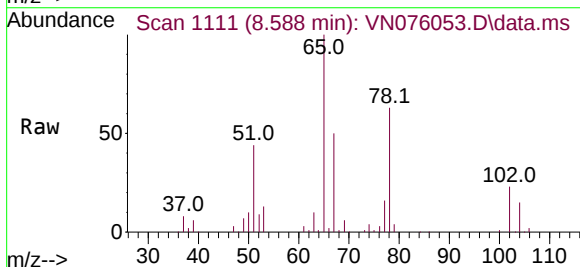

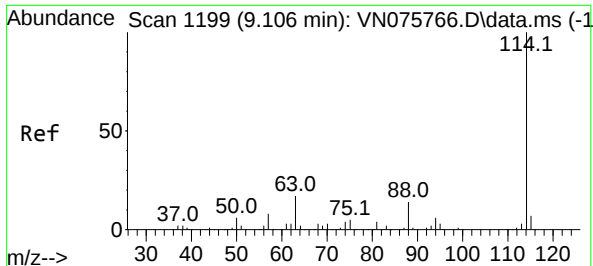

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54

Instrument :

MSVOA_N

ClientSampleId :

SB-3DL





Tgt Ion:114 Resp: 549529

Ion Ratio Lower Upper

114 100

63 16.3 0.0 34.4

88 14.6 0.0 28.8

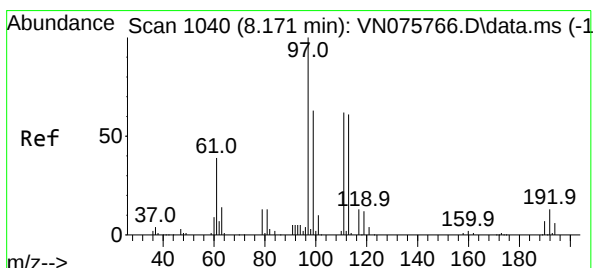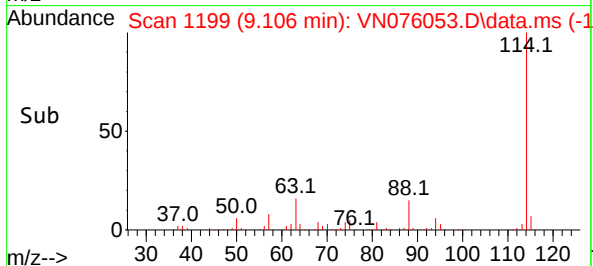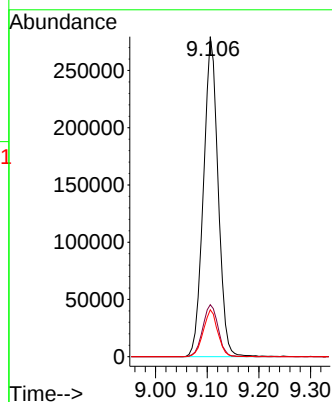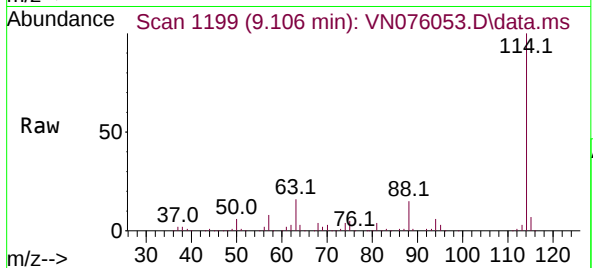

#35

Dibromofluoromethane

Concen: 47.691 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54




Tgt Ion:113 Resp: 162301


Ion Ratio Lower Upper

113 100

111 101.6 83.4 125.2

192 20.0 16.1 24.1

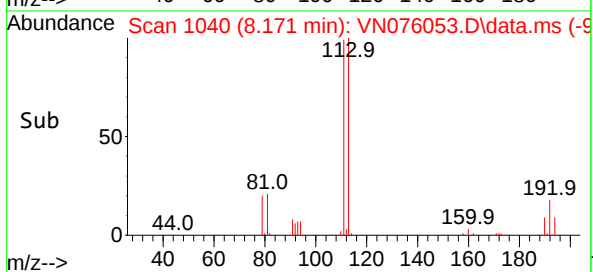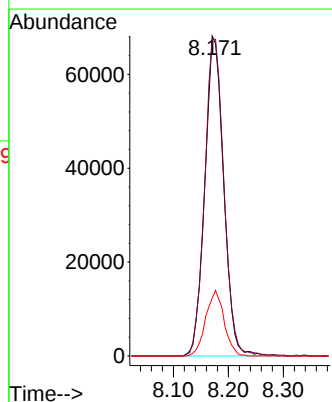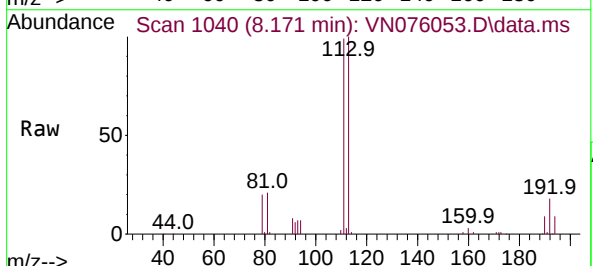

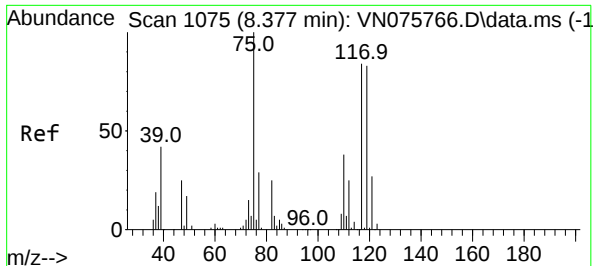

#36

1,1-Dichloropropene

Concen: 5.315 ug/l

RT: 8.229 min Scan# 1

Delta R.T. -0.147 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54

Instrument :

MSVOA_N

ClientSampleId :

SB-3DL





Tgt Ion: 75 Resp: 24029

Ion Ratio Lower Upper

75 100

110 10.6 18.8 56.4#

77 0.0 24.1 36.1#

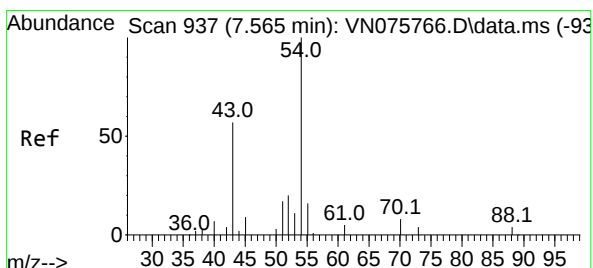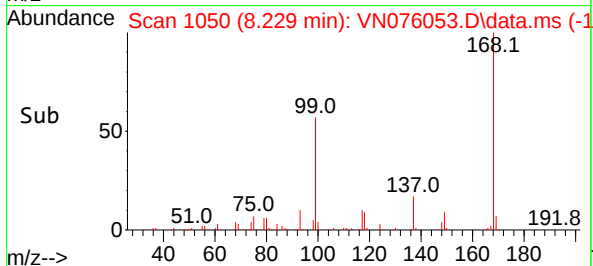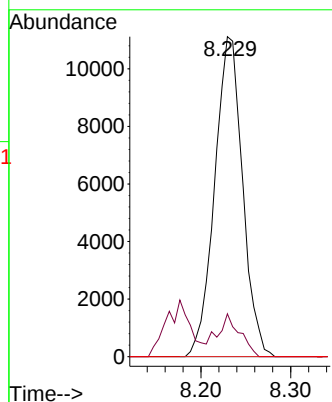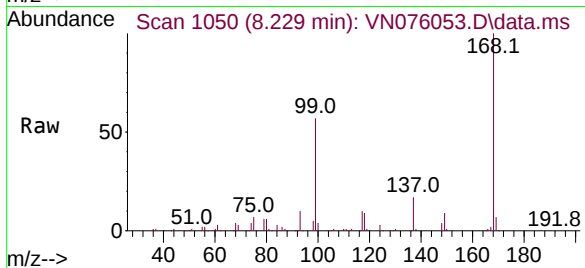

#37

Ethyl Acetate

Concen: 0.663 ug/l

RT: 7.577 min Scan# 939

Delta R.T. 0.012 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54




Tgt Ion: 43 Resp: 2406


Ion Ratio Lower Upper

43 100

61 3.3 13.0 19.4#


70 3.0 9.4 14.0#

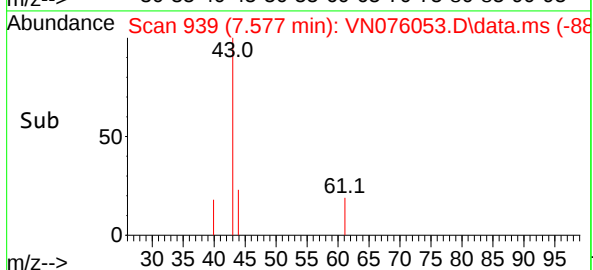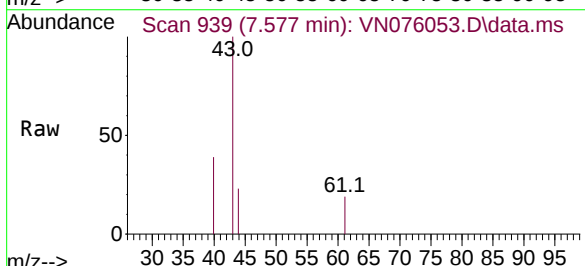



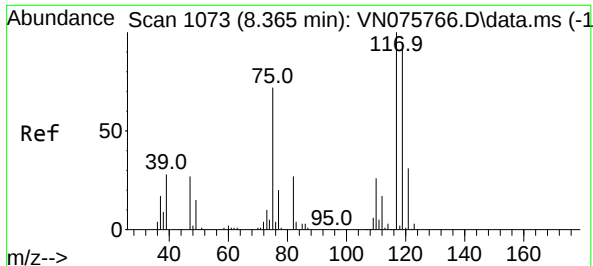


#38
Carbon Tetrachloride
Concen: 6.514 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.130 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Instrument :
MSVOA_N
ClientSampleId :
SB-3DL



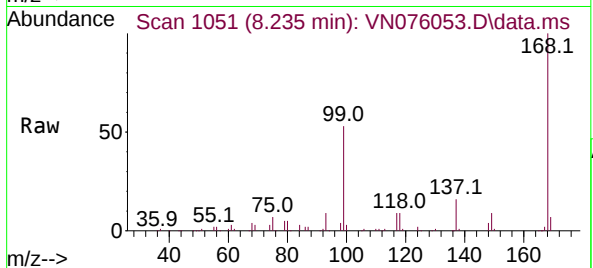



Tgt Ion:117 Resp: 32960
Ion Ratio Lower Upper
117 100
119 6.1 76.1 114.1#
121 0.0 24.5 36.7#

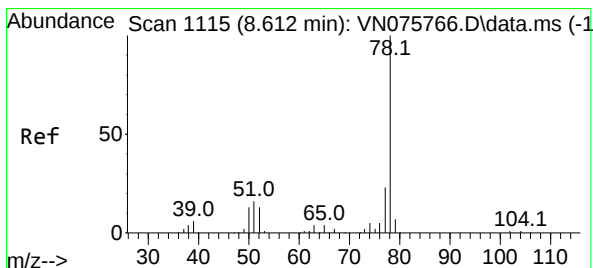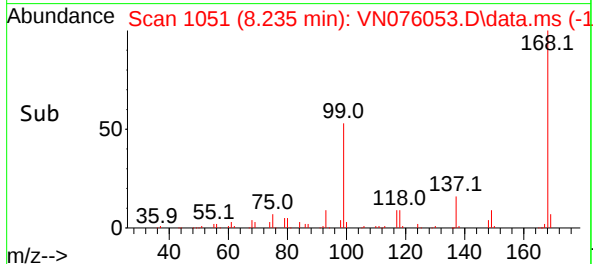

#40
Benzene
Concen: 32.374 ug/l
RT: 8.612 min Scan# 1115
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 78 Resp: 451553
Ion Ratio Lower Upper
78 100
77 23.1 18.5 27.7

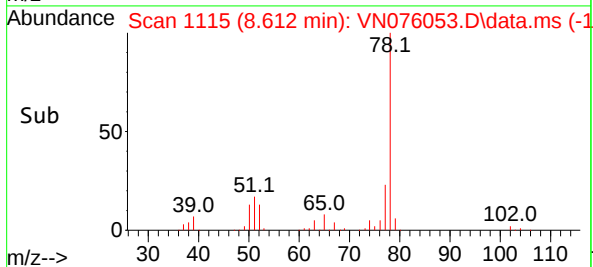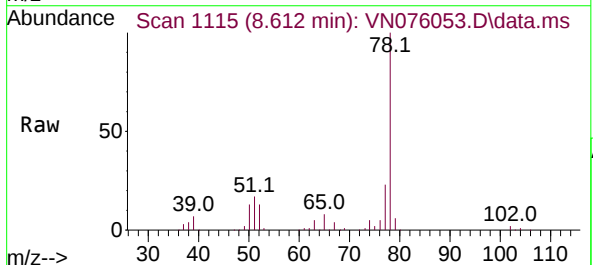

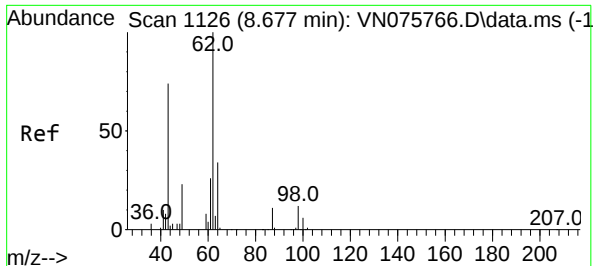

#42

1,2-Dichloroethane

Concen: 0.864 ug/l

RT: 8.612 min Scan# 1115

Delta R.T. -0.065 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54

Instrument :

MSVOA_N

ClientSampleId :





SB-3DL

Tgt Ion: 62 Resp: 4008

Ion Ratio Lower Upper

62 100

98 1.5 0.0 20.8

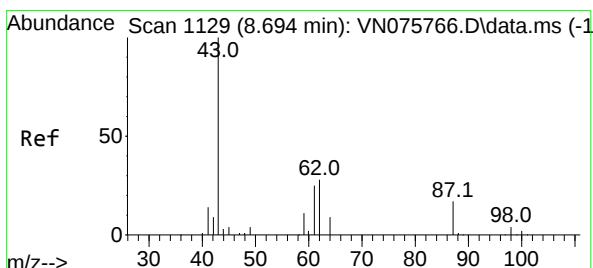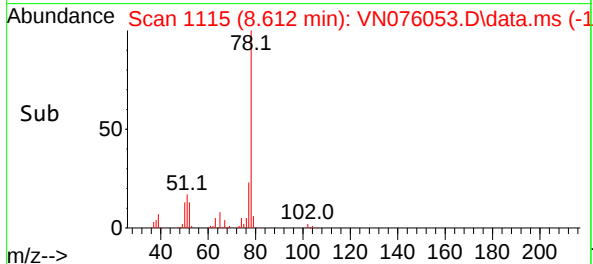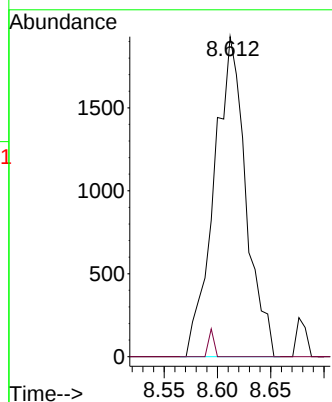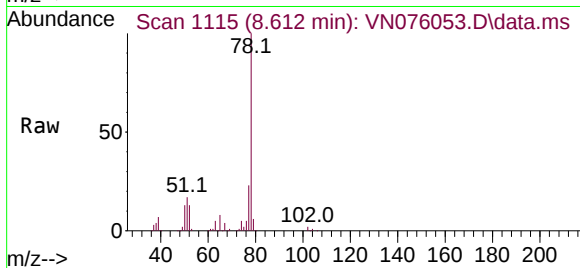

#43

Isopropyl Acetate

Concen: 1.067 ug/l

RT: 8.706 min Scan# 1131

Delta R.T. 0.012 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54




Tgt Ion: 43 Resp: 6392


Ion Ratio Lower Upper

43 100

61 11.5 24.2 36.4#

87 2.5 13.3 19.9#


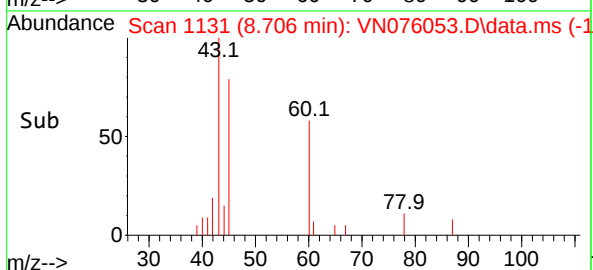

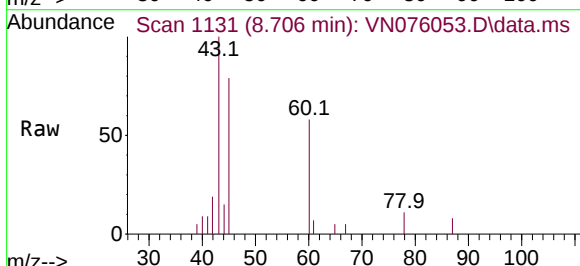




#50
Toluene-d8
Concen: 48.517 ug/l
RT: 10.570 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 98 Resp: 617330
Ion Ratio Lower Upper
98 100
100 66.0 52.1 78.1

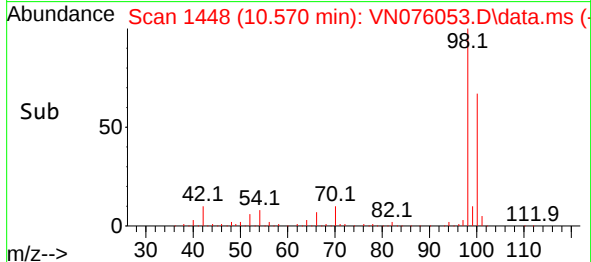

#51
4-Methyl-2-Pentanone
Concen: 0.547 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 43 Resp: 1980
Ion Ratio Lower Upper
43 100
58 26.4 35.5 53.3#




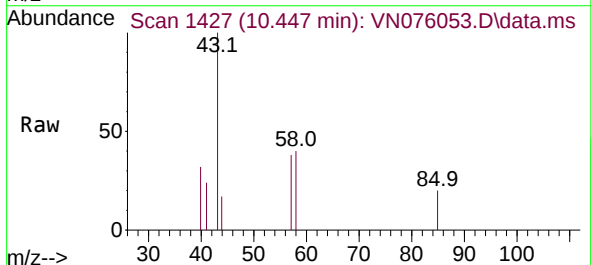




#52
Toluene
Concen: 24.078 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 92 Resp: 218726
Ion Ratio Lower Upper
92 100
91 169.4 137.3 205.9

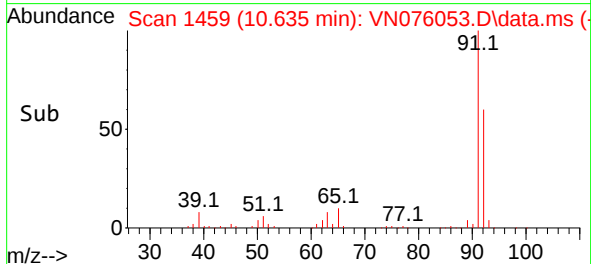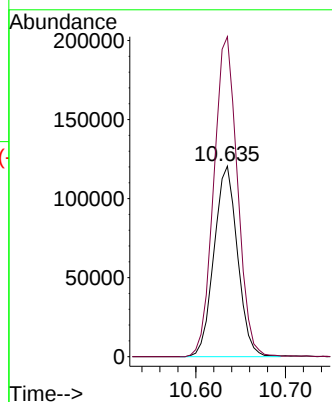

#53
t-1,3-Dichloropropene
Concen: 0.529 ug/l
RT: 10.629 min Scan# 1458
Delta R.T. -0.206 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 75 Resp: 2558
Ion Ratio Lower Upper
75 100
77 116.5 24.9 37.3#



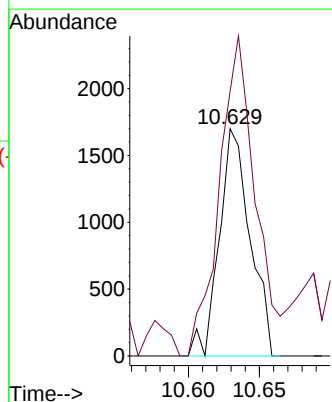





#55
 1,1,2-Trichloroethane
 Concen: 0.368 ug/l
 RT: 10.888 min Scan# 1511
 Delta R.T. -0.130 min
 Lab File: VN076053.D
 Acq: 29 Dec 2022 16:54




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-3DL


Tgt Ion: 97	Resp:	1311
Ion	Ratio	Lower Upper
97	100	
83	0.0	65.0 97.4#
85	0.0	43.0 64.6#
99	0.0	50.2 75.2#

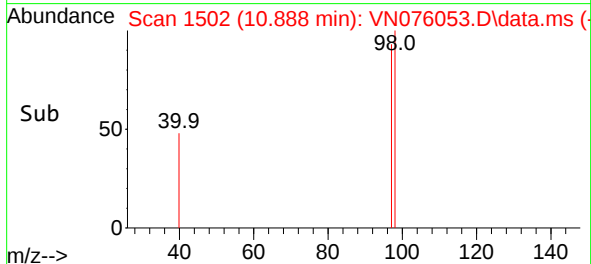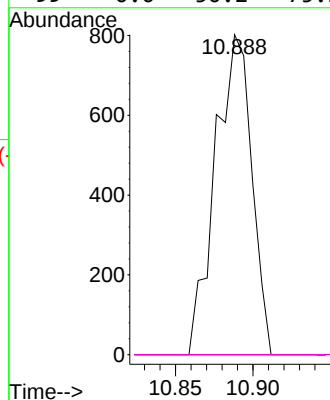

#59
 2-Hexanone
 Concen: 0.809 ug/l
 RT: 11.176 min Scan# 1551
 Delta R.T. -0.024 min
 Lab File: VN076053.D
 Acq: 29 Dec 2022 16:54

Tgt Ion: 43	Resp:	2137
Ion	Ratio	Lower Upper
43	100	
58	0.0	30.6 92.0#


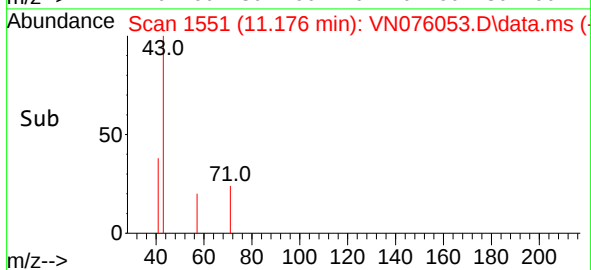
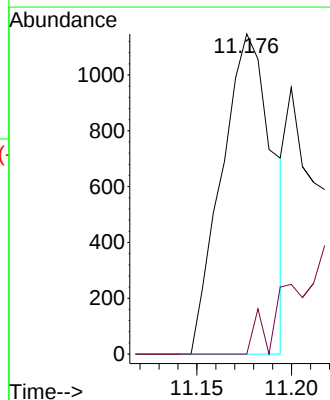





#62
4-Bromofluorobenzene
Concen: 47.172 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 95 Resp: 198797
Ion Ratio Lower Upper
95 100
174 87.6 0.0 171.6
176 85.6 0.0 169.2

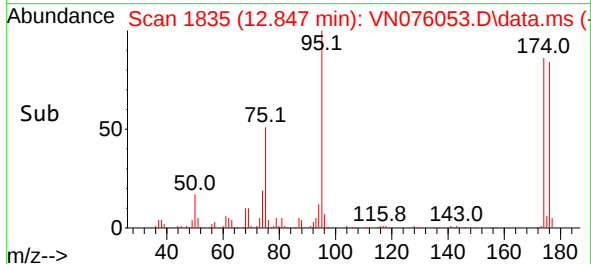

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 117 Resp: 474445
Ion Ratio Lower Upper
117 100
82 51.3 41.3 61.9
119 30.8 24.6 37.0


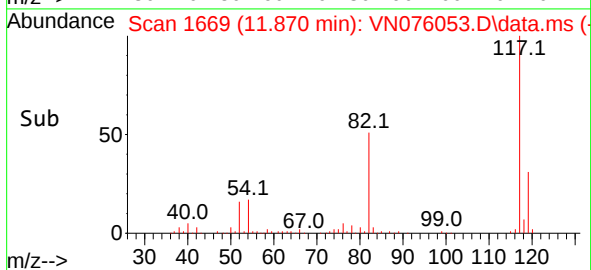




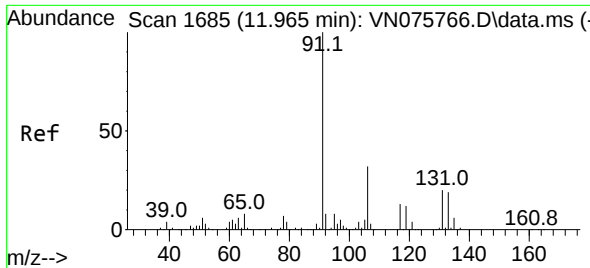

#67
Ethyl Benzene
Concen: 1.718 ug/l
RT: 11.970 min Scan# 1685
Delta R.T. 0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 91 Resp: 28242
Ion Ratio Lower Upper
91 100
106 27.7 25.7 38.5

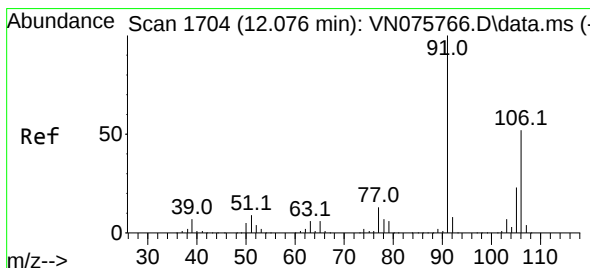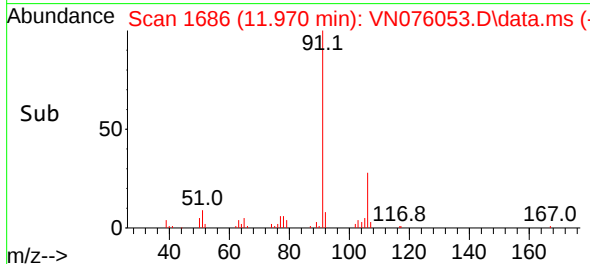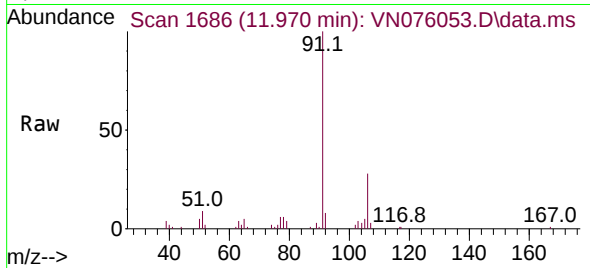

#68
m/p-Xylenes
Concen: 9.994 ug/l
RT: 12.070 min Scan# 1703
Delta R.T. -0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 106 Resp: 65008
Ion Ratio Lower Upper
106 100
91 195.7 156.6 235.0


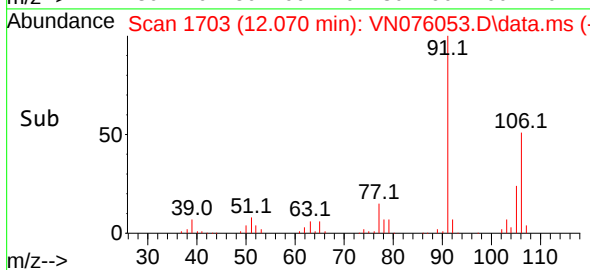

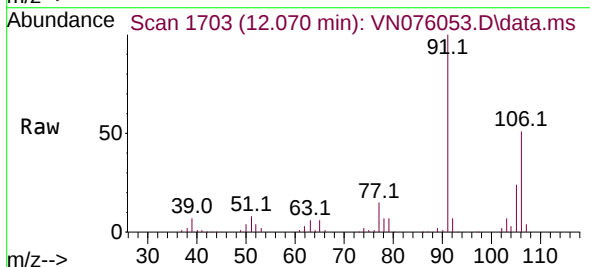




#69
o-Xylene
Concen: 9.123 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion:106 Resp: 58729
Ion Ratio Lower Upper
106 100
91 205.7 103.8 311.6

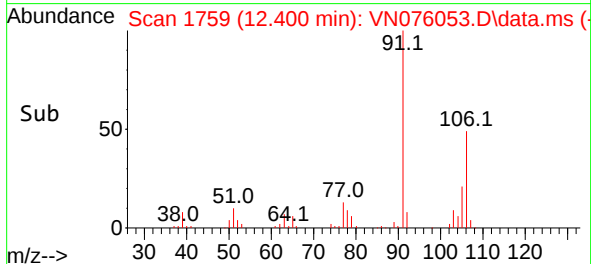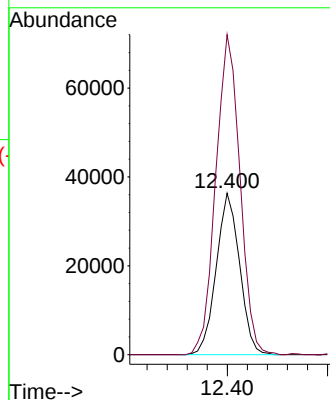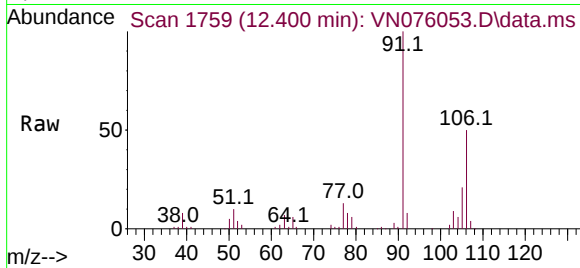

#70
Styrene
Concen: 1.384 ug/l
RT: 12.412 min Scan# 1761
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion:104 Resp: 14170
Ion Ratio Lower Upper
104 100
78 88.2 37.5 56.3#
103 97.0 43.5 65.3#

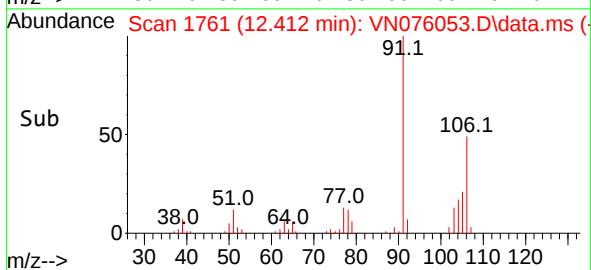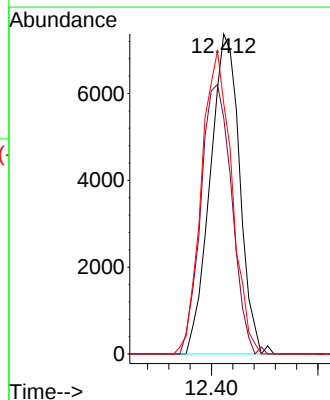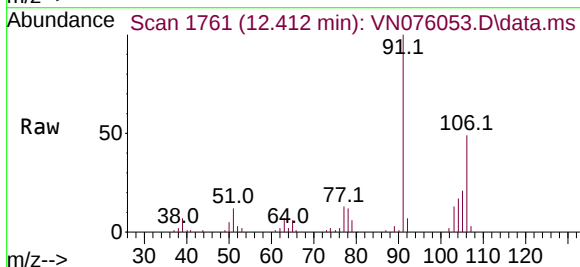



#71

Bromoform

Concen: 0.647 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.270 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54

Instrument :

MSVOA_N

ClientSampleId :

SB-3DL





Tgt Ion:173 Resp: 1698

Ion Ratio Lower Upper

173 100

175 629.4 24.3 72.8#

254 0.0 0.0 0.0

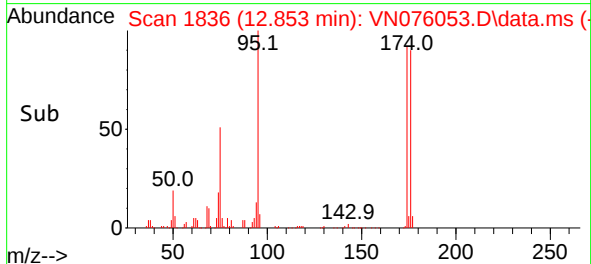

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. -0.000 min

Lab File: VN076053.D

Acq: 29 Dec 2022 16:54




Tgt Ion:152 Resp: 209951


Ion Ratio Lower Upper

152 100

115 58.1 29.1 87.4

150 154.6 0.0 347.0




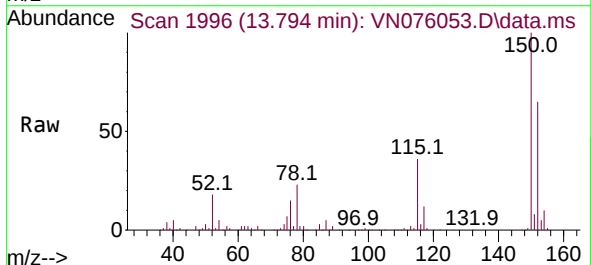




#76
1,2,3-Trichloropropane
Concen: 23.505 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. -0.147 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 75 Resp: 99475
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

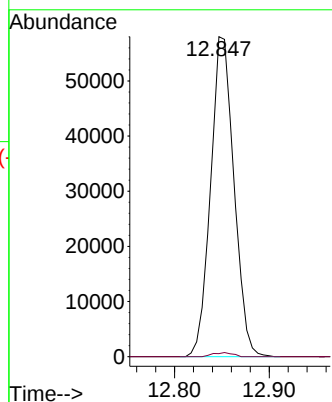

#78
n-propylbenzene
Concen: 0.240 ug/l
RT: 13.041 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 91 Resp: 4022
Ion Ratio Lower Upper
91 100
120 15.4 12.0 36.1


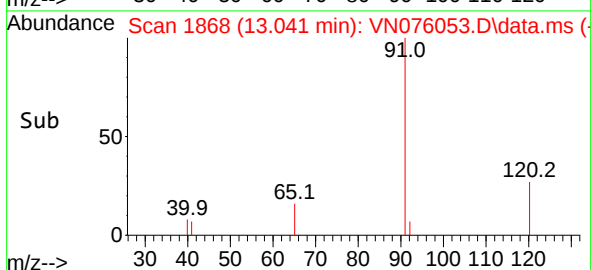

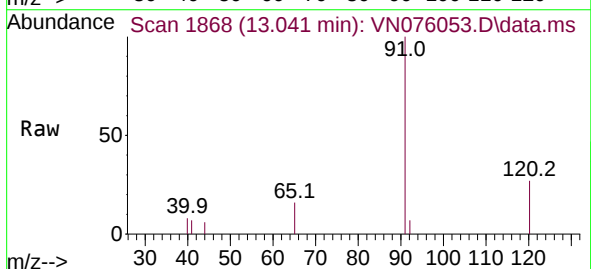




#79
2-Chlorotoluene
Concen: 0.226 ug/l
RT: 13.094 min Scan# 1877
Delta R.T. -0.035 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 91 Resp: 2359
Ion Ratio Lower Upper
91 100
126 0.0 17.5 52.5#

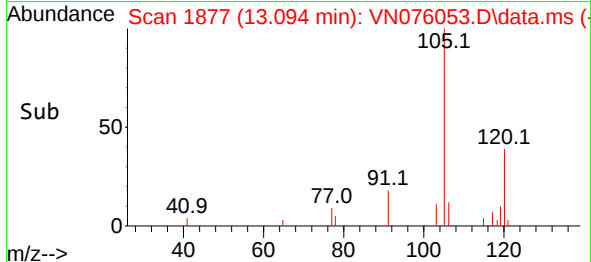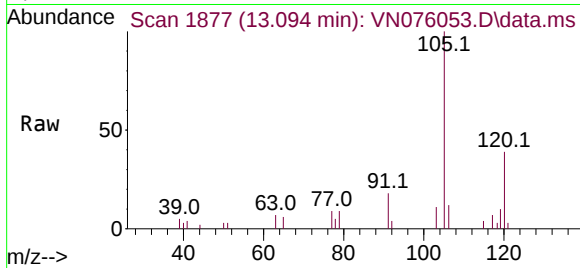

#80
1,3,5-Trimethylbenzene
Concen: 1.044 ug/l
RT: 13.176 min Scan# 1891
Delta R.T. -0.000 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 105 Resp: 13257
Ion Ratio Lower Upper
105 100
120 60.2 24.7 74.1




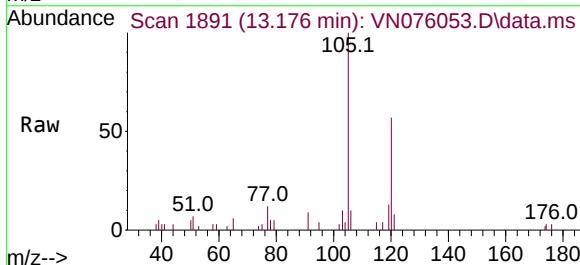




#81
trans-1,4-Dichloro-2-butene
Concen: 84.606 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.106 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion: 75 Resp: 99475
Ion Ratio Lower Upper
75 100
53 0.0 73.8 110.6#
89 0.0 39.5 59.3#

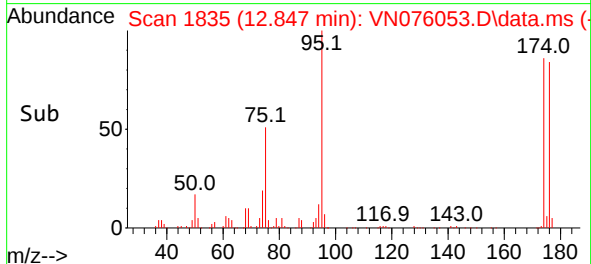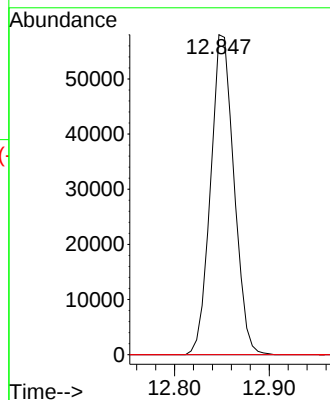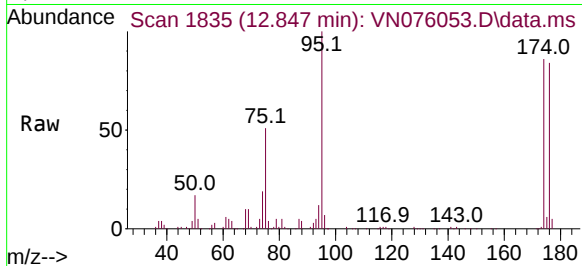

#82
4-Chlorotoluene
Concen: 0.226 ug/l
RT: 13.094 min Scan# 1877
Delta R.T. -0.035 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion: 91 Resp: 2359
Ion Ratio Lower Upper
91 100
126 0.0 17.5 52.5#



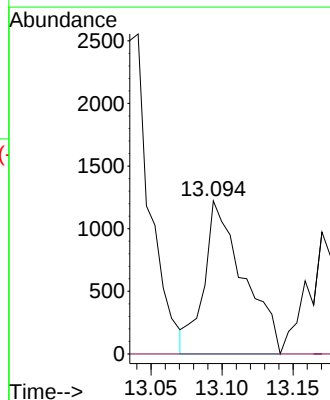
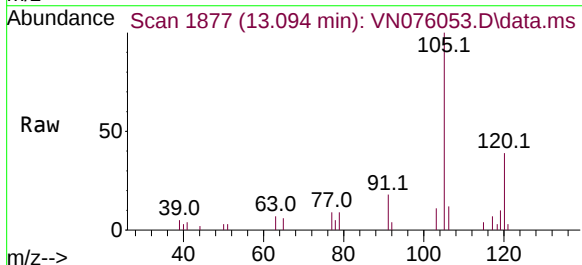




#83
tert-Butylbenzene
Concen: 0.537 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. 0.047 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54




Instrument :
MSVOA_N
ClientSampleId :
SB-3DL


Tgt Ion:119 Resp: 6017
Ion Ratio Lower Upper
119 100
91 81.8 31.9 95.5
134 0.0 13.8 41.4#

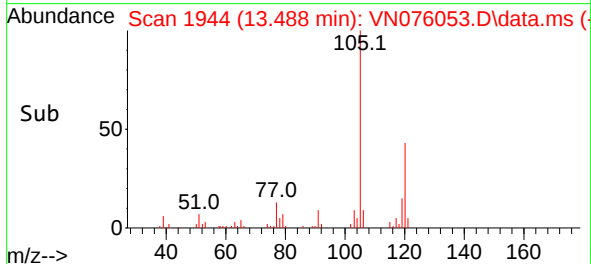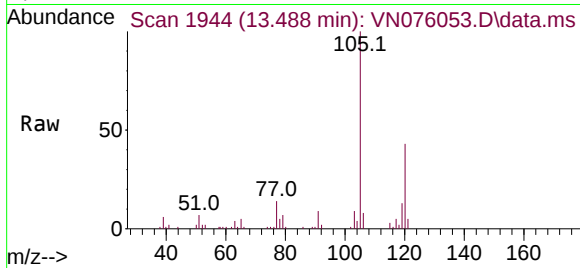

#84
1,2,4-Trimethylbenzene
Concen: 3.406 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. 0.006 min
Lab File: VN076053.D
Acq: 29 Dec 2022 16:54

Tgt Ion:105 Resp: 42911
Ion Ratio Lower Upper
105 100
120 45.9 23.3 69.8


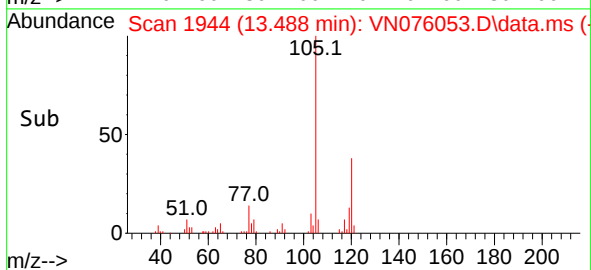

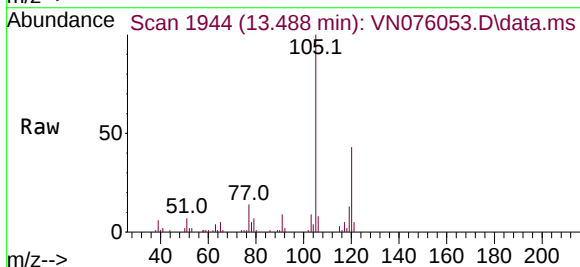




#85
 sec-Butylbenzene
 Concen: 2.777 ug/l
 RT: 13.488 min Scan# 1966
 Delta R.T. -0.130 min
 Lab File: VN076053.D
 Acq: 29 Dec 2022 16:54

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-3DL

Tgt Ion:105 Resp: 42911
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.1 30.1#

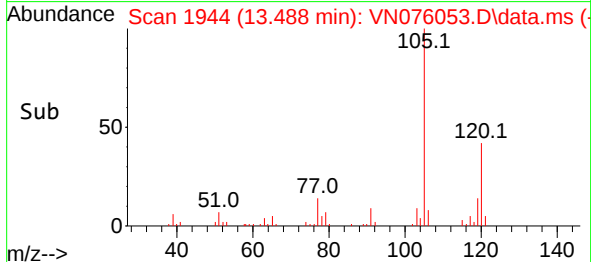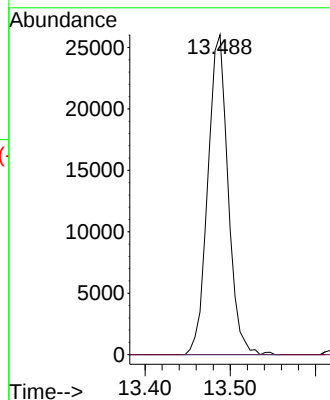

#95
 Naphthalene
 Concen: 19.078 ug/l
 RT: 15.647 min Scan# 2311
 Delta R.T. 0.006 min
 Lab File: VN076053.D
 Acq: 29 Dec 2022 16:54

Tgt Ion:128 Resp: 201899
 Ion Ratio Lower Upper
 128 100
 127 13.1 10.4 15.6
 129 10.8 8.7 13.1

