
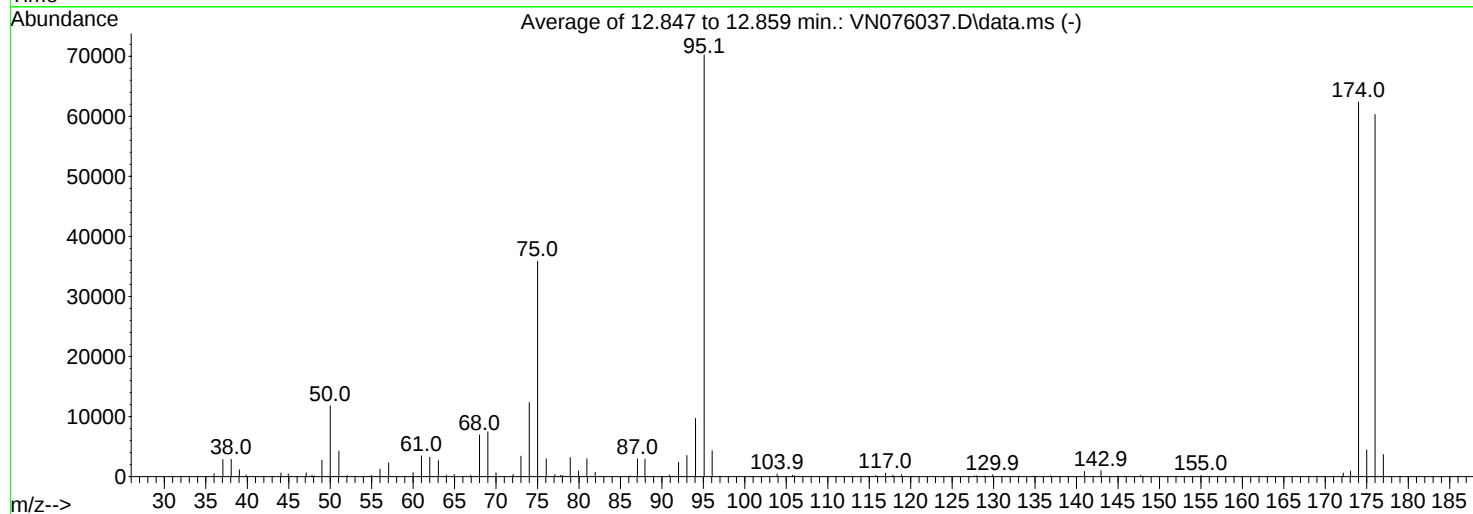


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122922\
 Data File : VN076037.D
 Acq On : 29 Dec 2022 09:01
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

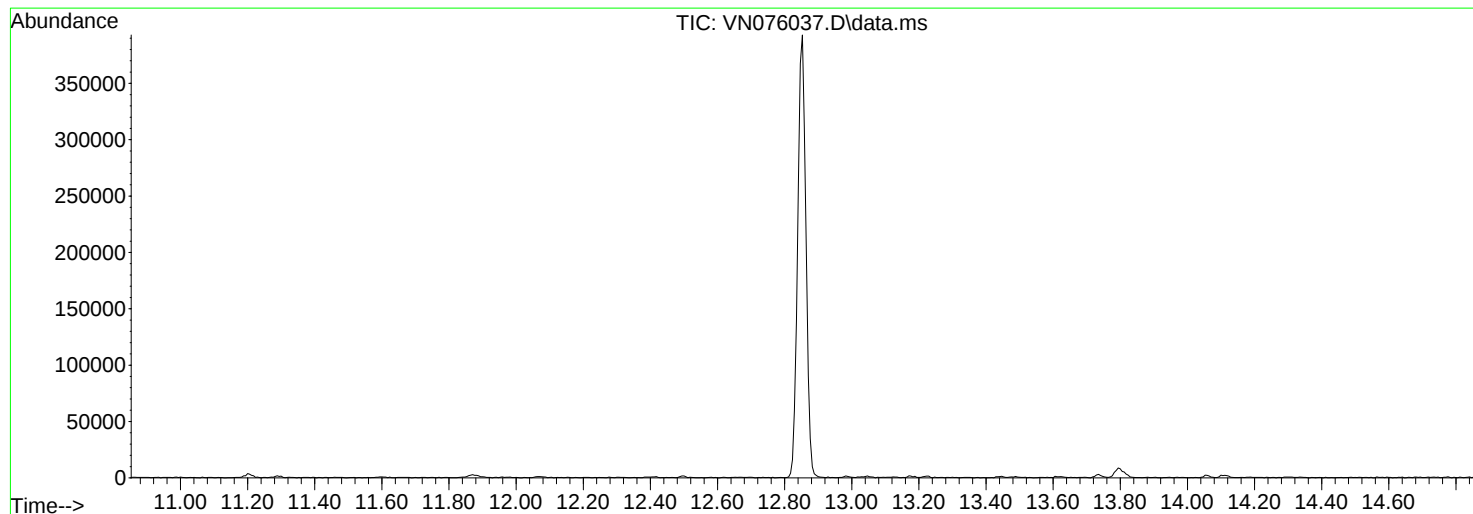

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	11796	PASS
75	95	30	60	51.1	35877	PASS
95	95	100	100	100.0	70243	PASS
96	95	5	9	6.1	4315	PASS
173	174	0.00	2	1.4	904	PASS
174	95	50	100	88.8	62389	PASS
175	174	5	9	7.1	4445	PASS
176	174	95	101	96.7	60307	PASS
177	176	5	9	6.1	3680	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	516	50.00	11796	64.95	376	77.80	23
37.05	2840	51.05	4224	66.95	208	78.05	18
38.05	2880	52.05	200	68.00	6931	78.95	317
39.05	1151	54.95	211	69.00	7463	79.95	92
39.85	256	56.00	1258	70.00	655	80.95	2999
44.05	616	57.05	2304	72.05	385	81.95	718
44.95	466	60.00	700	73.00	3401	86.15	146
47.10	650	61.00	3478	74.00	12343	87.05	2991
47.80	253	62.00	3234	75.00	35877	87.95	2914
48.10	97	63.05	2659	76.05	2975	90.90	261
49.00	2741	64.00	272	77.10	346	92.00	2394

Average of 12.847 to 12.859 min.: VN076037.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	3513	116.95	596	142.95	1008	174.00	62389
94.05	9713	117.85	253	144.90	75	175.00	4445
95.10	70243	118.90	344	145.10	71	176.00	60307
96.05	4315	127.70	101	145.80	59	177.00	3680
96.90	61	127.95	170	147.75	216	177.90	62
103.90	392	128.90	106	149.80	57		
105.75	242	129.90	325	150.00	67		
106.00	159	130.90	52	155.00	220		
114.90	62	134.85	122	157.20	86		
115.80	211	136.90	166	172.15	626		
116.00	69	140.95	849	173.05	904		

Instrument :

MSVOA_N

ClientSampleId :

BFB