
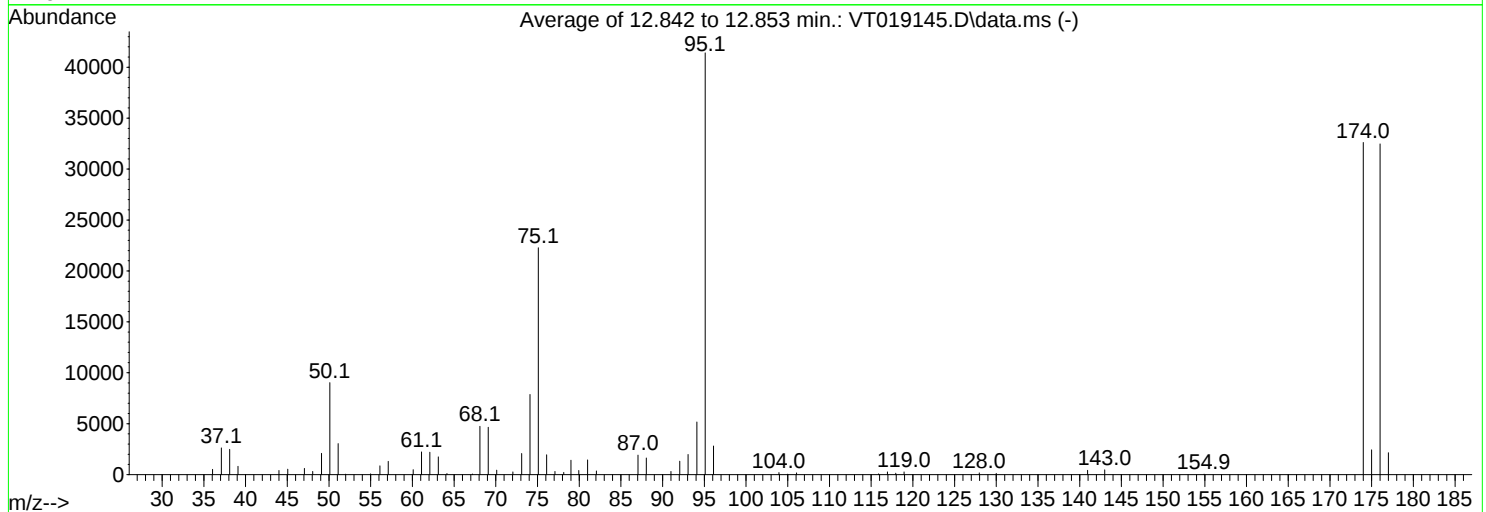


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT100325\
Data File : VT019145.D
Acq On : 3 Oct 2025 13:47
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_T/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\82T100325W.M
Title : SW846 8260
Last Update : Sat Oct 04 01:46:12 2025

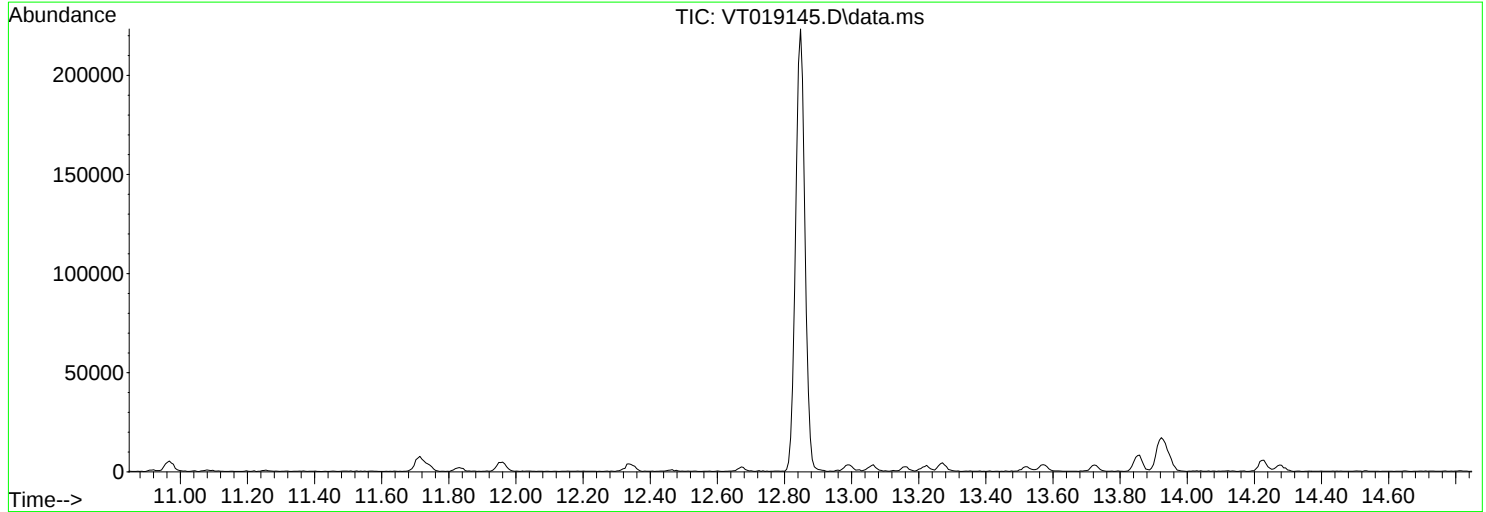

AutoFind: Scans 1931, 1932, 1933; Background Corrected with Scan 1922

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	9040	PASS
75	95	30	60	53.8	22280	PASS
95	95	100	100	100.0	41411	PASS
96	95	5	9	6.8	2811	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.8	32613	PASS
175	174	5	9	7.5	2433	PASS
176	174	95	101	99.6	32472	PASS
177	176	5	9	6.6	2158	PASS