
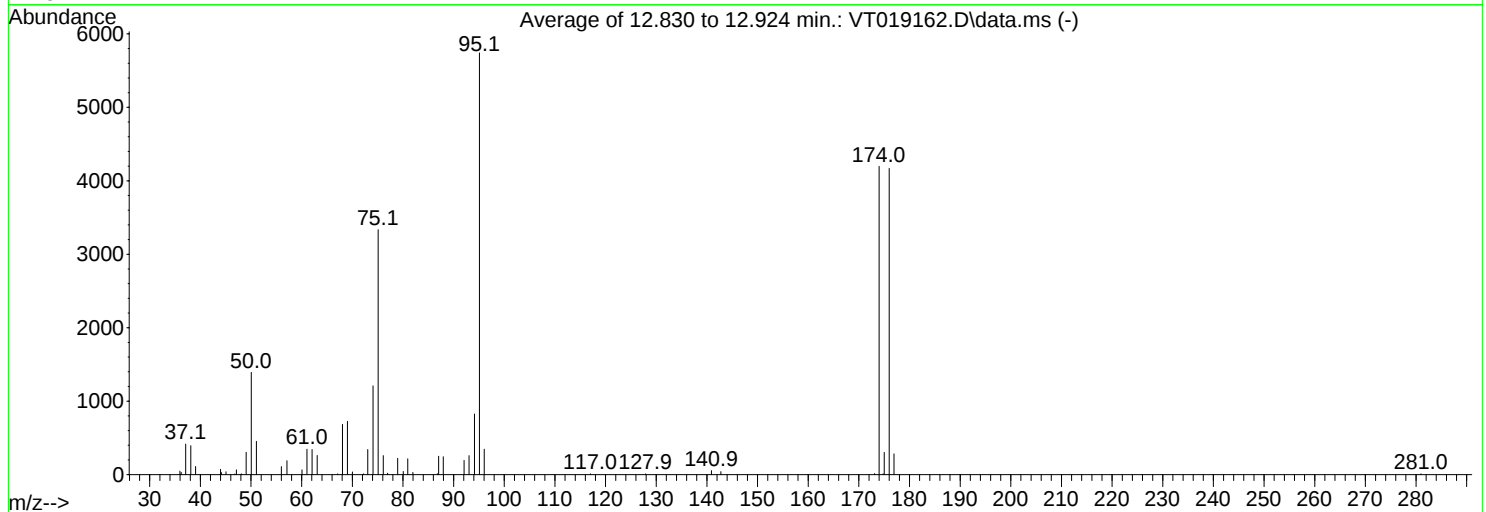


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT102325\
Data File : VT019162.D
Acq On : 23 Oct 2025 8:48
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_T/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\624T102225W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 24 06:05:07 2025

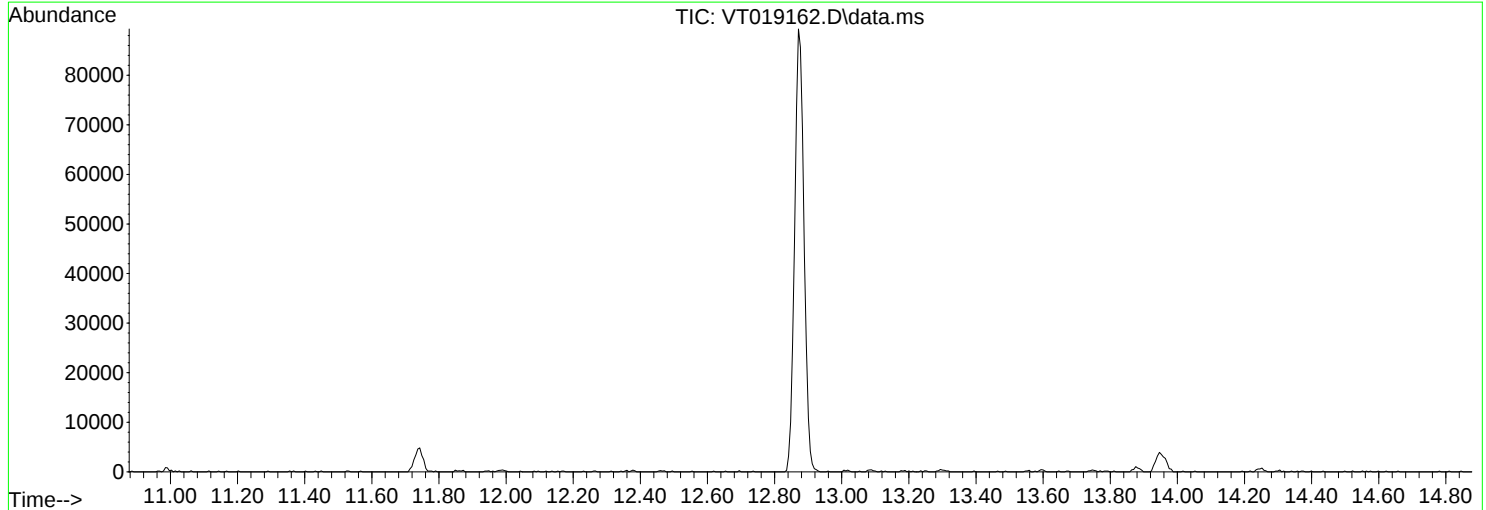

AutoFind: Averaged scan 1929 to 1945; Bkg corrected with scan 1928

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	1391	PASS
75	95	30	60	58.1	3335	PASS
95	95	100	100	100.0	5742	PASS
96	95	5	9	6.0	346	PASS
173	174	0.00	2	0.4	16	PASS
174	95	50	100	73.1	4197	PASS
175	174	5	9	7.2	303	PASS
176	174	95	101	99.3	4169	PASS
177	176	5	9	6.8	284	PASS