


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT102725\
Data File : VT019182.D
Acq On : 27 Oct 2025 6:57
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_T/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\624T102225W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 24 06:05:07 2025

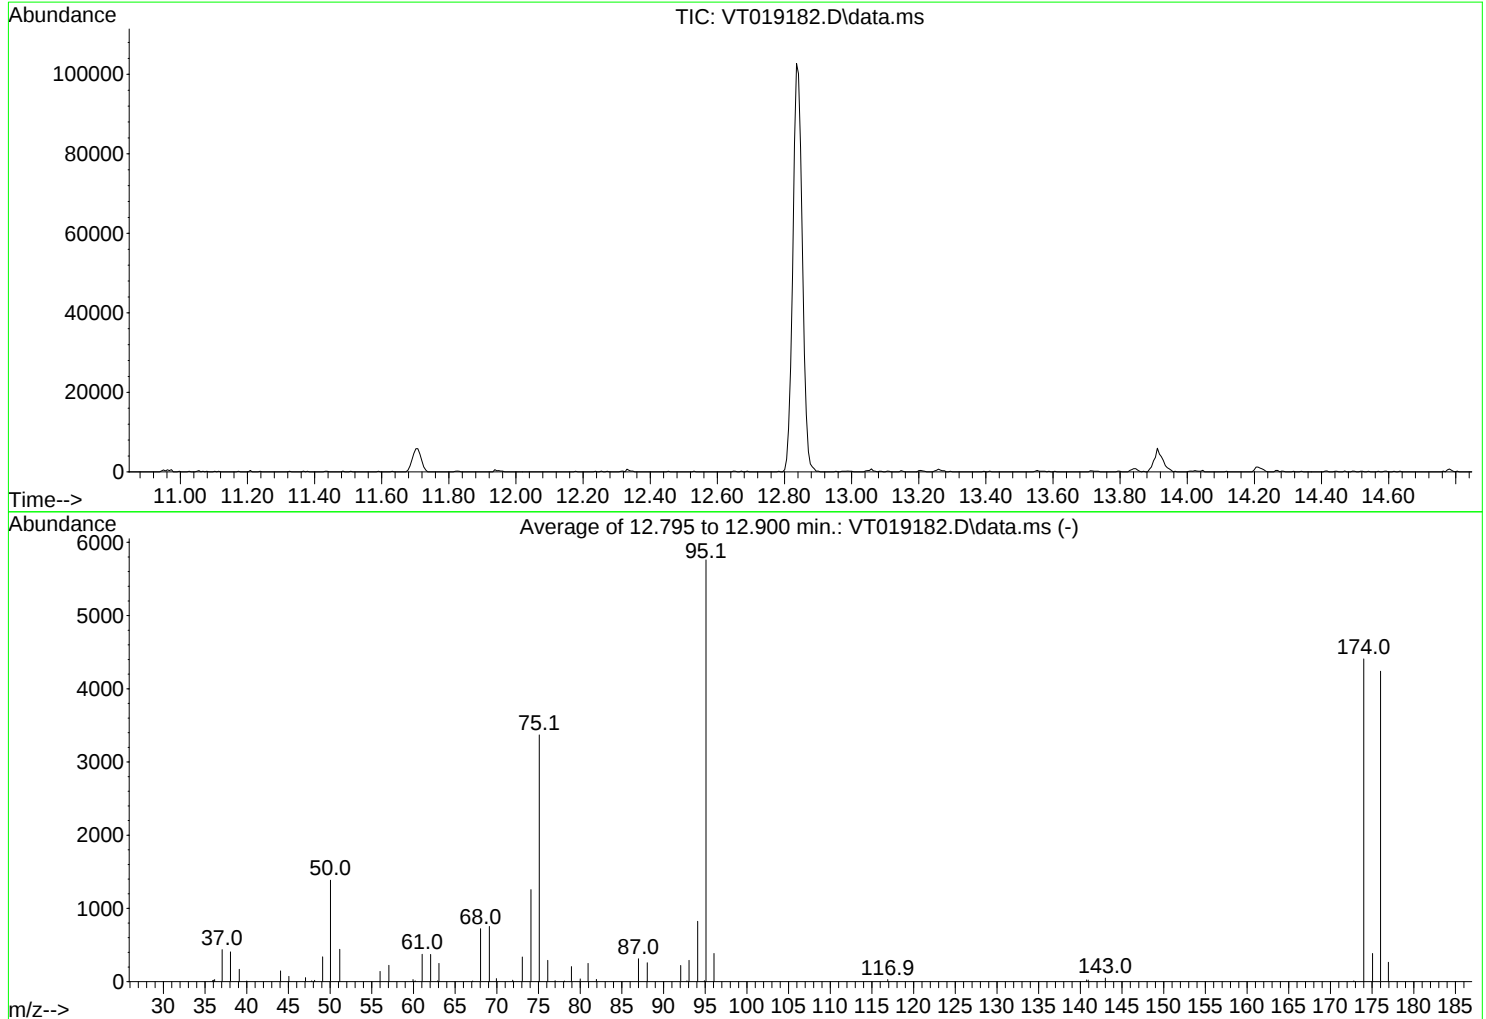

AutoFind: Averaged scan 1923 to 1941; Bkg corrected with scan 1922

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.1	1386	PASS
75	95	30	60	58.5	3370	PASS
95	95	100	100	100.0	5761	PASS
96	95	5	9	6.7	384	PASS
173	174	0.00	2	0.2	10	PASS
174	95	50	100	76.5	4408	PASS
175	174	5	9	8.7	384	PASS
176	174	95	101	96.2	4239	PASS
177	176	5	9	6.2	264	PASS