
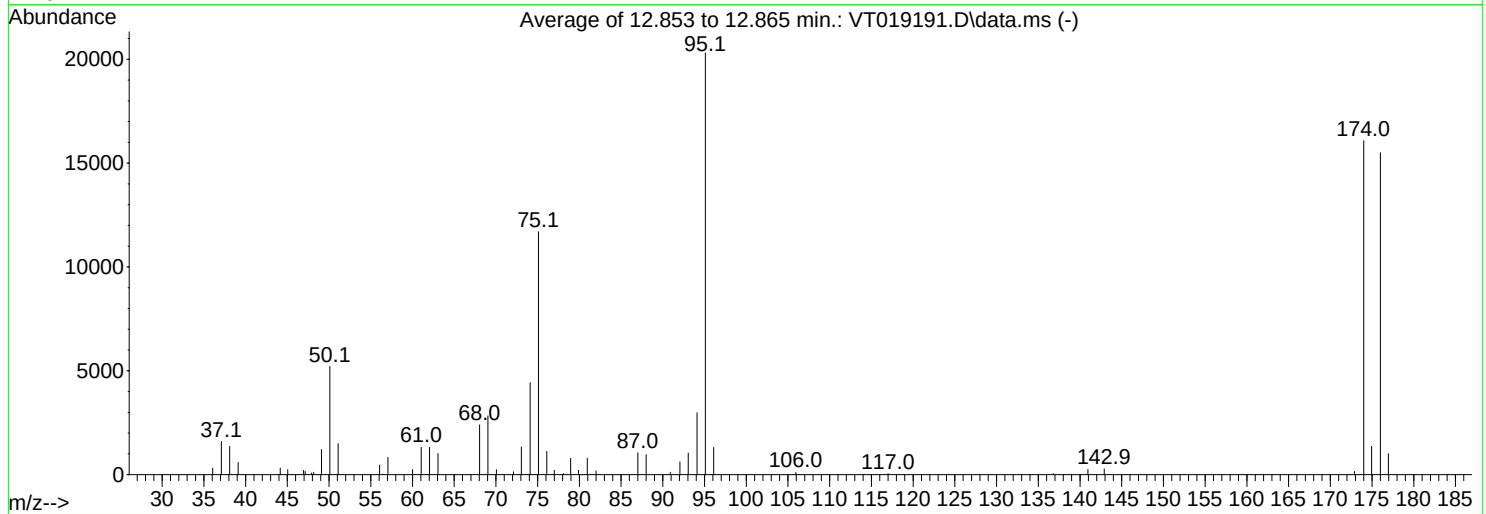


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT102925\
Data File : VT019191.D
Acq On : 29 Oct 2025 8:20
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_T/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\82T102925W.M
Title : SW846 8260
Last Update : Fri Oct 31 04:36:59 2025

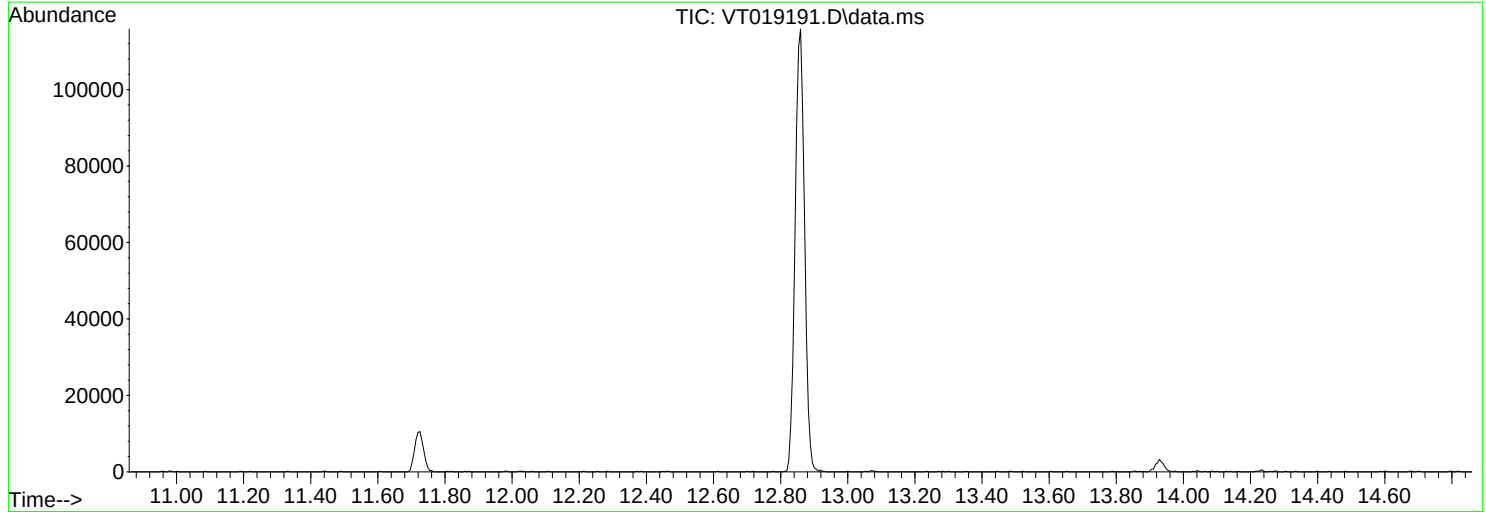

AutoFind: Scans 1933, 1934, 1935; Background Corrected with Scan 1924

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.7	5212	PASS
75	95	30	60	57.6	11693	PASS
95	95	100	100	100.0	20309	PASS
96	95	5	9	6.4	1308	PASS
173	174	0.00	2	0.9	150	PASS
174	95	50	100	79.2	16076	PASS
175	174	5	9	8.5	1360	PASS
176	174	95	101	96.4	15500	PASS
177	176	5	9	6.5	1013	PASS