
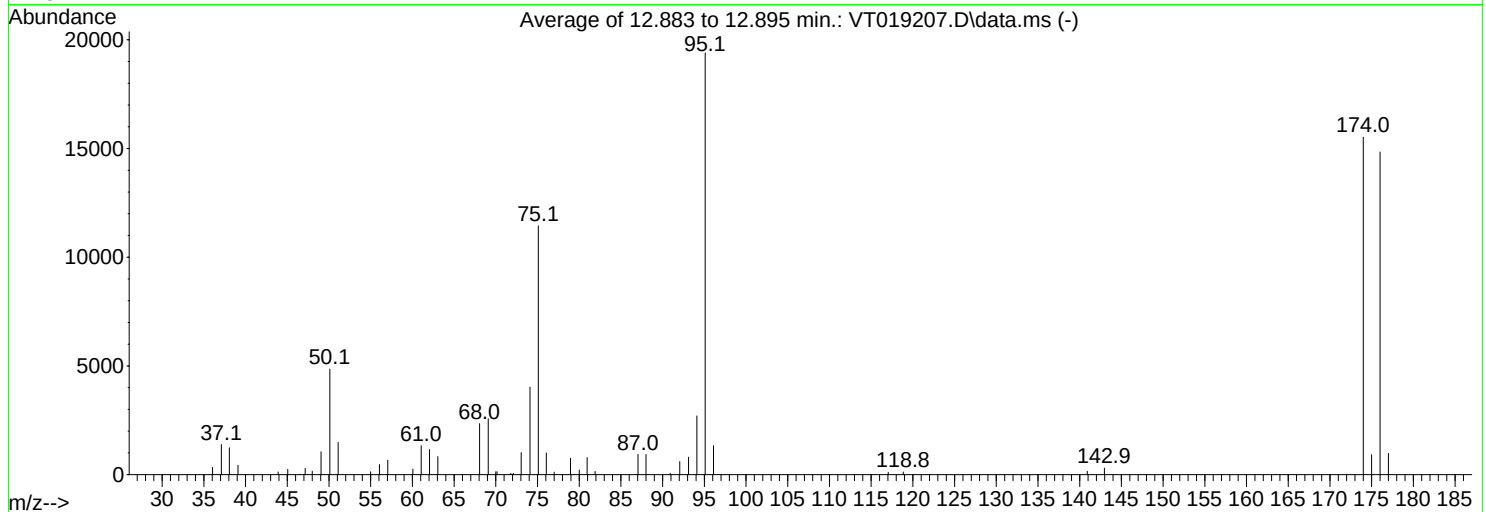


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT103025\
Data File : VT019207.D
Acq On : 30 Oct 2025 9:50
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_T/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\82T102925W.M
Title : SW846 8260
Last Update : Fri Oct 31 04:36:59 2025

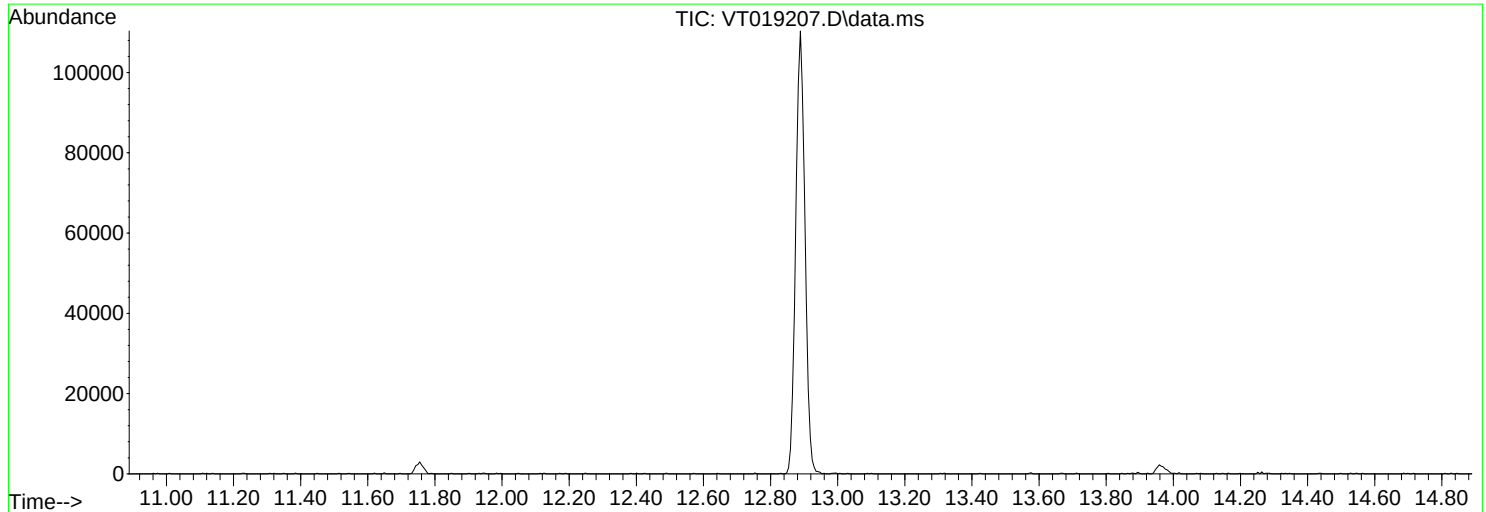

AutoFind: Scans 1938, 1939, 1940; Background Corrected with Scan 1929

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	4857	PASS
75	95	30	60	59.0	11445	PASS
95	95	100	100	100.0	19400	PASS
96	95	5	9	6.9	1330	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.0	15517	PASS
175	174	5	9	5.9	919	PASS
176	174	95	101	95.7	14846	PASS
177	176	5	9	6.6	978	PASS