


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT103125\
Data File : VT019218.D
Acq On : 31 Oct 2025 7:43
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_T/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\82T102925W.M
Title : SW846 8260
Last Update : Fri Oct 31 04:36:59 2025

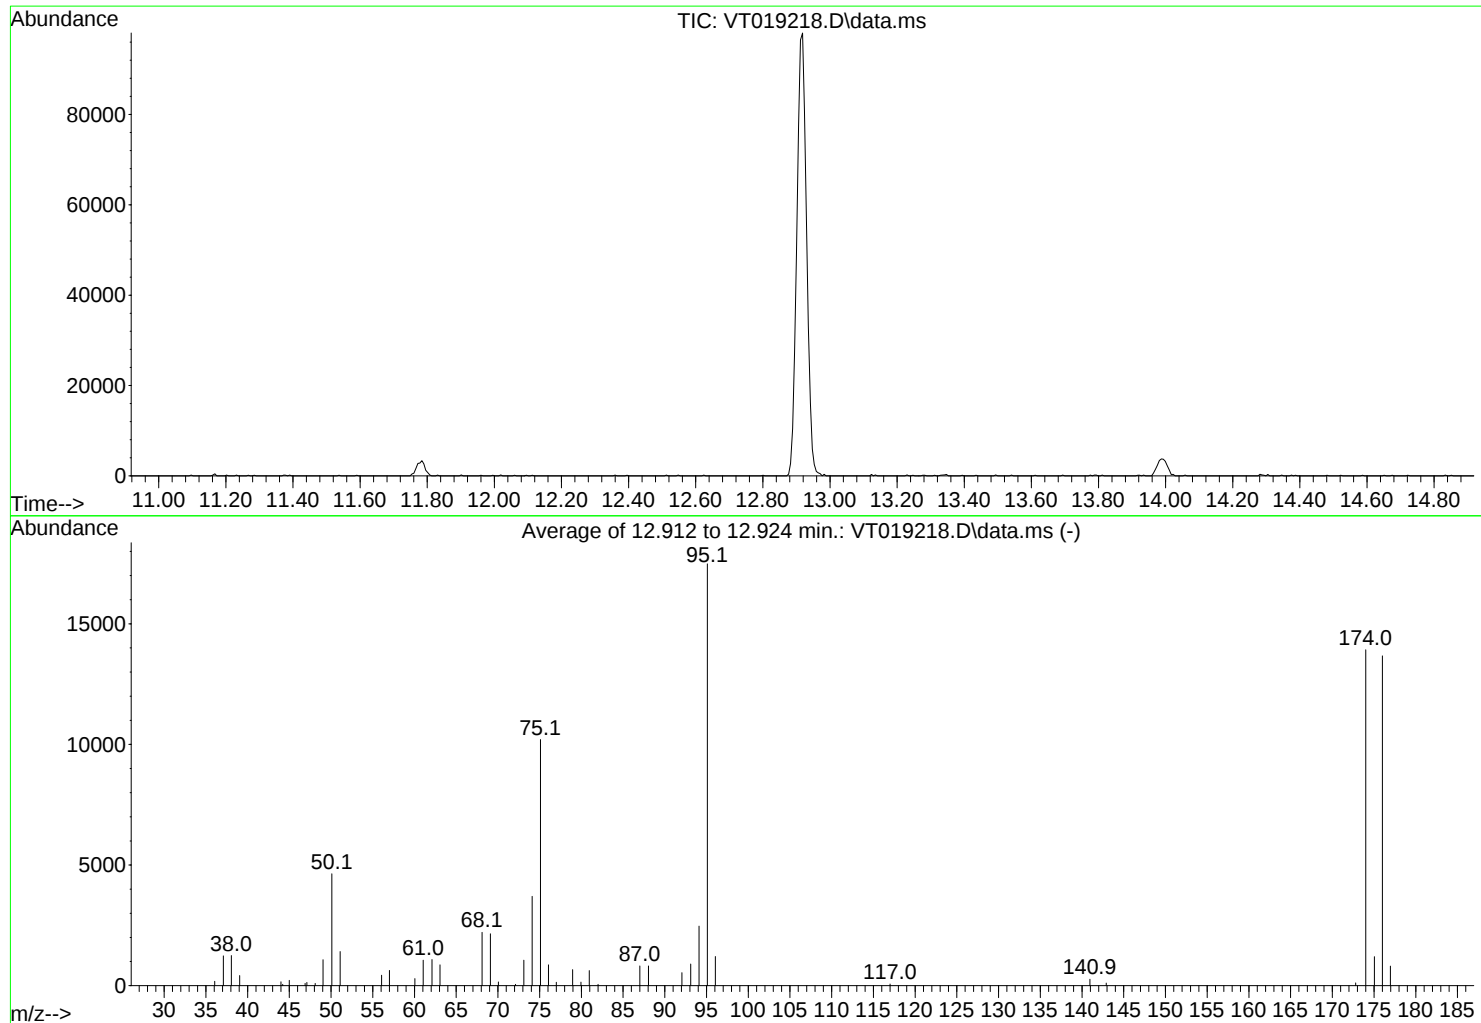

AutoFind: Scans 1943, 1944, 1945; Background Corrected with Scan 1934

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.5	4638	PASS
75	95	30	60	58.3	10199	PASS
95	95	100	100	100.0	17487	PASS
96	95	5	9	6.9	1206	PASS
173	174	0.00	2	0.8	110	PASS
174	95	50	100	79.6	13922	PASS
175	174	5	9	8.6	1199	PASS
176	174	95	101	98.2	13673	PASS
177	176	5	9	5.9	809	PASS