


Data Path : Z:\voasrv\HPCHEM1\MSVOA T\Data\VT112818\
 Data File : VT019099.D
 Acq On : 28 Nov 2018 9:41
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA T/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_T
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_T\METHODS\82T112818TCLP.M
 Title : SW846 8260
 Last Update : Thu Nov 29 06:21:27 2018

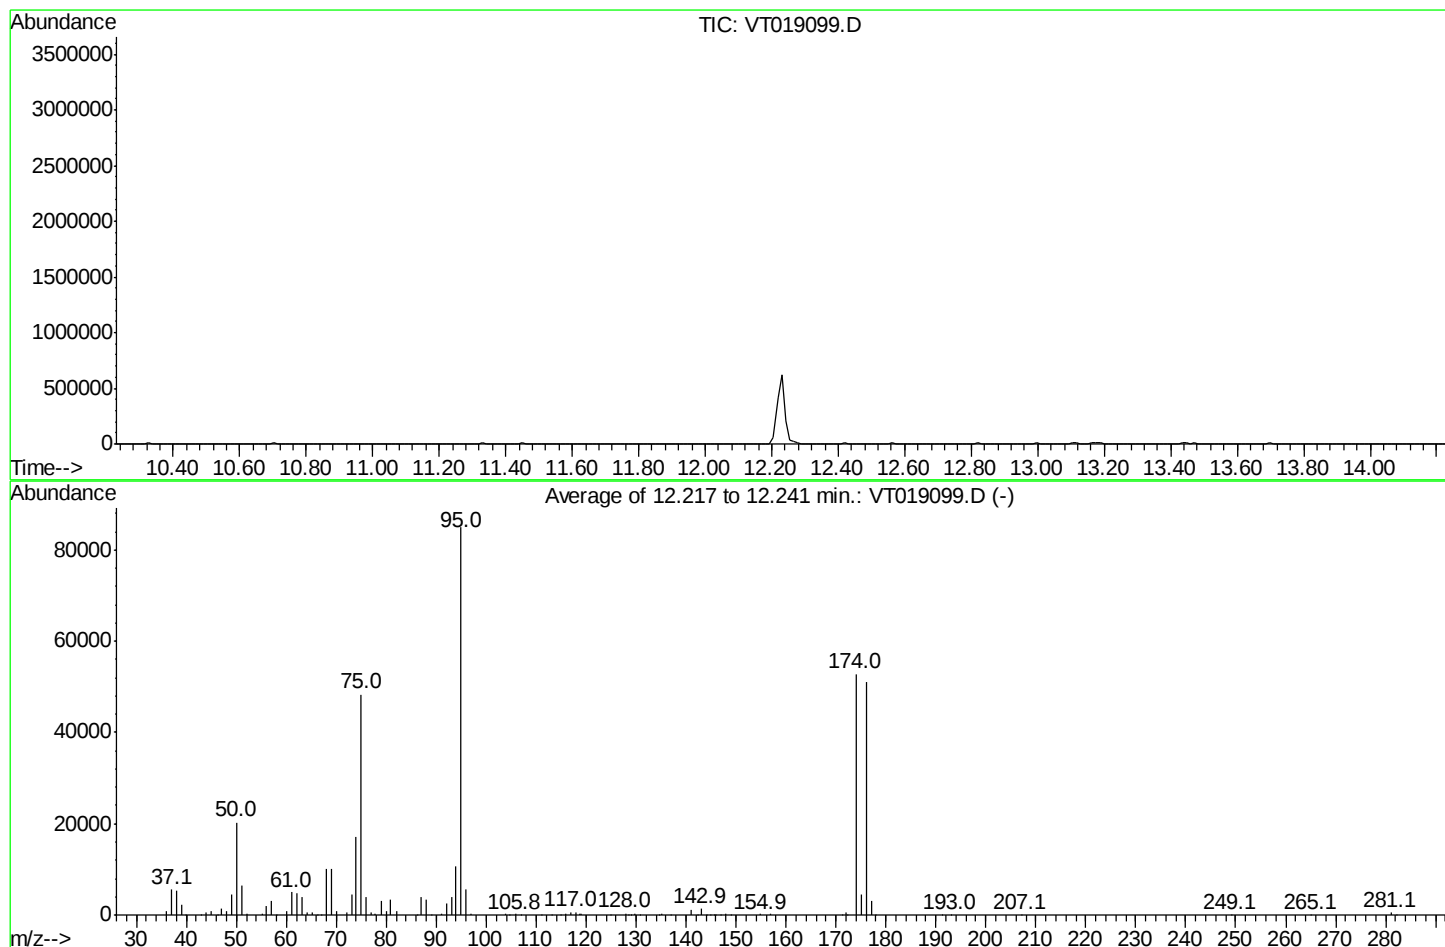

AutoFind: Scans 908, 909, 910; Background Corrected with Scan 903

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	20249	PASS
75	95	30	60	56.9	48389	PASS
95	95	100	100	100.0	84973	PASS
96	95	5	9	6.7	5676	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	62.1	52800	PASS
175	174	5	9	8.7	4585	PASS
176	174	95	101	96.5	50976	PASS
177	176	5	9	6.1	3123	PASS