
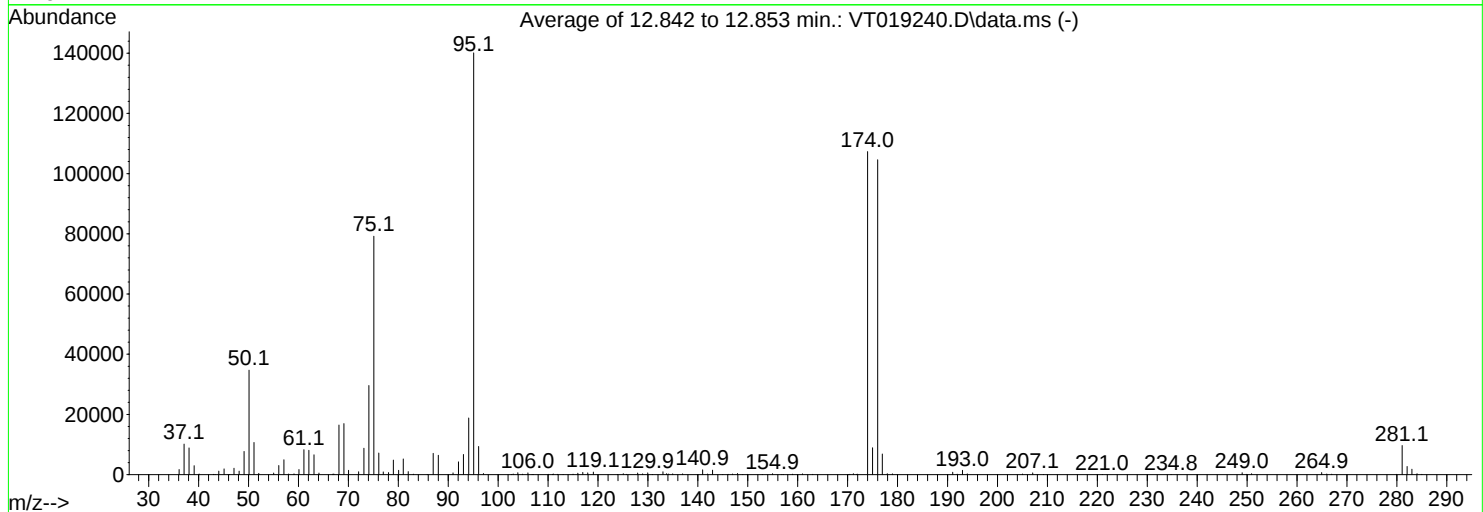


Data Path : Z:\voasrv\HPCHEM1\MSVOA_T\Data\VT120825\
Data File : VT019240.D
Acq On : 8 Dec 2025 8:56
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_T/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_T\methods\82T120825S.M
Title : SW846 8260
Last Update : Tue Dec 09 01:13:34 2025

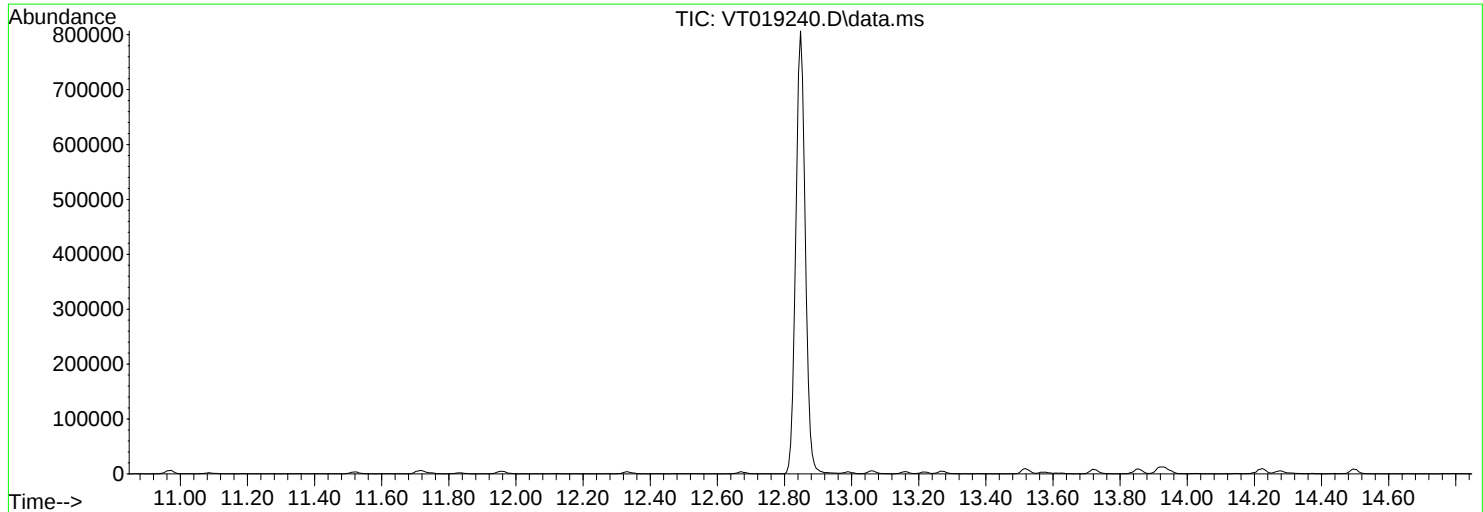

AutoFind: Scans 1931, 1932, 1933; Background Corrected with Scan 1922

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	34733	PASS
75	95	30	60	56.5	79192	PASS
95	95	100	100	100.0	140117	PASS
96	95	5	9	6.7	9382	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.6	107317	PASS
175	174	5	9	8.3	8928	PASS
176	174	95	101	97.5	104597	PASS
177	176	5	9	6.6	6876	PASS