


Data Path : W:\HPCHEM1\MSVOA T\DATA\VT050818\
Data File : VT019039.D
Acq On : 8 May 2018 15:46
Operator : SY/MD
Sample : BFB
Misc : 5.00µg/10mL/MSVOA T/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_T\METHODS\2015\82T050818S.M
Title : SW846 8260
Last Update : Wed May 09 04:36:54 2018

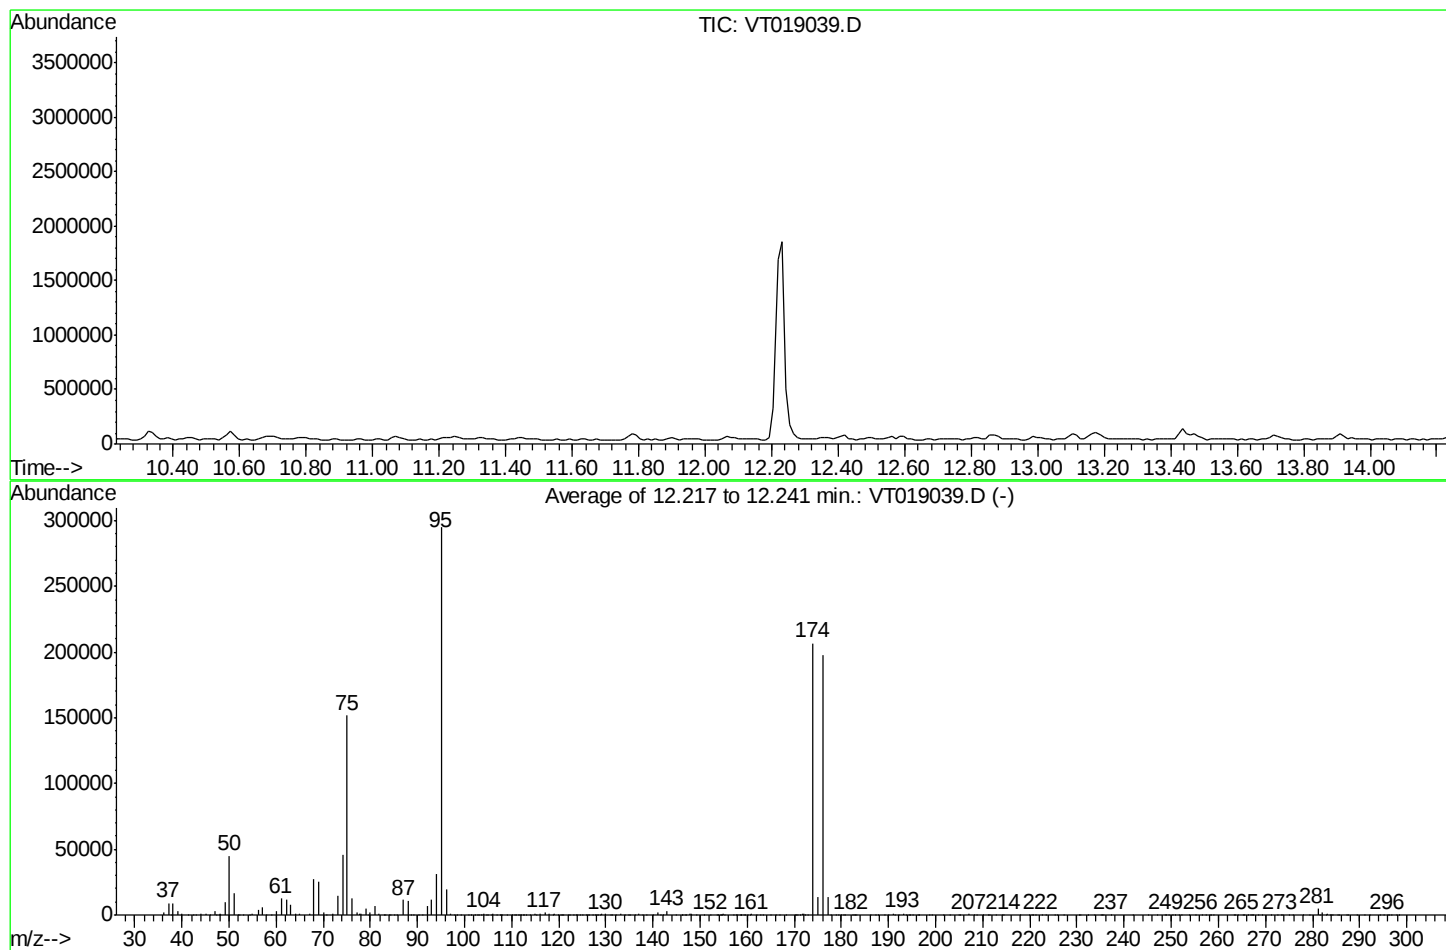

AutoFind: Scans 908, 909, 910; Background Corrected with Scan 903

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	45180	PASS
75	95	30	60	51.4	151631	PASS
95	95	100	100	100.0	294853	PASS
96	95	5	9	6.7	19627	PASS
173	174	0.00	2	0.1	297	PASS
174	95	50	100	70.0	206448	PASS
175	174	5	9	6.4	13186	PASS
176	174	95	101	95.9	197994	PASS
177	176	5	9	7.1	14124	PASS