


Data Path : W:\HPCHEM1\MSVOA T\Data\VT050918\
Data File : VT019048.D
Acq On : 9 May 2018 9:30
Operator : SY/MD
Sample : BFB
Misc : 5.00µ/5mL/MSVOA T/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_T\METHODS\2015\82T050818S.M
Title : SW846 8260
Last Update : Thu May 10 07:01:04 2018

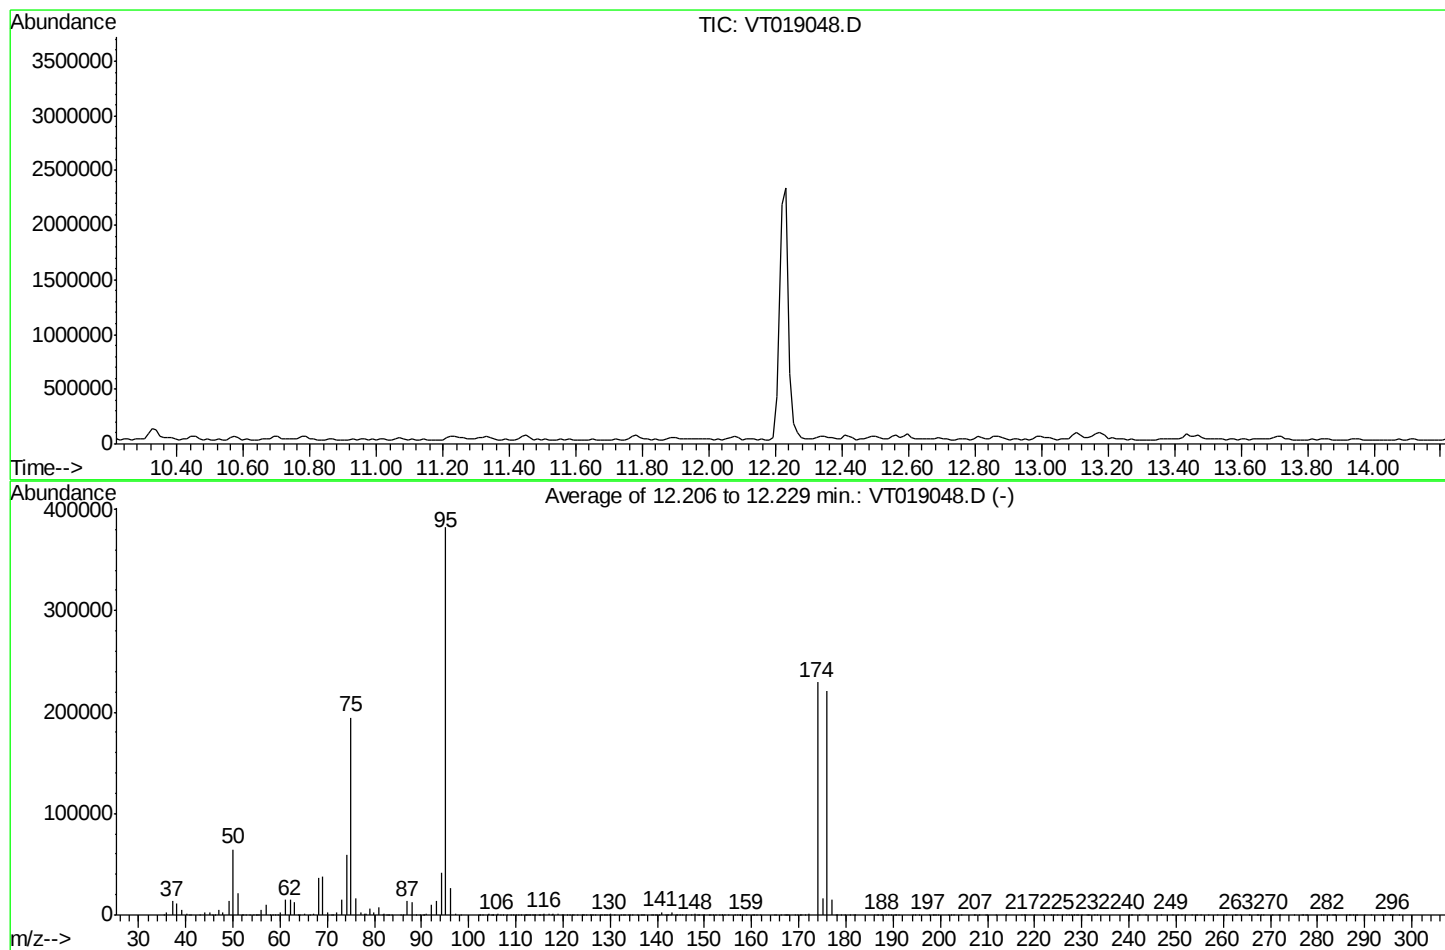

AutoFind: Scans 907, 908, 909; Background Corrected with Scan 903

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	64465	PASS
75	95	30	60	50.9	194440	PASS
95	95	100	100	100.0	382170	PASS
96	95	5	9	6.8	25958	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	60.1	229570	PASS
175	174	5	9	7.1	16357	PASS
176	174	95	101	96.4	221338	PASS
177	176	5	9	6.9	15261	PASS