


Data Path : W:\HPCHEM1\MSVOA T\Data\VT051018\
Data File : VT019066.D
Acq On : 10 May 2018 8:48
Operator : SY/MD
Sample : BFB
Misc : 6.83g/5mL/MSVOA T/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_T
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_T\METHODS\2015\82T050818S.M
Title : SW846 8260
Last Update : Thu May 10 07:01:04 2018

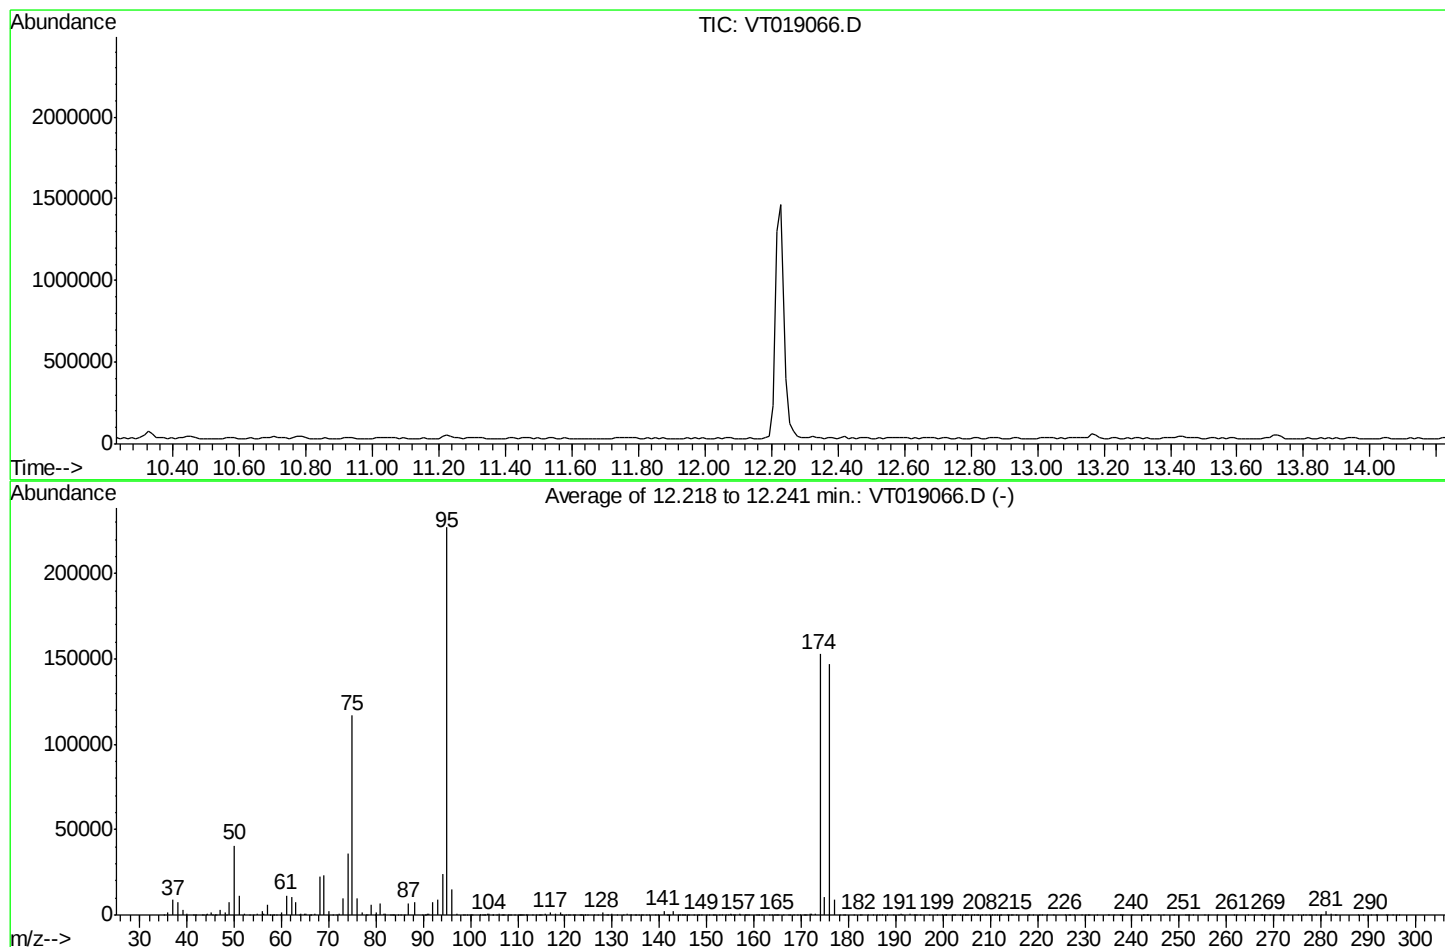

AutoFind: Scans 908, 909, 910; Background Corrected with Scan 904

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	40855	PASS
75	95	30	60	51.5	116953	PASS
95	95	100	100	100.0	227240	PASS
96	95	5	9	6.7	15284	PASS
173	174	0.00	2	0.4	592	PASS
174	95	50	100	67.3	152994	PASS
175	174	5	9	7.0	10668	PASS
176	174	95	101	96.0	146949	PASS
177	176	5	9	6.2	9166	PASS