


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU011119\
Data File : VU029130.D
Acq On : 11 Jan 2019 08:34
Operator : MD/SY
Sample : BFB70
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB70

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jan 11 23:23:56 2019

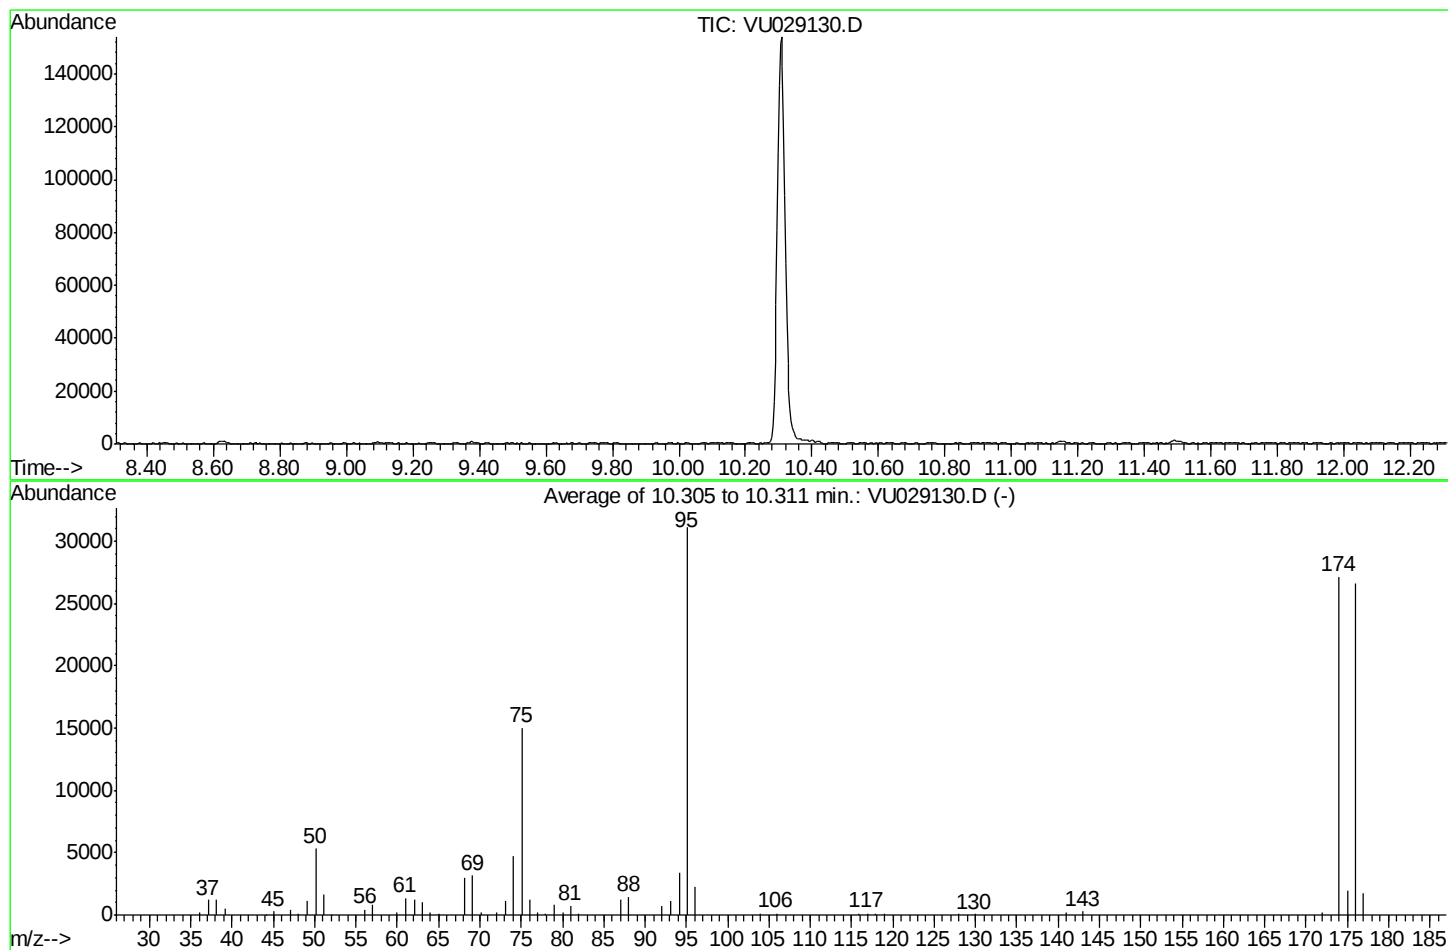

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5333	PASS
75	95	30	80	48.4	15044	PASS
95	95	100	100	100.0	31114	PASS
96	95	5	9	7.4	2294	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.3	27170	PASS
175	174	5	9	7.1	1920	PASS
176	174	95	101	98.0	26637	PASS
177	176	5	9	6.6	1747	PASS

m/z	Abundance
40.00	120.0
44.00	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB70

m/z	Abundance
36.00	229.0
37.10	1200.0
38.00	1099.0
39.10	446.0
44.10	295.0
45.00	287.0
47.00	442.0
48.00	135.0
49.00	1024.0
50.10	4986.0
51.10	1557.0
52.00	100.0
56.10	436.0
57.00	735.0
59.90	186.0
61.00	1238.0
62.10	1214.0
63.10	922.0
64.00	140.0
65.00	122.0
68.10	2824.0
69.10	2910.0
70.10	170.0
72.00	153.0
73.00	1082.0
74.10	4533.0
75.10	13923.0
76.10	1139.0
77.00	292.0
77.90	127.0
78.90	705.0
80.00	213.0
81.00	704.0
82.00	114.0
87.00	1272.0
88.00	1417.0
92.00	733.0
93.10	1051.0
94.10	3104.0
95.10	29840.0
96.10	2176.0
104.00	119.0
106.00	115.0
116.90	159.0
117.90	107.0
119.00	161.0
128.00	110.0
140.90	228.0
143.00	265.0
171.90	241.0
174.00	26128.0
175.00	1967.0
176.00	26160.0
177.00	1679.0

Instrument :
MSVOA_U
ClientSampleId :
BFB70

m/z	Abundance
36.00	206.0
37.10	1246.0
38.10	1238.0
39.10	500.0
44.10	344.0
45.00	319.0
47.00	412.0
48.00	115.0
49.10	1128.0
50.10	5470.0
51.10	1674.0
56.10	423.0
57.00	809.0
59.90	213.0
61.00	1401.0
62.10	1324.0
63.10	1059.0
64.00	171.0
65.00	126.0
68.10	3070.0
69.10	3290.0
70.10	206.0
72.00	196.0
73.00	1227.0
74.10	4885.0
75.10	15689.0
76.10	1263.0
77.00	269.0
77.80	109.0
79.00	812.0
80.00	237.0
81.00	799.0
82.00	123.0
87.00	1304.0
88.00	1513.0
92.00	796.0
93.00	1143.0
94.10	3406.0
95.10	31976.0
96.10	2376.0
104.00	118.0
105.90	125.0
115.90	105.0
116.90	161.0
117.90	137.0
118.90	145.0
127.90	104.0
129.90	111.0
140.90	273.0
143.00	283.0
171.90	206.0
174.00	27968.0
175.00	1942.0
176.00	27600.0
177.00	1793.0

Instrument :
MSVOA_U
ClientSampleId :
BFB70

m/z	Abundance
36.00	185.0
37.10	1244.0
38.10	1293.0
39.10	490.0
39.90	103.0
44.10	402.0
45.00	292.0
47.00	404.0
47.90	117.0
49.00	1143.0
50.10	5544.0
51.10	1684.0
56.10	398.0
57.10	801.0
59.90	220.0
61.00	1433.0
62.10	1309.0
63.10	1150.0
64.00	175.0
65.10	129.0
68.10	2909.0
69.10	3340.0
70.10	225.0
72.00	234.0
73.10	1238.0
74.10	4910.0
75.10	15522.0
76.10	1310.0
77.10	214.0
77.80	113.0
79.00	827.0
80.00	222.0
81.00	789.0
82.00	128.0
87.00	1257.0
88.00	1511.0
92.00	752.0
93.00	1129.0
94.10	3539.0
95.10	31528.0
96.10	2331.0
103.90	102.0
105.90	113.0
115.90	112.0
116.90	150.0
117.90	134.0
118.90	140.0
129.90	113.0
140.90	273.0
143.00	271.0
171.90	183.0
174.00	27416.0
175.00	1852.0
176.00	26152.0
177.00	1771.0

Instrument :
MSVOA_U
ClientSampleId :
BFB70