

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010219\
 Data File : VU028984.D
 Acq On : 02 Jan 2019 12:06
 Operator : MD/SY
 Sample : J6593-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE806

Quant Time: Jan 03 04:10:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jan 03 03:47:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	103413	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	97849	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	44825	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	32510	5.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	117.40%
7) Chloroethane-d5	1.68	69	27008	5.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.80%
11) 1,1-Dichloroethene-d2	2.27	63	42370	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	4.19	46	77812	53.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.60%
24) Chloroform-d	4.65	84	56311	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
26) 1,2-Dichloroethane-d4	5.31	65	28281	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.34	84	122072	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
36) 1,2-Dichloropropane-d6	6.33	67	40429	5.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.60%
41) Toluene-d8	7.56	98	108635	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
43) trans-1,3-Dichloropropene-	7.85	79	15073	5.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	109.60%
46) 2-Hexanone-d5	8.31	63	69343	55.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.64%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	29124	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	39855	5.31	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	6952	5.954 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010219\
Data File : VU028984.D
Acq On : 02 Jan 2019 12:06
Operator : MD/SY
Sample : J6593-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE806

Quant Time: Jan 03 04:10:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jan 03 03:47:56 2019
Response via : Initial Calibration

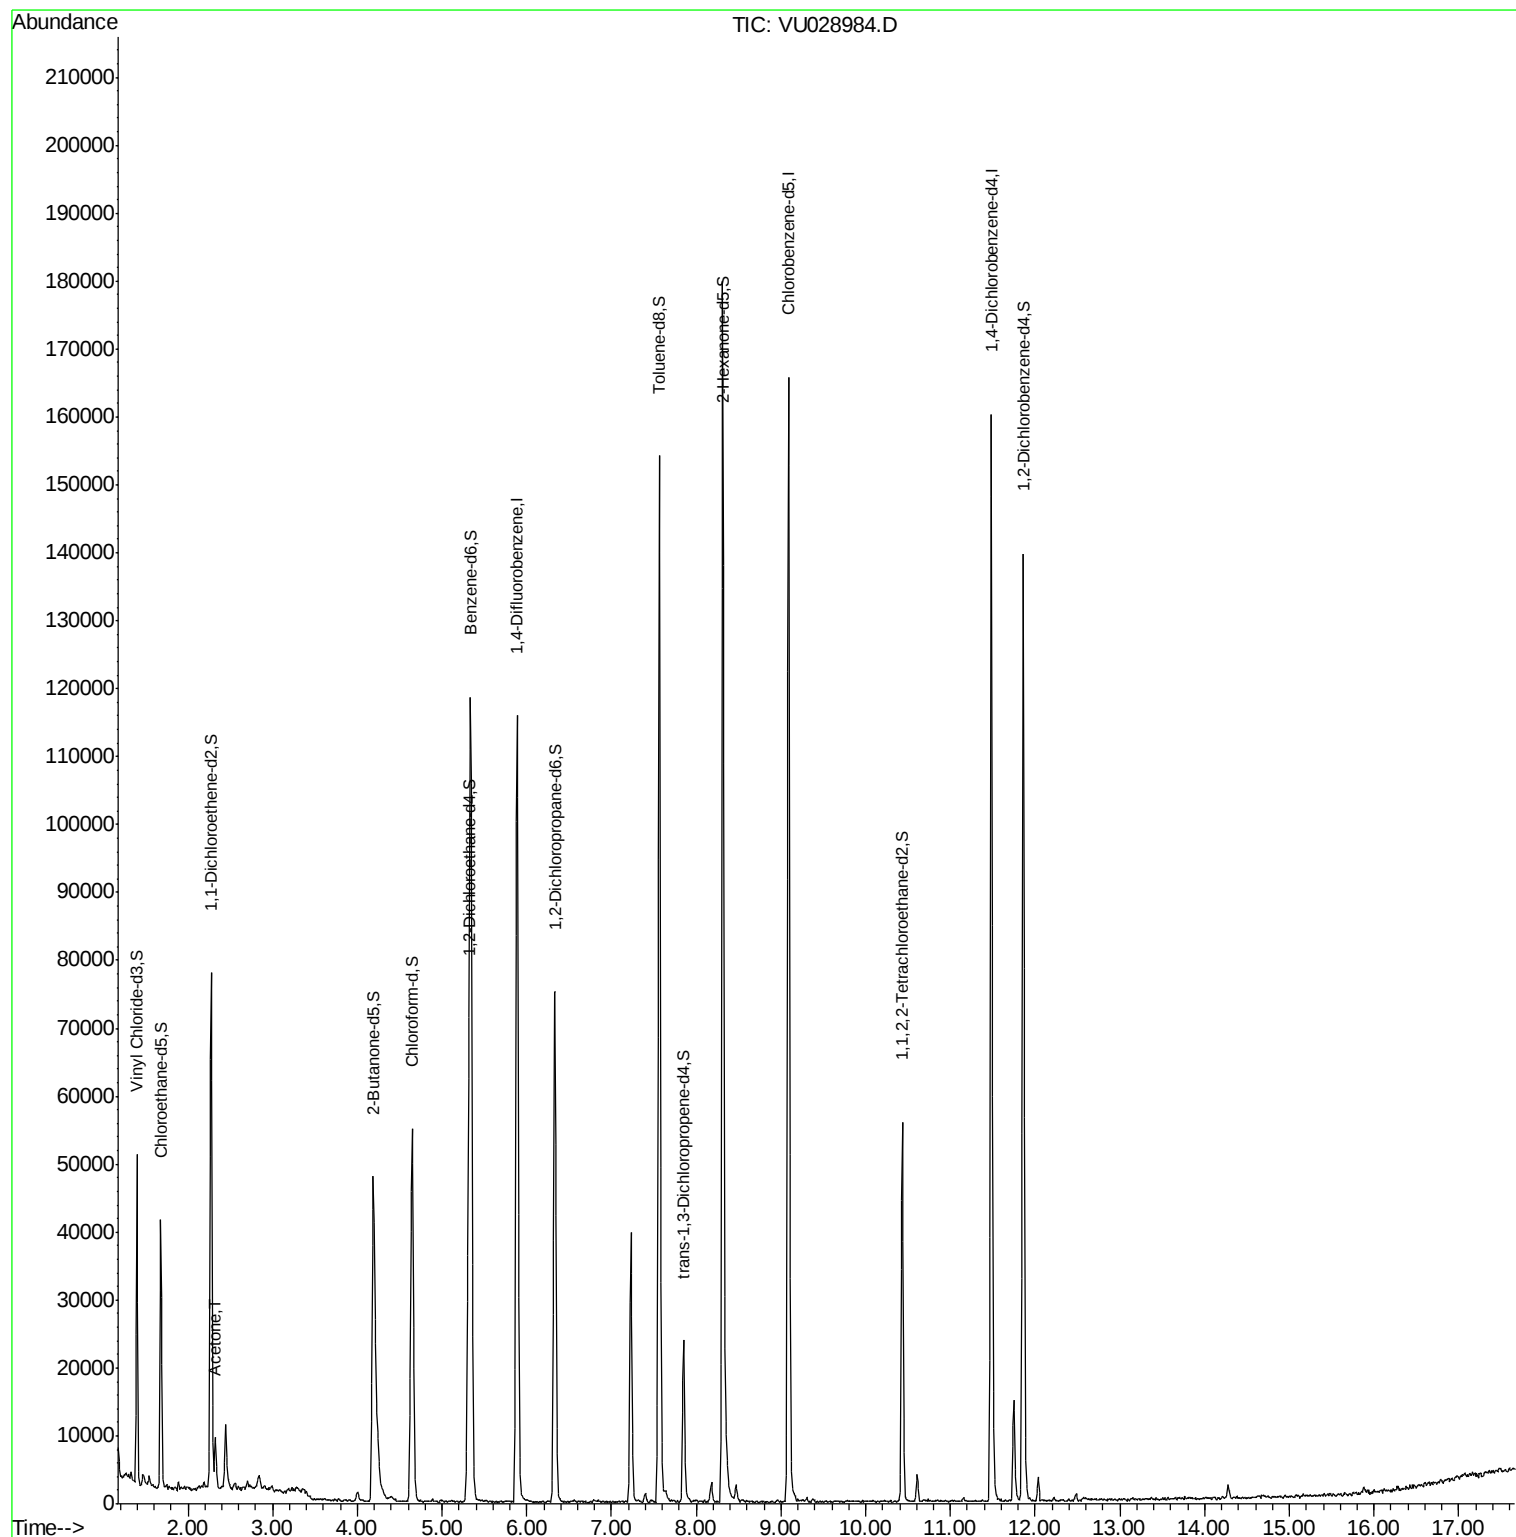

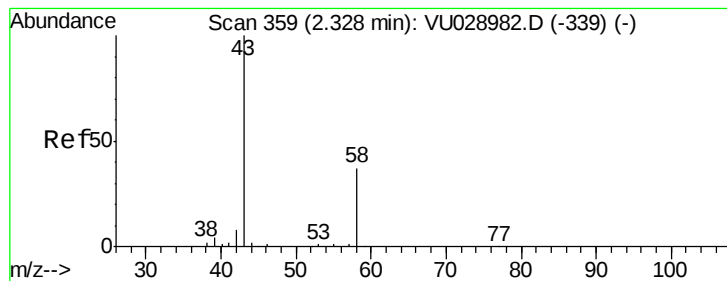

#13
 Acetone
 Concen: 5.954 ug/L
 RT: 2.32 min Scan# 357
 Delta R.T. -0.01 min
 Lab File: VU028984.D
 Acq: 02 Jan 2019 12:06

Instrument :
 MSVOA_U
 ClientSampleId :
 BE806

Tot Ion: 43 Resp: 6952
 Ion Ratio Lower Upper
 43 100
 58 37.7 0.0 71.8

