


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010219\
Data File : VU028981.D
Acq On : 02 Jan 2019 09:16
Operator : MD/SY
Sample : BFB68
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB68

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jan 03 03:47:56 2019

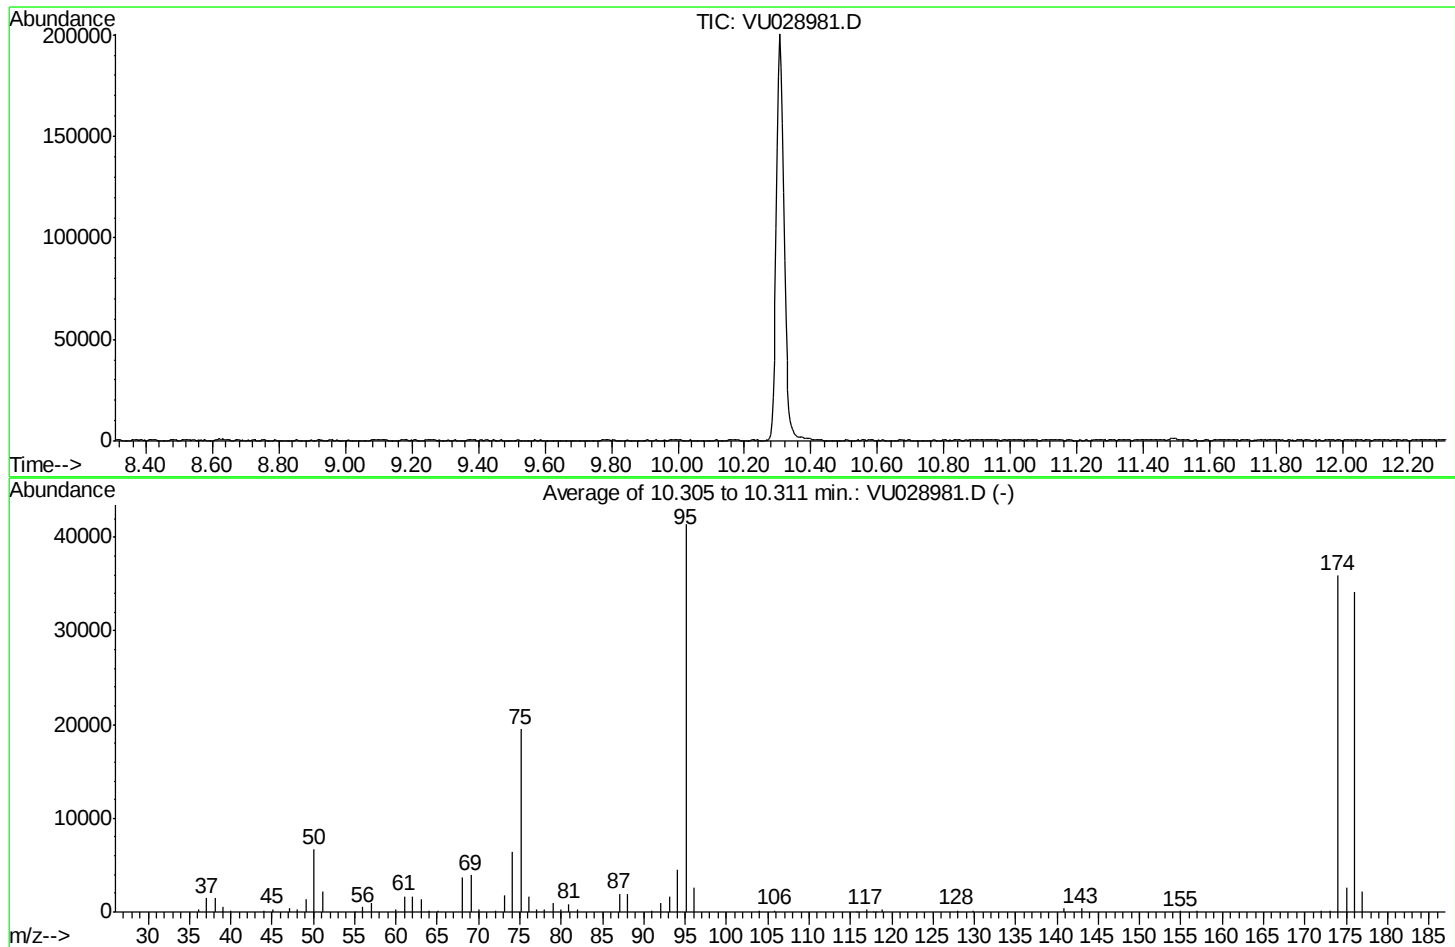

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	6676	PASS
75	95	30	80	47.2	19541	PASS
95	95	100	100	100.0	41386	PASS
96	95	5	9	6.3	2587	PASS
173	174	0.00	2	0.4	148	PASS
174	95	50	120	86.8	35922	PASS
175	174	5	9	7.2	2599	PASS
176	174	95	101	95.1	34160	PASS
177	176	5	9	6.6	2248	PASS

m/z	Abundance
36.00	388.0
37.10	1615.0
38.10	1463.0
39.00	570.0
44.00	470.0
45.10	308.0
47.10	491.0
48.00	215.0
49.10	1443.0
50.10	6890.0
51.10	2310.0
55.00	118.0
56.00	578.0
57.00	1000.0
60.00	329.0
61.10	1834.0
62.10	1637.0
63.10	1381.0
64.00	158.0
68.10	3709.0
69.10	4183.0
70.10	291.0
72.00	217.0
73.10	1779.0
74.10	6718.0
75.10	20184.0
76.10	1757.0
77.10	247.0
77.90	272.0
79.00	901.0
79.90	254.0
81.00	872.0
81.90	248.0
87.10	2059.0
88.00	1871.0
90.90	163.0
92.00	904.0
93.10	1608.0
94.10	4615.0
95.10	42424.0
96.10	2628.0
103.90	116.0
105.90	156.0
115.80	145.0
117.00	241.0
117.80	118.0
118.90	207.0
127.90	147.0
129.80	109.0
140.90	354.0
143.00	381.0
155.00	103.0
156.90	113.0
171.90	195.0
173.00	444.0
174.00	36240.0
175.00	2700.0
176.00	34512.0
177.00	2327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB68

m/z	Abundance
36.00	340.0
37.10	1520.0
38.10	1487.0
39.10	517.0
40.10	101.0
44.00	460.0
45.10	309.0
47.10	505.0
48.00	236.0
49.10	1465.0
50.10	6911.0
51.10	2306.0
56.00	532.0
57.00	940.0
60.00	319.0
61.00	1726.0
62.10	1668.0
63.10	1429.0
64.10	160.0
65.10	105.0
68.10	3717.0
69.10	4023.0
70.10	292.0
72.00	209.0
73.10	1820.0
74.10	6678.0
75.10	20120.0
76.10	1682.0
77.00	290.0
78.00	243.0
79.00	954.0
79.90	287.0
80.90	858.0
81.90	232.0
87.10	2009.0
88.00	1942.0
91.00	157.0
92.00	947.0
93.00	1624.0
94.10	4596.0
95.10	42656.0
96.10	2664.0
103.90	123.0
105.80	145.0
117.00	231.0
118.10	102.0
118.90	225.0
128.00	146.0
129.80	112.0
140.90	364.0
143.00	415.0
155.00	117.0
156.90	122.0
172.00	198.0
174.00	36968.0
175.00	2653.0
176.00	35128.0
177.00	2305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB68

m/z	Abundance
36.10	268.0
37.00	1332.0
38.10	1372.0
39.00	464.0
40.00	139.0
44.00	421.0
45.10	289.0
47.10	429.0
48.00	239.0
49.10	1305.0
50.10	6227.0
51.10	2101.0
56.00	446.0
57.00	813.0
60.00	313.0
61.00	1521.0
62.00	1539.0
63.10	1226.0
64.10	132.0
65.00	138.0
68.10	3456.0
69.10	3624.0
70.10	248.0
72.00	195.0
73.10	1654.0
74.10	5897.0
75.10	18320.0
76.10	1481.0
77.00	260.0
78.00	218.0
79.00	886.0
79.90	300.0
80.90	794.0
81.90	174.0
87.00	1845.0
88.00	1868.0
91.00	138.0
92.00	955.0
93.10	1531.0
94.10	4279.0
95.10	39080.0
96.00	2471.0
103.90	121.0
105.80	126.0
116.90	205.0
118.90	212.0
127.90	134.0
129.80	102.0
140.90	320.0
143.00	345.0
155.00	110.0
172.00	169.0
174.00	34560.0
175.00	2445.0
176.00	32840.0
177.00	2114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB68

m/z	Abundance
44.00	332.0

Instrument :
MSVOA_U
ClientSampleId :
BFB68