


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010319\
Data File : VU028990.D
Acq On : 03 Jan 2019 10:56
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Title : SW846 8260
Last Update : Fri Jan 04 02:22:53 2019

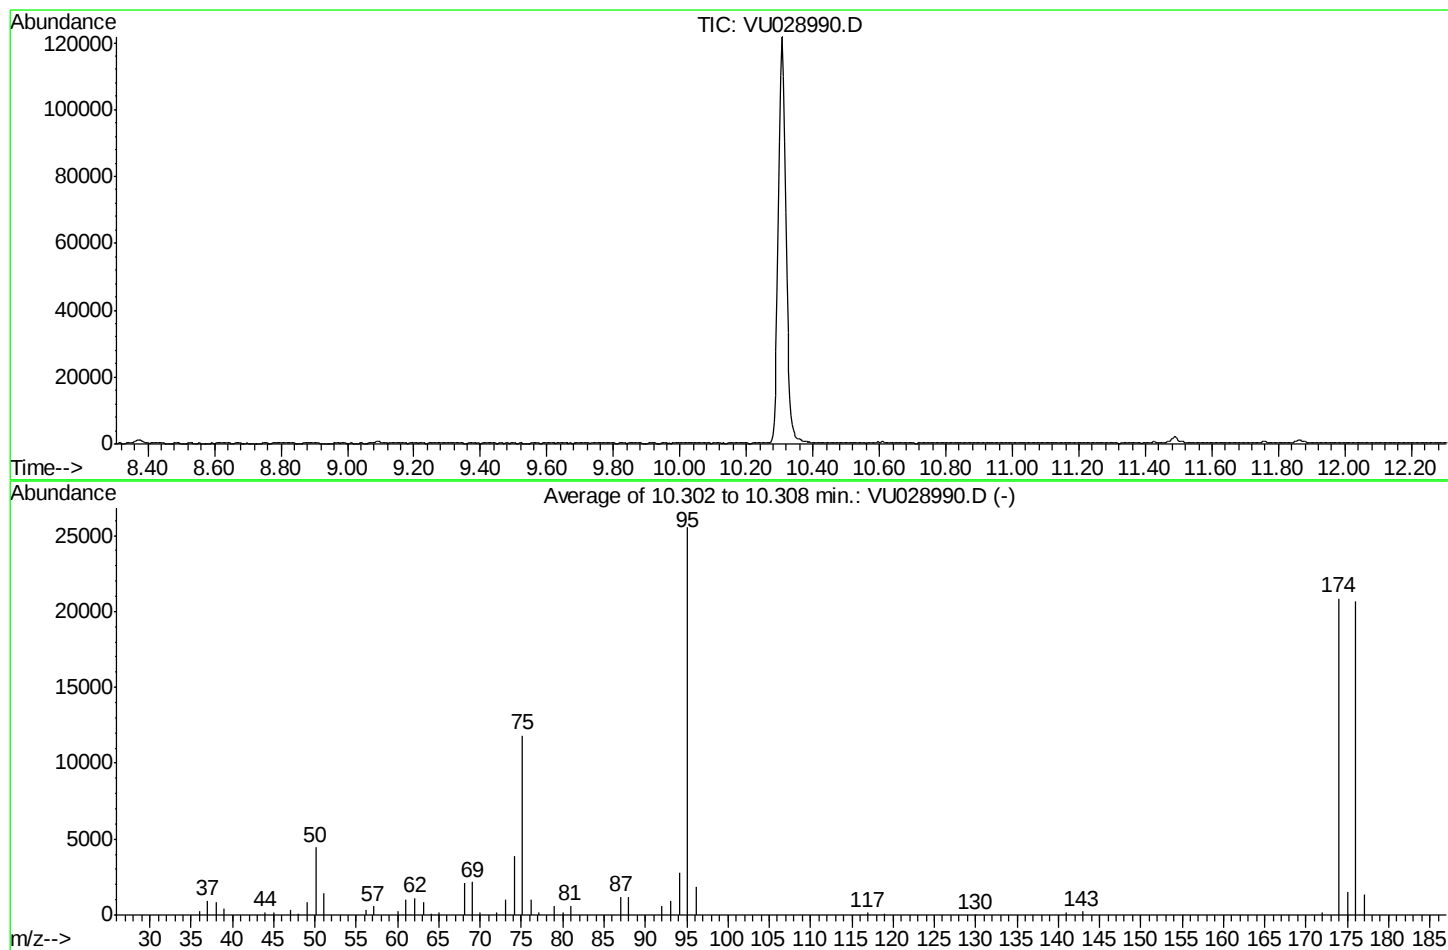

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4460	PASS
75	95	30	60	46.3	11825	PASS
95	95	100	100	100.0	25544	PASS
96	95	5	9	7.2	1847	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.6	20837	PASS
175	174	5	9	7.3	1519	PASS
176	174	95	101	99.0	20626	PASS
177	176	5	9	6.5	1345	PASS