


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010419\
 Data File : VU029014.D
 Acq On : 04 Jan 2019 08:31
 Operator : MD/SY
 Sample : BFB69
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB69

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jan 04 22:41:21 2019

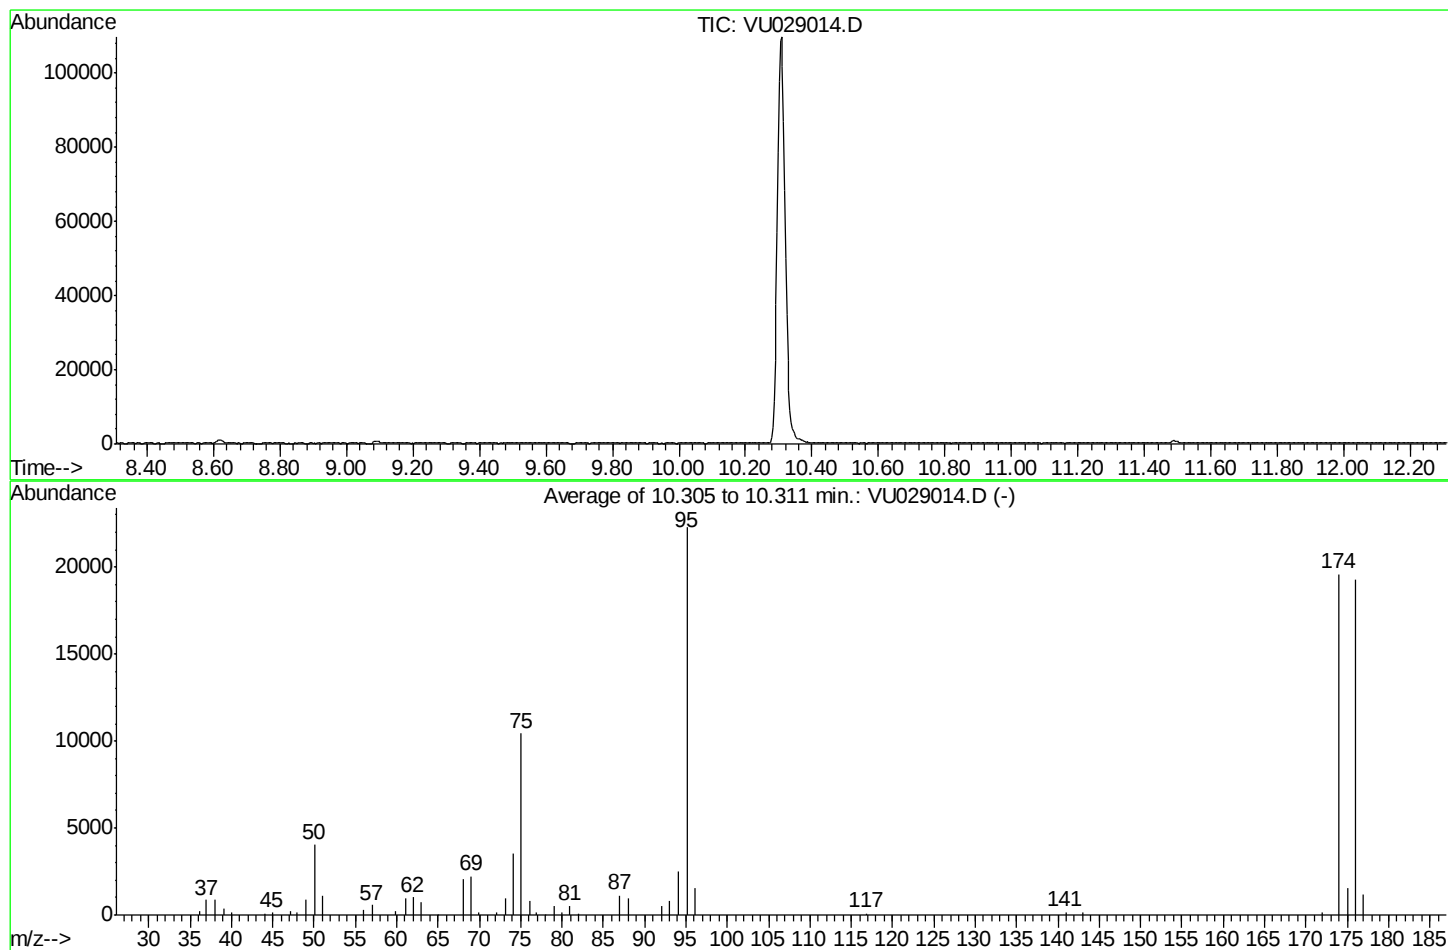

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4024	PASS
75	95	30	80	46.9	10448	PASS
95	95	100	100	100.0	22285	PASS
96	95	5	9	7.1	1579	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.9	19586	PASS
175	174	5	9	7.8	1519	PASS
176	174	95	101	98.5	19301	PASS
177	176	5	9	6.1	1179	PASS

m/z	Abundance
44.00	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB69

m/z	Abundance
36.10	243.0
37.00	944.0
38.00	859.0
39.10	397.0
40.00	124.0
44.00	272.0
45.00	143.0
47.10	226.0
48.00	130.0
49.00	875.0
50.10	3976.0
51.10	1198.0
56.00	346.0
57.00	579.0
59.90	226.0
61.10	944.0
62.00	1031.0
63.00	744.0
65.00	113.0
68.10	2166.0
69.00	2346.0
69.90	142.0
72.00	180.0
73.10	1012.0
74.10	3461.0
75.10	10760.0
76.10	782.0
77.00	193.0
78.00	113.0
79.00	494.0
80.00	163.0
80.90	577.0
82.00	122.0
87.00	1112.0
88.10	999.0
92.00	550.0
93.00	926.0
94.10	2622.0
95.10	22880.0
96.10	1713.0
116.90	155.0
140.90	212.0
143.10	168.0
171.90	131.0
174.00	19440.0
175.00	1608.0
176.00	19128.0
177.00	1282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB69

m/z	Abundance
36.10	227.0
37.00	896.0
38.00	883.0
39.00	348.0
40.00	114.0
44.00	262.0
44.90	132.0
47.10	231.0
48.00	145.0
49.00	913.0
50.10	4179.0
51.10	1139.0
56.10	312.0
57.00	578.0
59.90	237.0
61.00	987.0
62.00	1062.0
63.00	756.0
68.00	2123.0
69.00	2325.0
70.00	142.0
72.00	158.0
73.10	968.0
74.10	3581.0
75.10	10652.0
76.10	871.0
76.90	153.0
79.00	523.0
80.10	189.0
80.90	561.0
87.00	1118.0
88.00	992.0
92.00	533.0
93.00	821.0
94.10	2573.0
95.10	22920.0
96.10	1631.0
116.80	115.0
141.00	179.0
143.00	139.0
172.00	159.0
174.00	20160.0
175.00	1576.0
176.00	19952.0
177.00	1203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB69

m/z	Abundance
36.10	173.0
37.00	773.0
38.00	831.0
39.00	297.0
40.00	104.0
44.00	288.0
45.00	111.0
47.10	253.0
48.00	142.0
49.00	828.0
50.10	3918.0
51.10	1032.0
56.10	240.0
57.00	530.0
59.90	189.0
61.00	928.0
62.00	975.0
63.00	695.0
68.00	1983.0
69.00	2033.0
70.00	126.0
72.10	118.0
73.10	843.0
74.10	3477.0
75.10	9934.0
76.00	882.0
76.90	119.0
79.00	504.0
80.10	205.0
81.00	494.0
87.00	1102.0
88.00	949.0
92.00	465.0
93.10	715.0
94.00	2372.0
95.10	21056.0
96.10	1395.0
141.00	149.0
143.00	136.0
172.00	182.0
174.00	19160.0
175.00	1374.0
176.00	18824.0
177.00	1052.0

Instrument :
MSVOA_U
ClientSampleId :
BFB69