


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU010421\
 Data File : VU041836.D
 Acq On : 04 Jan 2021 09:35
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB32

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jan 05 01:00:34 2021

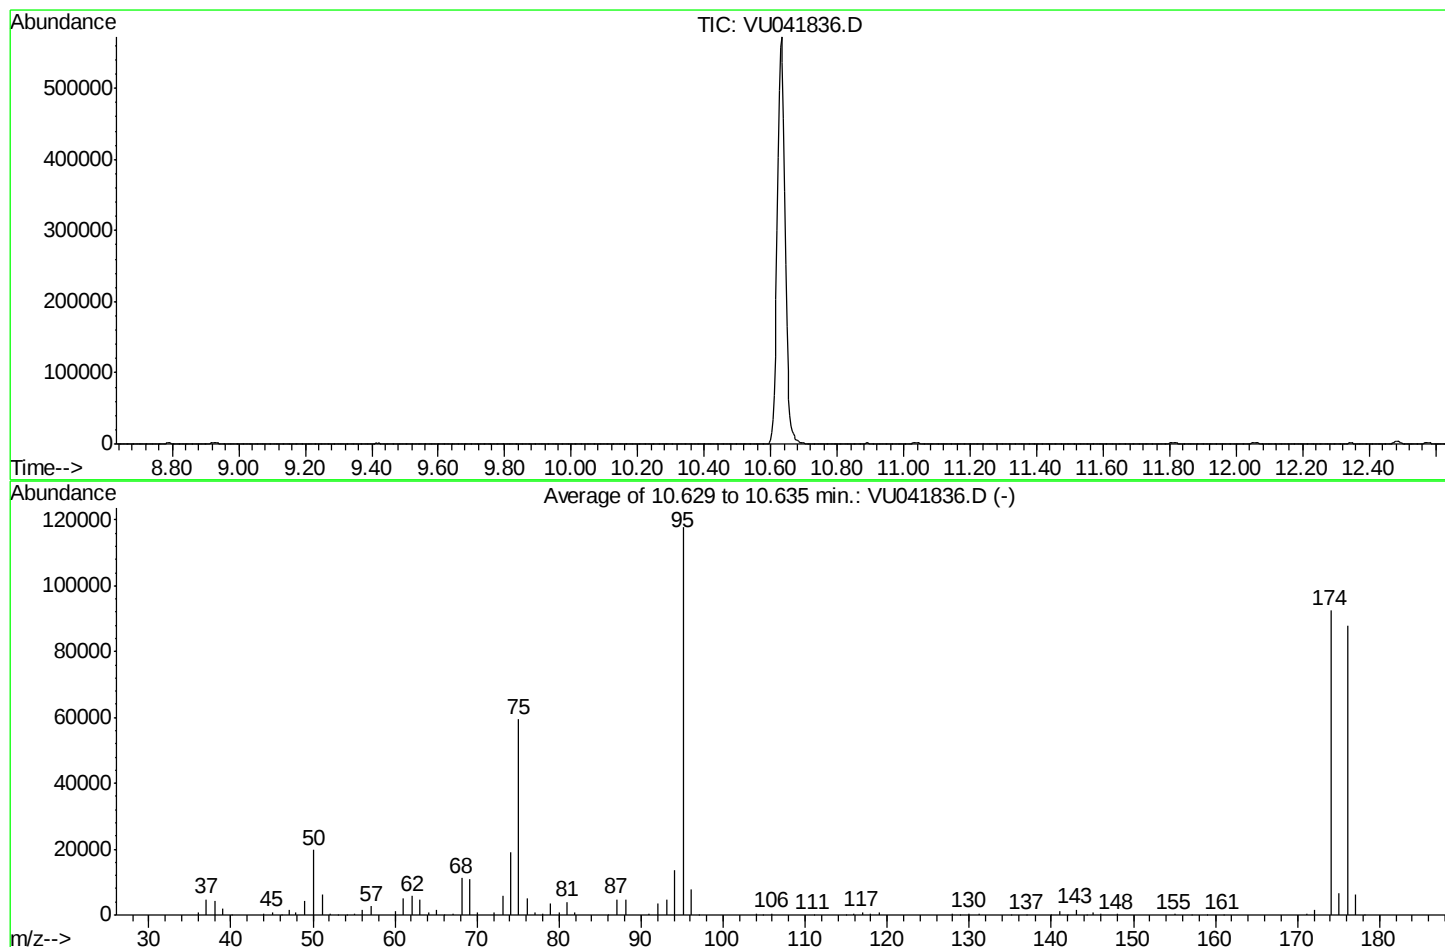

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	19688	PASS
75	95	30	80	50.5	59440	PASS
95	95	100	100	100.0	117770	PASS
96	95	5	9	6.5	7628	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.5	92424	PASS
175	174	5	9	7.2	6664	PASS
176	174	95	101	95.1	87917	PASS
177	176	5	9	7.0	6189	PASS

m/z	Abundance
36.00	824.0
37.00	4997.0
38.00	4499.0
39.00	1830.0
40.10	144.0
44.00	619.0
45.10	818.0
46.10	183.0
47.10	1481.0
47.90	617.0
49.00	4567.0
50.10	19976.0
51.10	6192.0
52.00	369.0
53.10	139.0
54.10	122.0
55.00	400.0
56.00	1461.0
57.10	2722.0
60.00	1223.0
61.00	5133.0
62.10	5458.0
63.10	4793.0
64.10	805.0
65.10	1503.0
67.20	232.0
68.10	11226.0
69.10	10879.0
70.10	1033.0
72.10	849.0
73.10	5864.0
74.10	19360.0
75.10	59896.0
76.10	5052.0
77.10	840.0
77.90	504.0
79.00	3849.0
80.00	1092.0
81.00	4036.0
82.00	906.0
85.90	206.0
87.10	4590.0
88.10	4748.0
91.00	429.0
92.10	3492.0
93.10	4656.0
94.10	13896.0
95.10	118056.0
96.10	7528.0
97.00	138.0
104.00	421.0
104.90	126.0
106.00	550.0
115.00	141.0
115.90	354.0
117.00	810.0
118.00	415.0
119.00	779.0
128.00	425.0
128.90	178.0
130.00	472.0
131.20	235.0
135.00	145.0
137.00	114.0
139.90	110.0
141.10	1014.0
142.00	158.0
143.10	1511.0
145.10	656.0
146.00	221.0
148.00	239.0
155.00	221.0
157.10	173.0
159.00	142.0
161.00	127.0
171.20	347.0
172.10	1519.0
174.10	91832.0
175.10	6694.0
176.10	86968.0
177.10	6089.0
178.20	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	795.0
37.00	4923.0
38.00	4250.0
39.10	1800.0
40.10	138.0
44.00	618.0
45.00	919.0
46.20	129.0
47.10	1529.0
48.00	713.0
49.00	4477.0
50.10	20448.0
51.10	6201.0
52.00	310.0
53.10	145.0
55.00	341.0
56.00	1495.0
57.10	2797.0
60.00	1245.0
61.10	5240.0
62.10	5928.0
63.00	4826.0
64.10	763.0
65.10	1450.0
65.90	119.0
67.20	252.0
68.10	11390.0
69.10	11160.0
70.00	989.0
72.10	811.0
73.10	5857.0
74.10	19704.0
75.10	61288.0
76.10	5222.0
77.00	833.0
77.90	591.0
79.00	3727.0
80.00	1001.0
81.00	4048.0
81.90	841.0
85.90	139.0
87.00	4933.0
88.10	4768.0
91.00	446.0
92.10	3593.0
93.10	4678.0
94.10	14116.0
95.10	121240.0
96.10	7900.0
97.10	149.0
104.00	477.0
104.90	133.0
105.90	533.0
115.00	156.0
115.90	315.0
117.00	812.0
118.00	479.0
119.00	824.0
128.00	404.0
128.90	152.0
130.00	464.0
131.20	233.0
135.10	143.0
137.00	146.0
141.10	1102.0
141.90	158.0
143.00	1592.0
144.30	125.0
145.10	634.0
145.90	270.0
148.00	232.0
155.00	218.0
157.10	212.0
159.00	166.0
161.00	100.0
171.10	238.0
172.10	1404.0
174.10	95096.0
175.10	6897.0
176.10	90728.0
177.10	6489.0
178.10	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.10	718.0
37.00	4486.0
38.00	3838.0
39.10	1688.0
40.10	146.0
44.00	531.0
45.00	867.0
47.10	1416.0
48.00	693.0
49.00	4023.0
50.10	18640.0
51.10	5768.0
52.10	269.0
53.10	150.0
55.00	272.0
56.00	1346.0
57.10	2578.0
60.00	1067.0
61.10	5000.0
62.10	5573.0
63.00	4499.0
64.00	709.0
65.10	1220.0
66.00	146.0
67.10	267.0
68.10	10856.0
69.10	10535.0
70.00	913.0
72.00	692.0
73.10	5398.0
74.10	18016.0
75.10	57136.0
76.10	5082.0
77.00	676.0
78.00	598.0
79.00	3185.0
80.00	869.0
81.00	3691.0
82.00	705.0
86.00	116.0
87.00	4661.0
88.10	4340.0
91.00	393.0
92.00	3434.0
93.10	4372.0
94.10	12961.0
95.10	114016.0
96.10	7457.0
97.10	180.0
104.00	461.0
104.90	109.0
105.90	496.0
111.00	113.0
115.00	146.0
115.90	246.0
117.00	760.0
118.00	507.0
119.00	770.0
127.90	319.0
128.90	122.0
130.00	424.0
131.20	180.0
135.00	137.0
137.00	189.0
141.10	1095.0
141.90	169.0
143.00	1586.0
145.10	611.0
145.90	239.0
148.00	238.0
155.00	216.0
157.10	212.0
159.00	180.0
171.00	131.0
172.00	1247.0
174.10	90344.0
175.10	6402.0
176.10	86056.0
177.10	5989.0
178.10	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
44.10	209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32