

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010519\
 Data File : VU029039.D
 Acq On : 04 Jan 2019 19:55
 Operator : MD/SY
 Sample : K1053-01 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMP-1-DRUM

Quant Time: Jan 05 03:49:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 04 02:22:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	114127	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	193150	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	179988	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	75894	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.30	65	74720	52.96	ug/l	0.00
Spiked Amount			Recovery	=	105.92%	
35) Dibromofluoromethane	4.88	113	66460	53.08	ug/l	0.00
Spiked Amount			Recovery	=	106.16%	
50) Toluene-d8	7.56	98	245964	49.76	ug/l	0.00
Spiked Amount			Recovery	=	99.52%	
62) 4-Bromofluorobenzene	10.30	95	80827	45.50	ug/l	0.00
Spiked Amount			Recovery	=	91.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	1118	Below Cal		91
4) Vinyl Chloride	1.28	62	1466	0.879 ug/l #		42
5) Bromomethane	1.62	94	114	Below Cal		96
11) Tert butyl alcohol	2.83	59	1691	4.715 ug/l #		73
16) Acetone	2.32	43	2635	2.965 ug/l		94
17) Carbon Disulfide	2.47	76	44	Below Cal #		75
18) Methyl Acetate	2.62	43	1441	0.697 ug/l		92
20) Methylene Chloride	2.70	84	312	0.207 ug/l		89
25) 2-Butanone	4.28	43	3355	2.795 ug/l		91
29) Tetrahydrofuran	4.57	42	290	0.398 ug/l #		56
31) Cyclohexane	4.98	56	2098	Below Cal #		1
36) 1,1-Dichloropropene	4.98	75	8309	4.304 ug/l #		46
38) Carbon Tetrachloride	4.98	117	10121	6.285 ug/l #		17
40) Benzene	5.39	78	10837	1.800 ug/l		97
41) Methacrylonitrile	4.57	41	2918	2.572 ug/l #		34
52) Toluene	7.64	92	7828	2.135 ug/l		91
67) Ethyl Benzene	9.25	91	1727	0.256 ug/l		96
68) m/p-Xylenes	9.37	106	2218	0.847 ug/l		97
69) o-Xylene	9.78	106	1009	0.400 ug/l		98
70) Styrene	9.80	104	2218	0.537 ug/l		90
76) 1,2,3-Trichloropropane	10.30	75	37481	20.156 ug/l #		36
81) trans-1,4-Dichloro-2-buten	10.30	75	37481	51.984 ug/l #		100
84) 1,2,4-Trimethylbenzene	11.15	105	1971	0.421 ug/l		88
85) sec-Butylbenzene	11.15	105	1971	0.352 ug/l #		57
90) Hexachloroethane	11.98	117	583	0.727 ug/l #		7
95) Naphthalene	13.74	128	33118	5.639 ug/l		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010519\
Data File : VU029039.D
Acq On : 04 Jan 2019 19:55
Operator : MD/SY
Sample : K1053-01 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM

Quant Time: Jan 05 03:49:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Fri Jan 04 02:22:53 2019
Response via : Initial Calibration

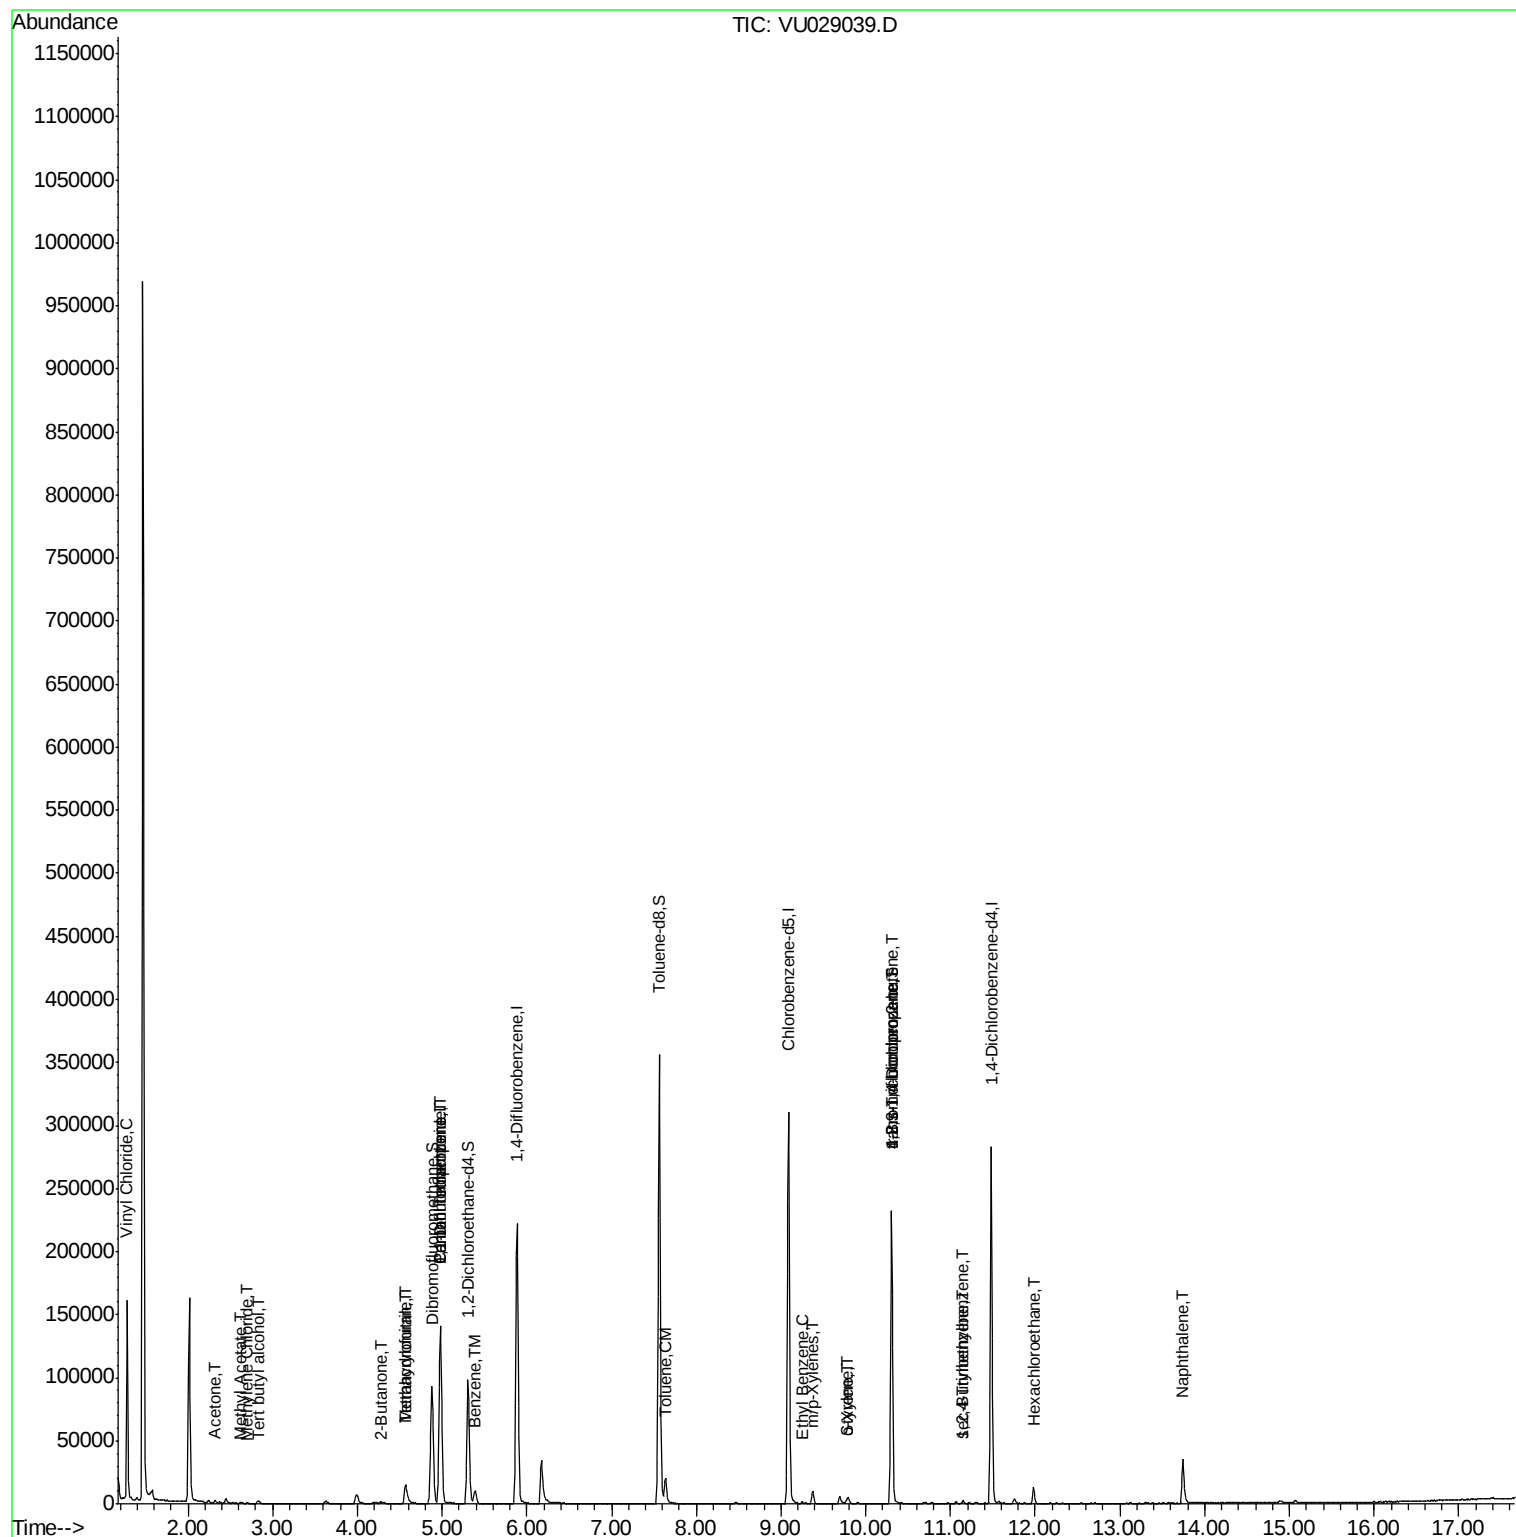

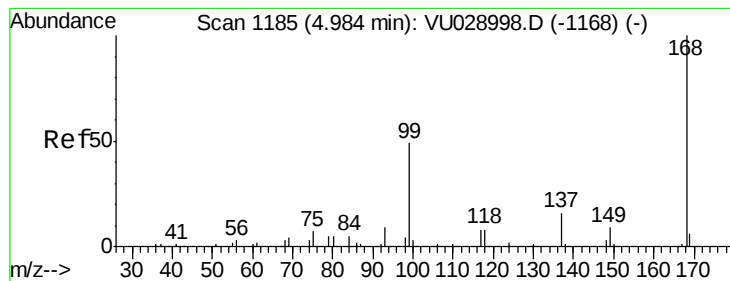

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1184

Delta R.T. -0.00 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :


COMP-1-DRUM

Tot Ion:168 Resp: 114127

Ion Ratio Lower Upper

168 100

99 52.1 42.0 63.0



Abundance Ion 167.90 (167.60 to 168.60): VU028998.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028998.D (-1168) (-)

4.98

60000

50000

40000

30000

20000

10000



0

4.90

5.00

5.10

Time-->



#4

Vinyl Chloride

Concen: 0.879 ug/l

RT: 1.28 min Scan# 34

Delta R.T. -0.12 min

Lab File: VU029039.D


Acq: 04 Jan 2019 19:55

Tgt Ion: 62 Resp: 1466

Ion Ratio Lower Upper

62 100

64 0.0 25.9 38.9#



Abundance Ion 61.90 (61.60 to 62.60): VU028998.D (-65) (-)

Ion 63.90 (63.60 to 64.60): VU028998.D (-65) (-)

1.28

1500

1000

500


0


1.26

1.28

1.30

Time-->



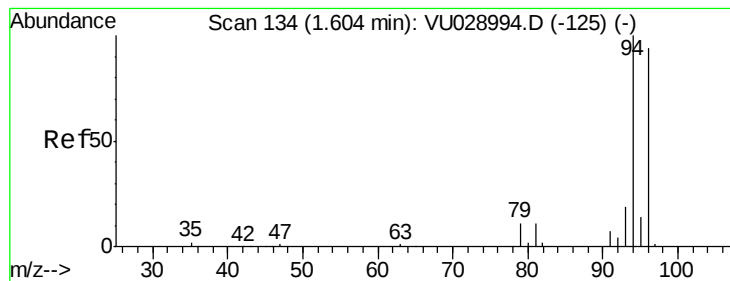

#5

Bromomethane

Concen: Below Cal

RT: 1.62 min Scan# 138

Delta R.T. 0.01 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :


COMP-1-DRUM

Tot Ion: 94 Resp: 114

Ion Ratio Lower Upper


94 100

96 98.4 75.5 113.3





Abundance Ion 93.90 (93.60 to 94.60): VU0

Ion 95.90 (95.60 to 96.60): VU0

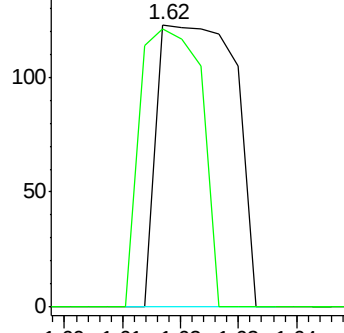

Time--> 1.60 1.61 1.62 1.63 1.64



#11

Tert butyl alcohol

Concen: 4.715 ug/l

RT: 2.83 min Scan# 515

Delta R.T. -0.00 min

Lab File: VU029039.D


Acq: 04 Jan 2019 19:55

Tgt Ion: 59 Resp: 1691

Ion Ratio Lower Upper


59 100

57 0.0 7.9 11.9#





Abundance Ion 59.00 (58.70 to 59.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

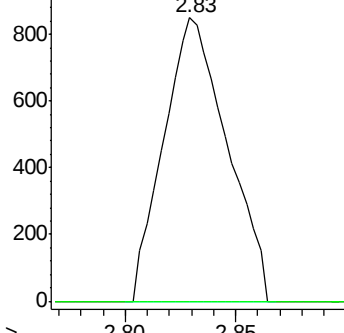

Time--> 2.80 2.85





#16

Acetone

Concen: 2.965 ug/l

RT: 2.32 min Scan# 357

Delta R.T. -0.00 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :





COMP-1-DRUM

Tot Ion: 43 Resp: 2635

Ion Ratio Lower Upper

43 100

58 32.3 28.6 42.8

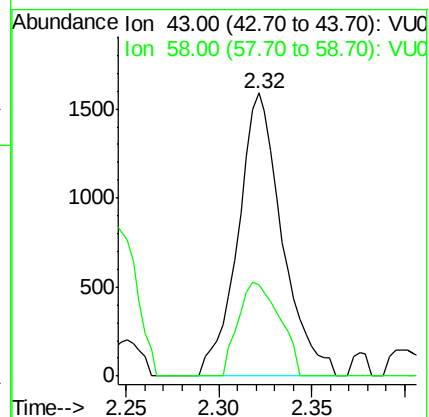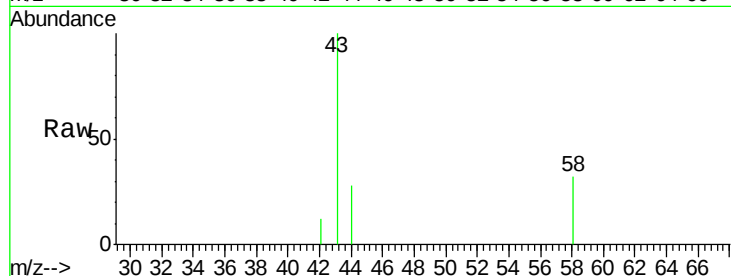

#17

Carbon Disulfide

Concen: Below Cal

RT: 2.47 min Scan# 402

Delta R.T. -0.01 min

Lab File: VU029039.D




Acq: 04 Jan 2019 19:55


Tgt Ion: 76 Resp: 44

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#



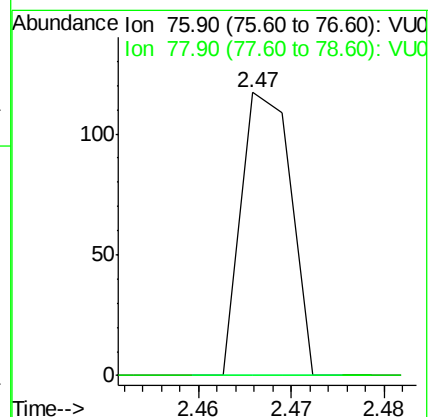





#18
Methvl Acetate
Concen: 0.697 ug/l
RT: 2.62 min Scan# 449
Delta R.T. 0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55




Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM


Tot Ion: 43 Resp: 1441
Ion Ratio Lower Upper
43 100
74 20.3 19.5 29.3

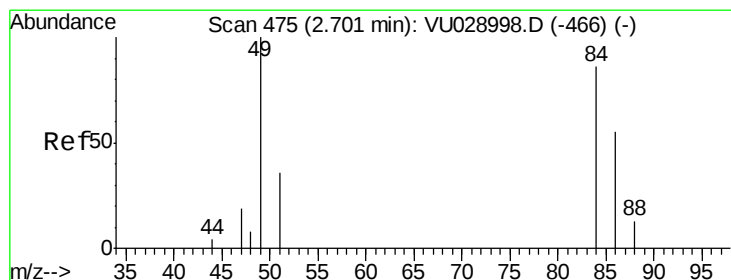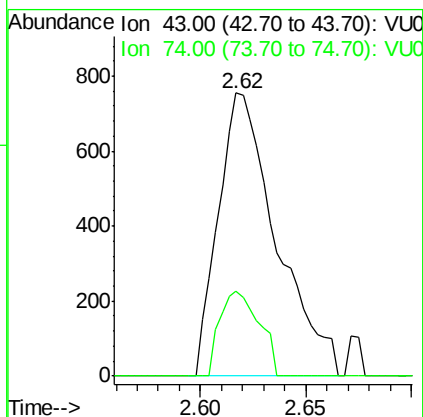

#20
Methylene Chloride
Concen: 0.207 ug/l
RT: 2.70 min Scan# 474
Delta R.T. -0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55

Tgt Ion: 84 Resp: 312
Ion Ratio Lower Upper
84 100
49 102.9 91.9 137.9
51 42.0 29.2 43.8
86 54.6 51.8 77.6

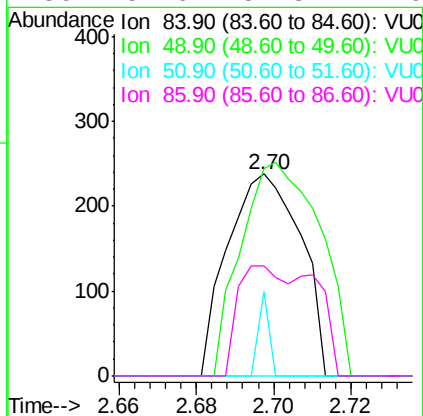



#25

2-Butanone

Concen: 2.795 ug/l

RT: 4.28 min Scan# 966

Delta R.T. 0.02 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :





COMP-1-DRUM

Tot Ion: 43 Resp: 3355

Ion Ratio Lower Upper

43 100

72 23.3 22.6 33.8

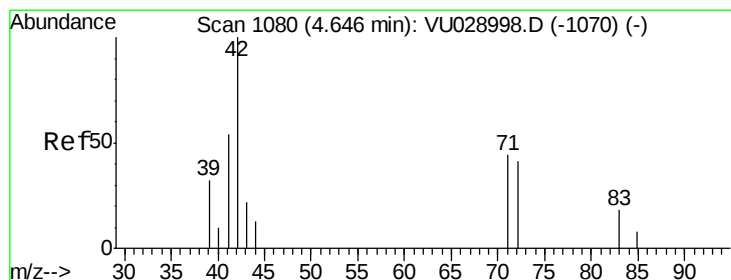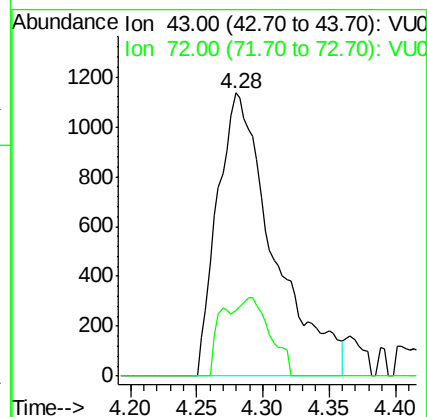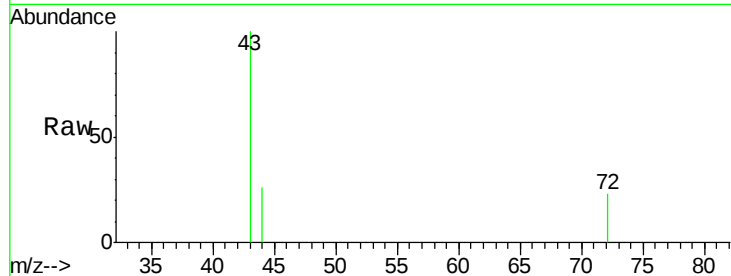

#29

Tetrahydrofuran

Concen: 0.398 ug/l

RT: 4.57 min Scan# 1056

Delta R.T. -0.06 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55




Tgt Ion: 42 Resp: 290


Ion Ratio Lower Upper

42 100

72 61.4 38.3 57.5#

71 0.0 36.1 54.1#

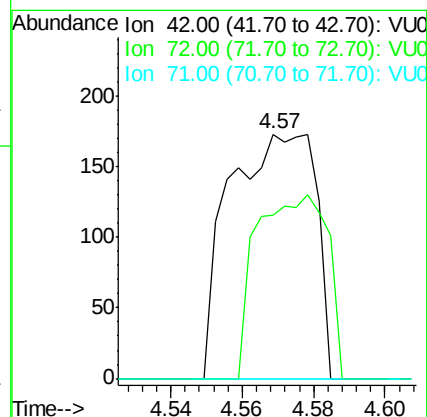

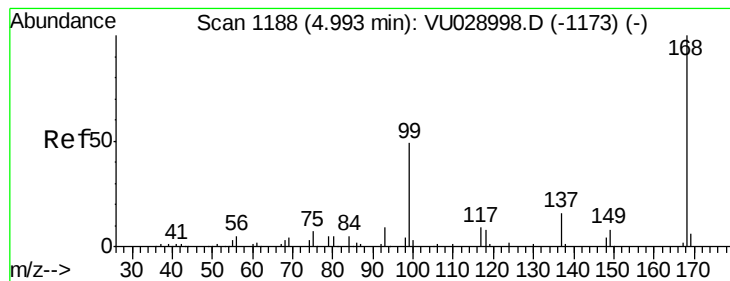

#31

Cyclohexane

Concen: Below Cal

RT: 4.98 min Scan# 1183

Delta R.T. -0.02 min


Lab File: VU029039.D

Acq: 04 Jan 2019 19:55




Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM

Tot Ion: 56 Resp: 2098

Ion	Ratio	Lower	Upper
56	100		
69	177.4	26.7	40.1#
84	166.0	65.7	98.5#



Abundance Ion 56.00 (55.70 to 56.70): VU0
Ion 69.00 (68.70 to 69.70): VU0
Ion 84.00 (83.70 to 84.70): VU0

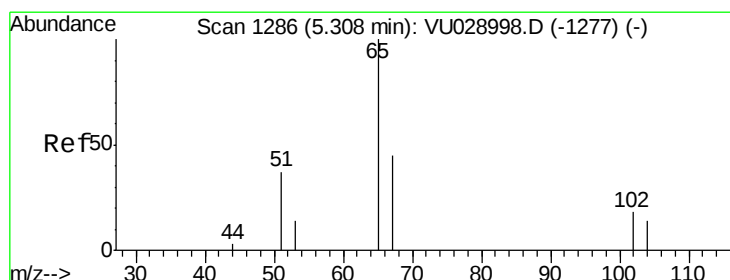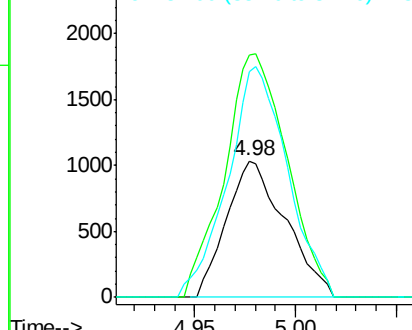

#33

1,2-Dichloroethane-d4

Concen: 52.962 ug/l

RT: 5.30 min Scan# 1285


Delta R.T. -0.00 min

Lab File: VU029039.D



Acq: 04 Jan 2019 19:55


Tgt Ion: 65 Resp: 74720

Ion	Ratio	Lower	Upper
65	100		
67	55.9	0.0	111.0



Abundance Ion 64.90 (64.60 to 65.60): VU0
Ion 66.90 (66.60 to 67.60): VU0

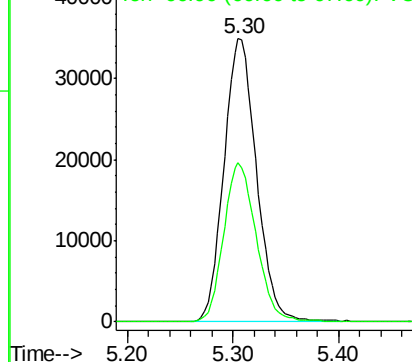

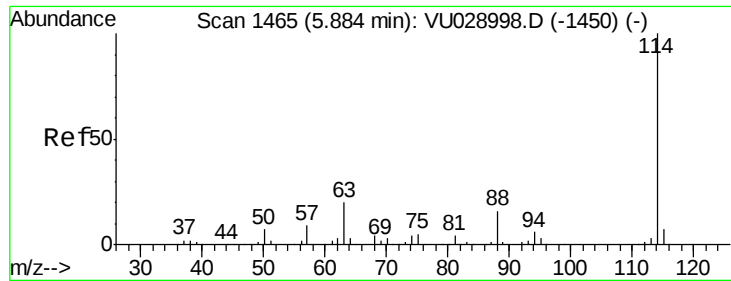

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.88 min Scan# 1465

Delta R.T. -0.00 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :

COMP-1-DRUM


Tot Ion:114 Resp: 193150

Ion Ratio Lower Upper

114 100

63 20.8 0.0 40.2




88 15.6 0.0 30.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

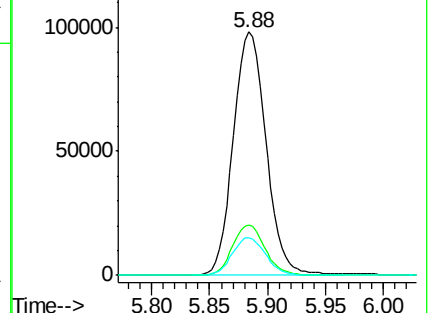

#35

Dibromofluoromethane

Concen: 53.081 ug/l

RT: 4.88 min Scan# 1153

Delta R.T. -0.00 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55


Tgt Ion:113 Resp: 66460

Ion Ratio Lower Upper

113 100

111 101.7 81.4 122.2



192 20.0 16.8 25.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



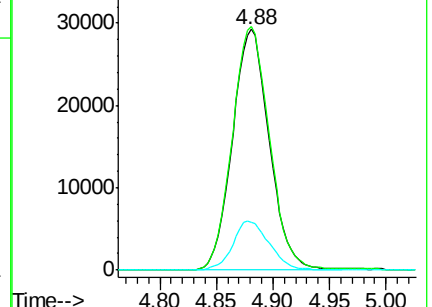





#36
 1,1-Dichloropropene
 Concen: 4.304 ug/l
 RT: 4.98 min Scan# 1183
 Delta R.T. -0.16 min
 Lab File: VU029039.D
 Acq: 04 Jan 2019 19:55




Instrument :
 MSVOA_U
 ClientSampleId :
 COMP-1-DRUM


Tot Ion: 75 Resp: 8309
 Ion Ratio Lower Upper
 75 100
 110 6.5 18.4 55.4#
 77 0.0 25.1 37.7#

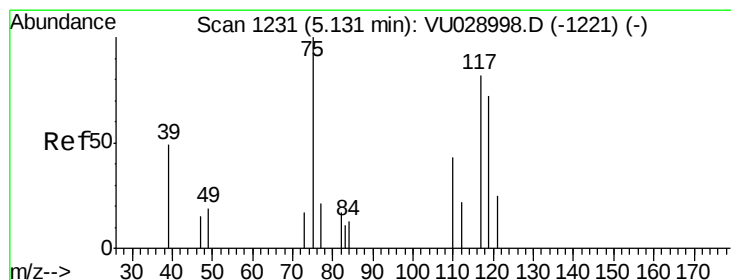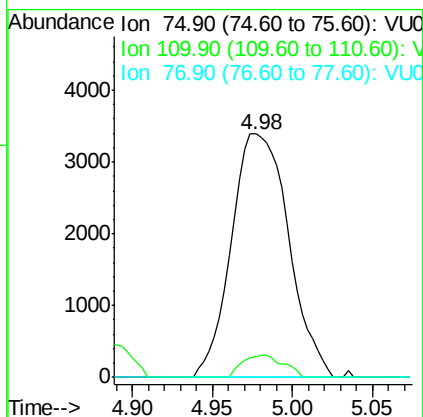

#38
 Carbon Tetrachloride
 Concen: 6.285 ug/l
 RT: 4.98 min Scan# 1184
 Delta R.T. -0.15 min
 Lab File: VU029039.D
 Acq: 04 Jan 2019 19:55

Tgt Ion: 117 Resp: 10121
 Ion Ratio Lower Upper
 117 100
 119 4.6 74.6 111.8#
 121 0.0 25.0 37.6#



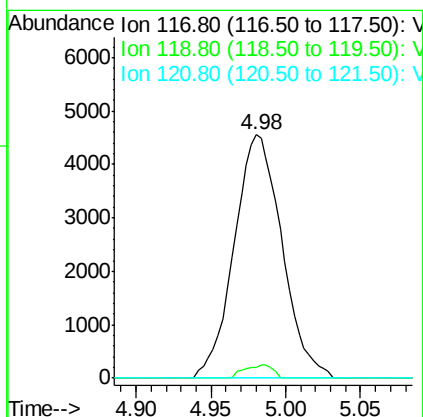
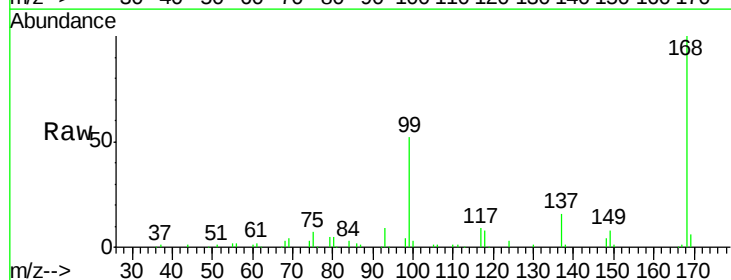




#40
Benzene
Concen: 1.800 ug/l
RT: 5.39 min Scan# 1311
Delta R.T. 0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55




Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM


Tot Ion: 78 Resp: 10837
Ion Ratio Lower Upper
78 100
77 25.0 18.9 28.3

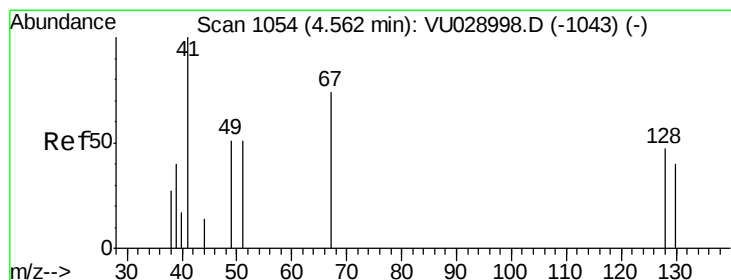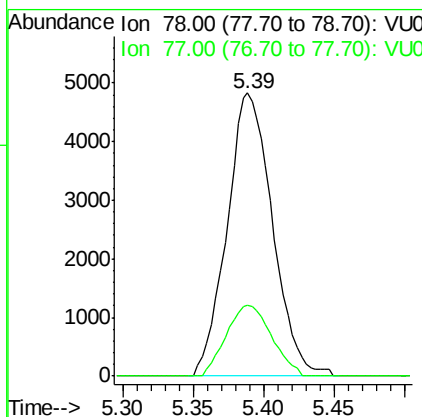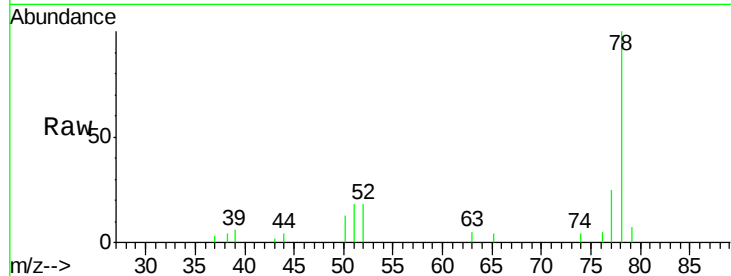

#41
Methacrylonitrile
Concen: 2.572 ug/l
RT: 4.57 min Scan# 1056
Delta R.T. 0.03 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55

Tgt Ion: 41 Resp: 2918
Ion Ratio Lower Upper
41 100
39 29.0 42.3 63.5#
67 0.0 64.4 96.6#
52 0.0 23.9 35.9#



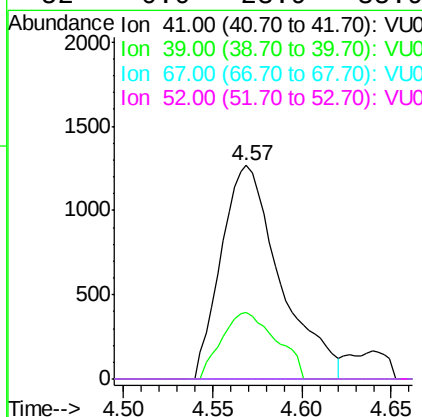





#50
Toluene-d8
Concen: 49.761 ug/l
RT: 7.56 min Scan# 1987
Delta R.T. -0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55




Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM


Tot Ion: 98 Resp: 245964
Ion Ratio Lower Upper
98 100
100 63.4 51.6 77.4

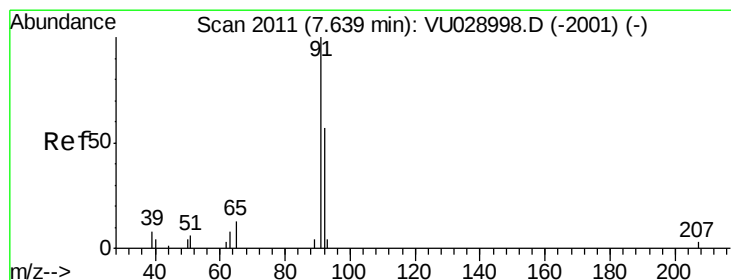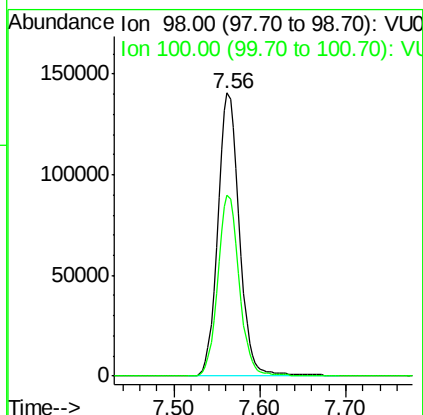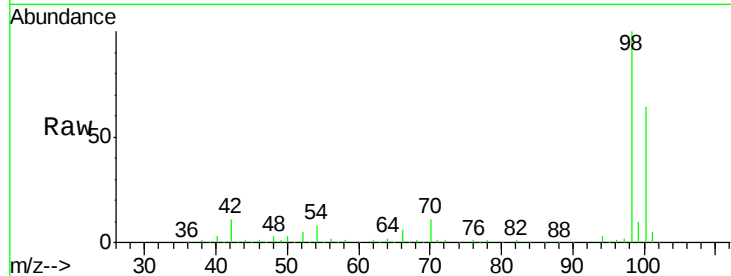

#52
Toluene
Concen: 2.135 ug/l
RT: 7.64 min Scan# 2010
Delta R.T. -0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55

Tgt Ion: 92 Resp: 7828
Ion Ratio Lower Upper
92 100
91 186.9 139.8 209.8



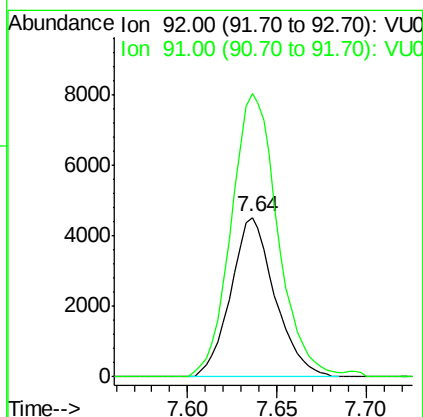



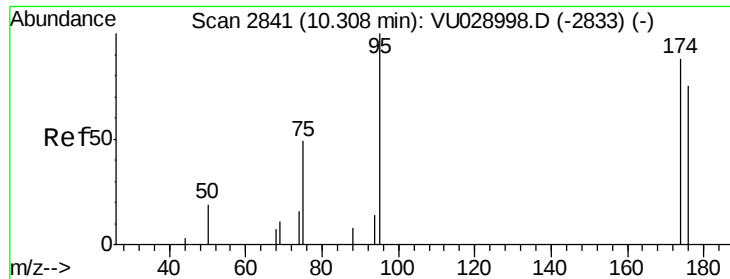

#62
4-Bromofluorobenzene
Concen: 45.500 ug/l
RT: 10.30 min Scan# 2840
Delta R.T. -0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55




Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM


Tot Ion: 95 Resp: 80827
Ion Ratio Lower Upper
95 100
174 82.2 0.0 170.6
176 80.1 0.0 165.0

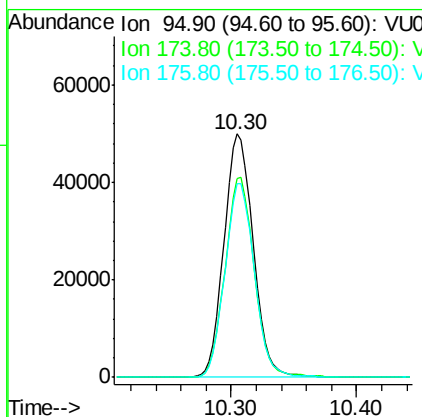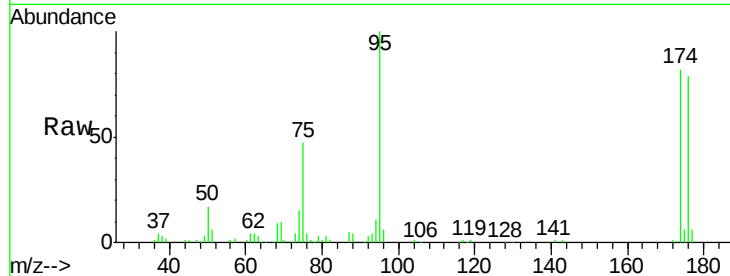

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2461
Delta R.T. -0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55

Tgt Ion: 117 Resp: 179988
Ion Ratio Lower Upper
117 100
82 55.2 43.9 65.9
119 31.9 26.0 39.0

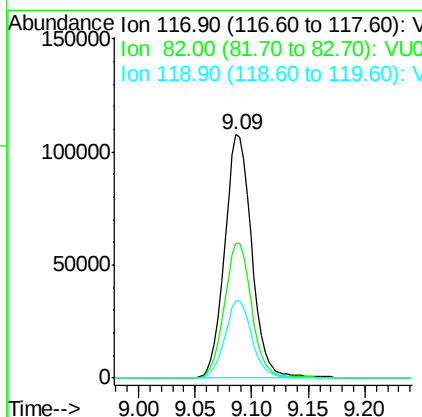



#67

Ethyl Benzene

Concen: 0.256 ug/l

RT: 9.25 min Scan# 2513

Delta R.T. 0.01 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :


COMP-1-DRUM

Tot Ion: 91 Resp: 1727




Ion Ratio Lower Upper

91 100

106 28.9 25.0 37.4

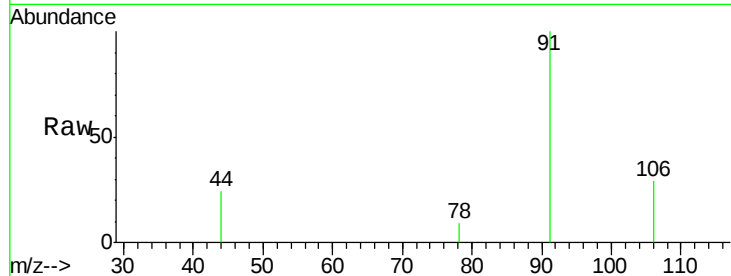

Abundance Ion 91.00 (90.70 to 91.70): VU028998.D (-2502) (-)

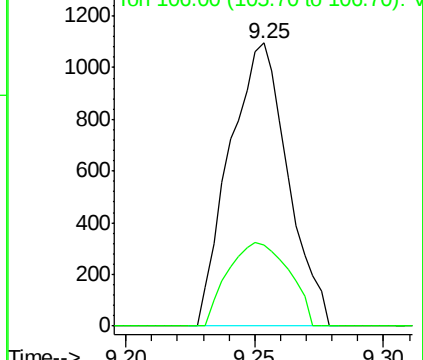

#68

m/p-Xylenes

Concen: 0.847 ug/l

RT: 9.37 min Scan# 2550

Delta R.T. -0.00 min

Lab File: VU029039.D


Acq: 04 Jan 2019 19:55

Tgt Ion: 106 Resp: 2218



Ion Ratio Lower Upper


106 100

91 206.3 161.7 242.5



Abundance Ion 106.00 (105.70 to 106.70): VU028998.D (-2541) (-)

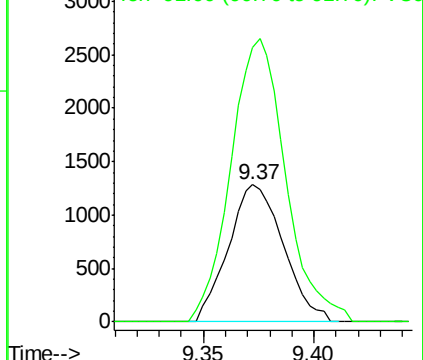







#69
o-Xylene
Concen: 0.400 ug/l
RT: 9.78 min Scan# 2676
Delta R.T. -0.00 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55

Instrument :
MSVOA_U
ClientSampleId :
COMP-1-DRUM

Tot Ion:106 Resp: 1009
Ion Ratio Lower Upper
106 100
91 208.8 106.1 318.3

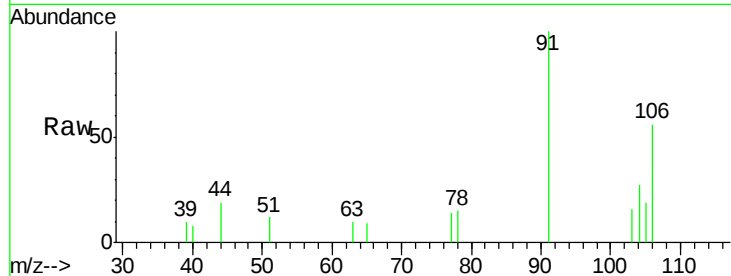


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VU0


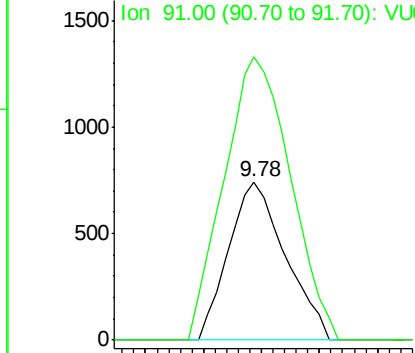



#70
Styrene
Concen: 0.537 ug/l
RT: 9.80 min Scan# 2682
Delta R.T. 0.01 min
Lab File: VU029039.D
Acq: 04 Jan 2019 19:55

Tgt Ion:104 Resp: 2218
Ion Ratio Lower Upper
104 100
78 45.9 38.6 58.0
103 44.6 44.5 66.7



Abundance Ion 104.00 (103.70 to 104.70): V
Ion 78.00 (77.70 to 78.70): VU0
Ion 103.00 (102.70 to 103.70): V

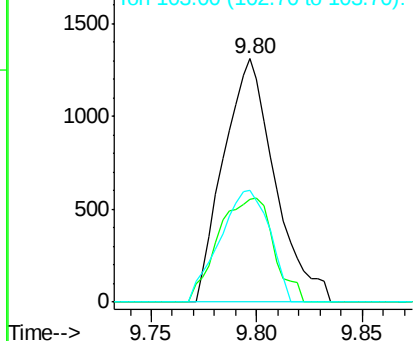

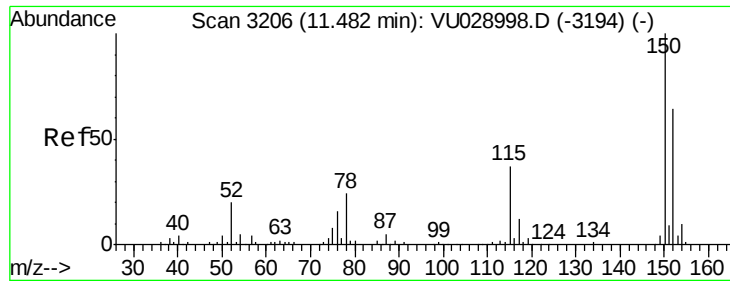

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.48 min Scan# 3206

Delta R.T. -0.00 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :

COMP-1-DRUM


Tot Ion:152 Resp: 75894

Ion Ratio Lower Upper

152 100

115 55.1 40.1 120.3




150 155.4 0.0 345.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

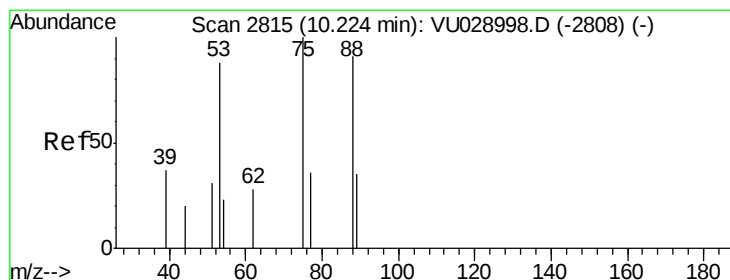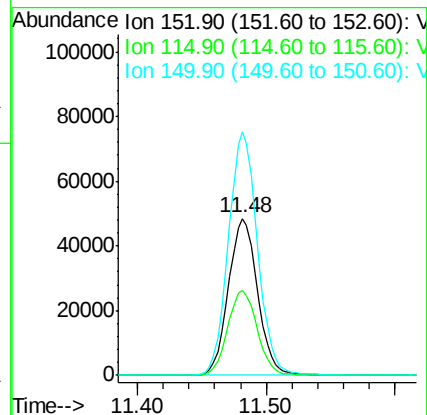

#76

1,2,3-Trichloropropane

Concen: 20.156 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.19 min

Lab File: VU029039.D


Acq: 04 Jan 2019 19:55

Tgt Ion: 75 Resp: 37481

Ion Ratio Lower Upper



75 100


77 1.2 20.9 62.8#



Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 77.00 (76.70 to 77.70): VU0

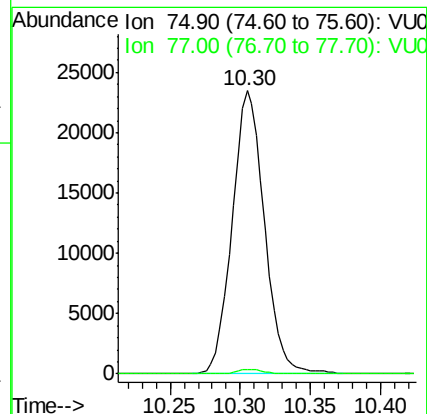

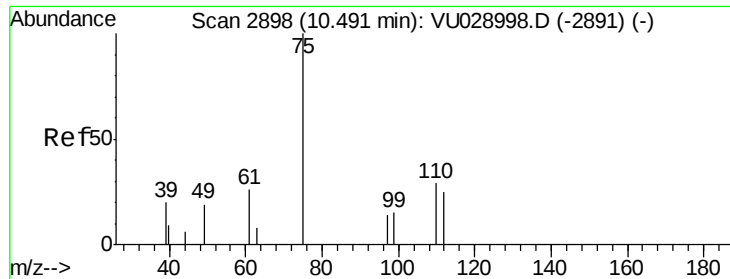

#81

trans-1,4-Dichloro-2-butene

Concen: 51.984 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.21 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :

COMP-1-DRUM


Tot Ion: 75 Resp: 37481

Ion Ratio Lower Upper

75 100

53 0.0 0.0 0.0


89 0.0 0.0 0.0

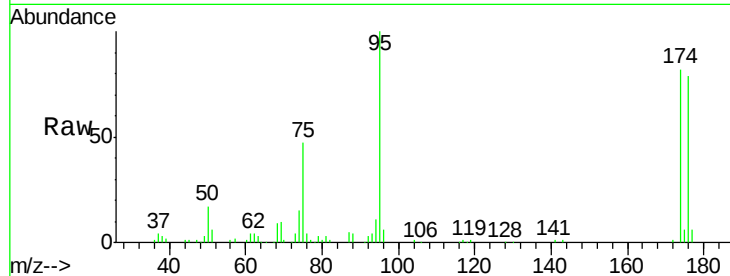



Abundance Ion 74.90 (74.60 to 75.60): VU028998.D (-2891) (-)

Ion 53.00 (52.70 to 53.70): VU028998.D (-2891) (-)

Ion 88.90 (88.60 to 89.60): VU028998.D (-2891) (-)

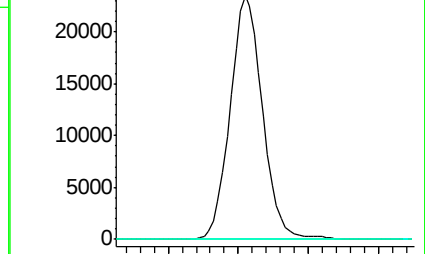

Time-->

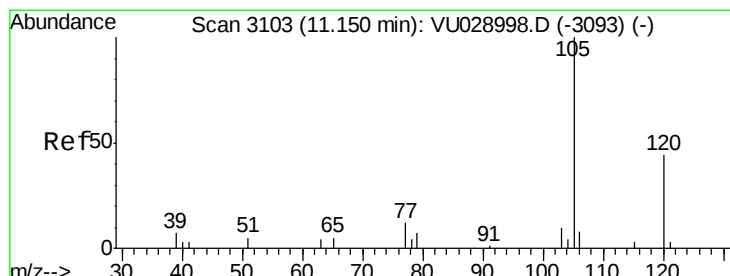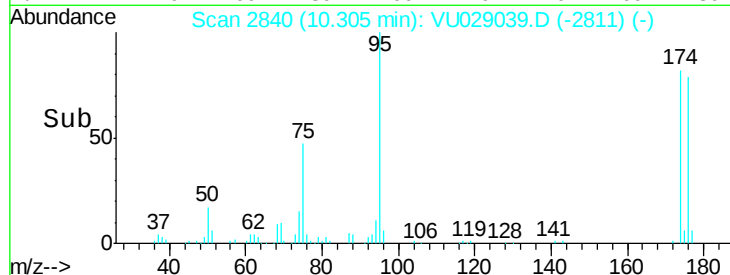

#84

1,2,4-Trimethylbenzene

Concen: 0.421 ug/l

RT: 11.15 min Scan# 3102

Delta R.T. -0.00 min

Lab File: VU029039.D


Acq: 04 Jan 2019 19:55

Tgt Ion: 105 Resp: 1971

Ion Ratio Lower Upper


105 100

120 38.0 23.1 69.3

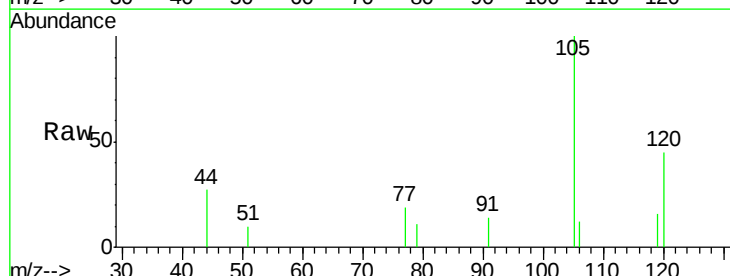



Abundance Ion 105.00 (104.70 to 105.70): VU028998.D (-3093) (-)

Ion 120.00 (119.70 to 120.70): VU028998.D (-3093) (-)

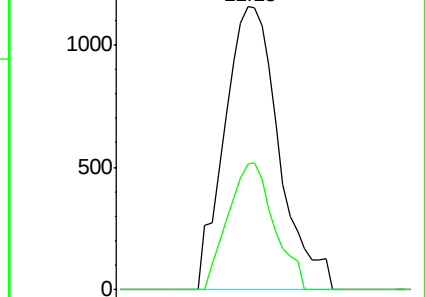

Time-->

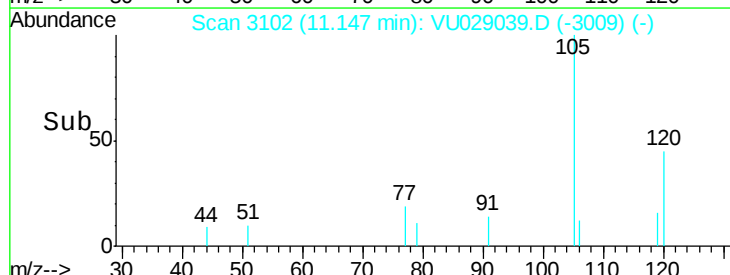

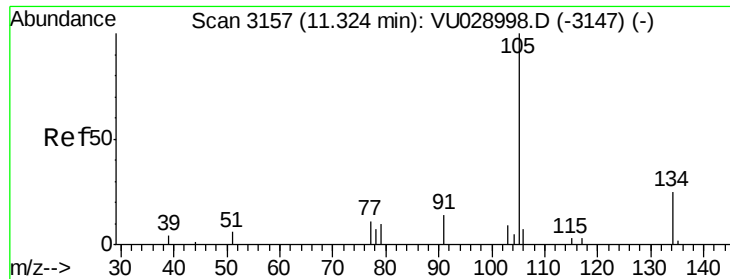

#85

sec-Butylbenzene

Concen: 0.352 ug/l

RT: 11.15 min Scan# 3102

Delta R.T. -0.17 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :


COMP-1-DRUM

Tot Ion:105 Resp: 1971

Ion Ratio Lower Upper




105 100

134 0.0 9.7 29.1#

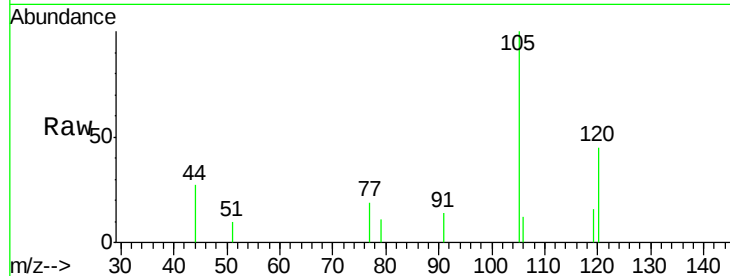

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 134.00 (133.70 to 134.70): V

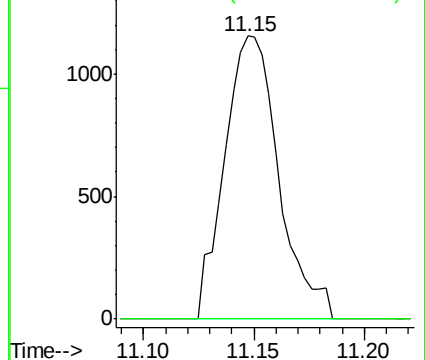

#90

Hexachloroethane

Concen: 0.727 ug/l

RT: 11.98 min Scan# 3362

Delta R.T. -0.16 min

Lab File: VU029039.D


Acq: 04 Jan 2019 19:55

Tgt Ion:117 Resp: 583

Ion Ratio Lower Upper



117 100


201 0.0 42.4 127.3#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

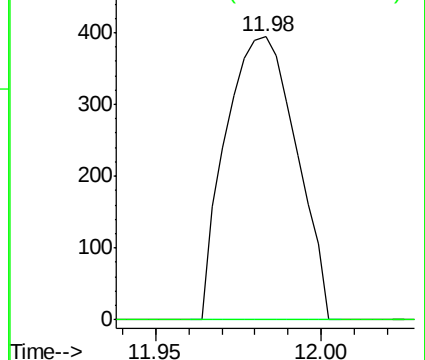

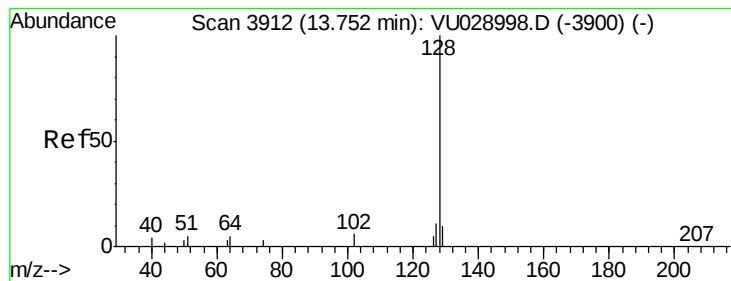

#95

Naphthalene

Concen: 5.639 ug/l

RT: 13.74 min Scan# 3909

Delta R.T. 0.00 min

Lab File: VU029039.D

Acq: 04 Jan 2019 19:55

Instrument :

MSVOA_U

ClientSampleId :

COMP-1-DRUM


Tot Ion:128 Resp: 33118

Ion Ratio Lower Upper

128 100

127 12.5 10.1 15.1

129 10.1 8.5 12.7

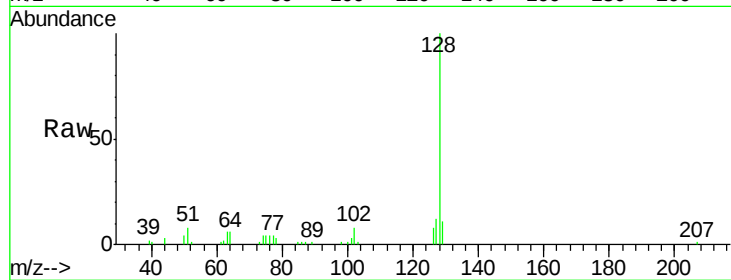

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

