

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010519\
 Data File : VU029025.D
 Acq On : 04 Jan 2019 14:15
 Operator : MD/SY
 Sample : K1056-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 05 04:06:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 04 02:22:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	116087	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	196156	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	181114	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	70748	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	74959	52.23	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	104.46%	
35) Dibromofluoromethane	4.88	113	65456	51.48	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	102.96%	
50) Toluene-d8	7.56	98	248804	49.56	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	99.12%	
62) 4-Bromofluorobenzene	10.30	95	77263	42.83	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	85.66%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010519\
Data File : VU029025.D
Acq On : 04 Jan 2019 14:15
Operator : MD/SY
Sample : K1056-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 05 04:06:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Fri Jan 04 02:22:53 2019
Response via : Initial Calibration

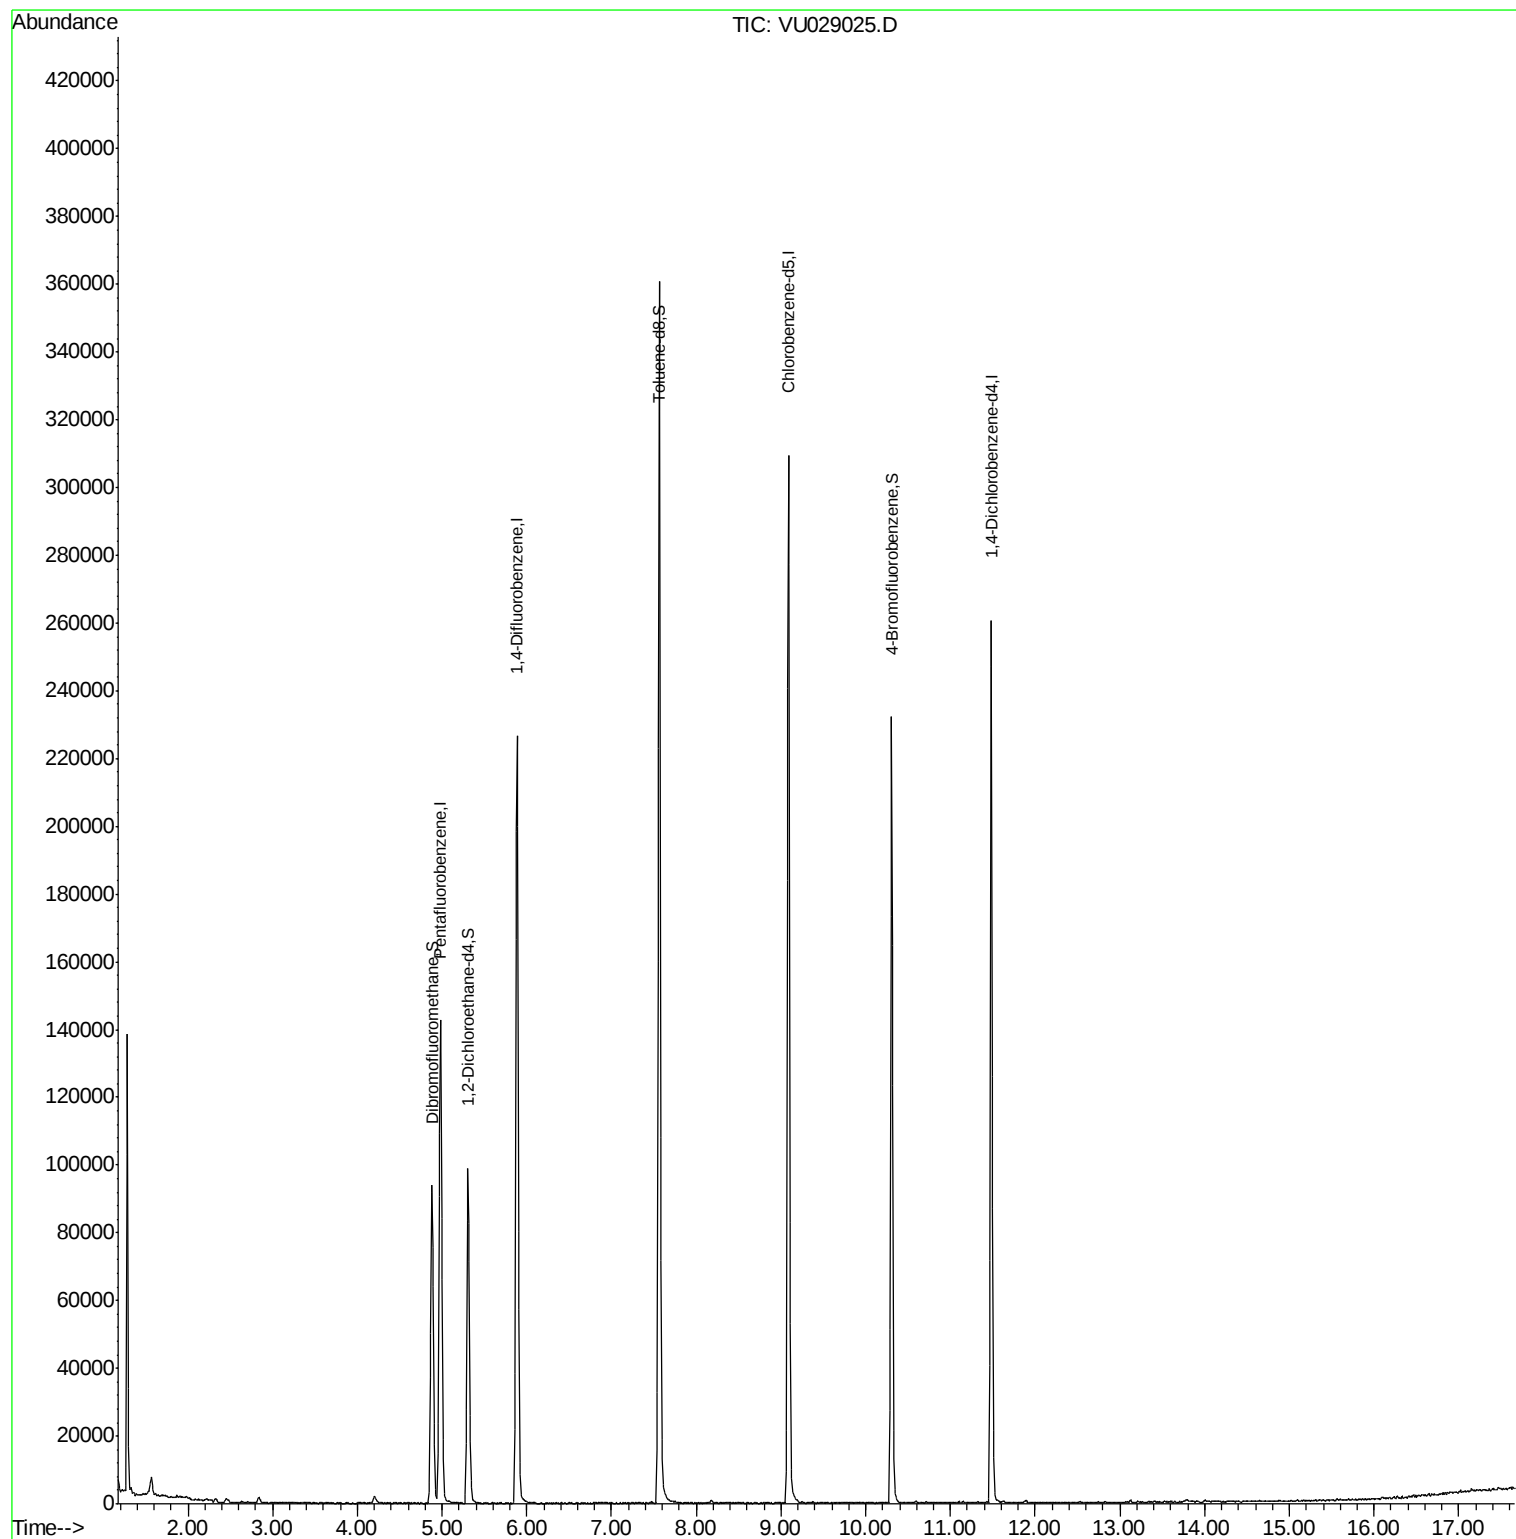

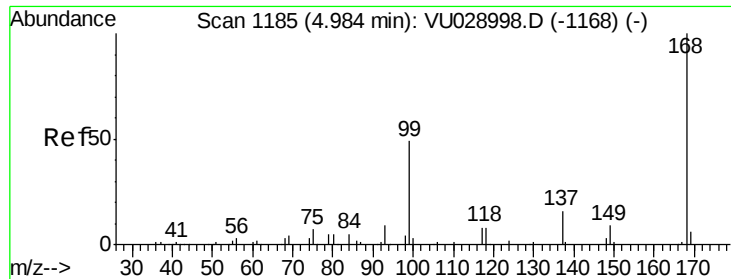

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1184

Delta R.T. 0.00 min

Lab File: VU029025.D

Acq: 04 Jan 2019 14:15

Instrument :

MSVOA_U

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion:168 Resp: 116087

Ion Ratio Lower Upper

168 100

99 51.5 42.0 63.0



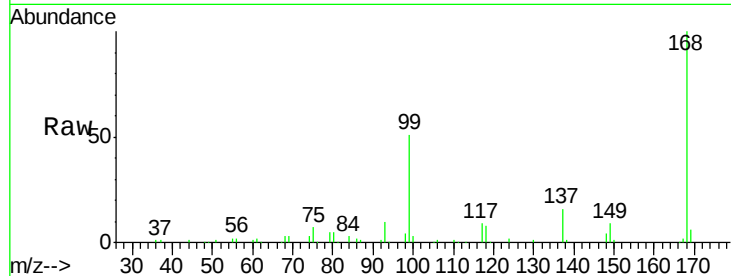


Abundance Ion 167.90 (167.60 to 168.60): VU028998.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028998.D (-1168) (-)

4.98

Time-->

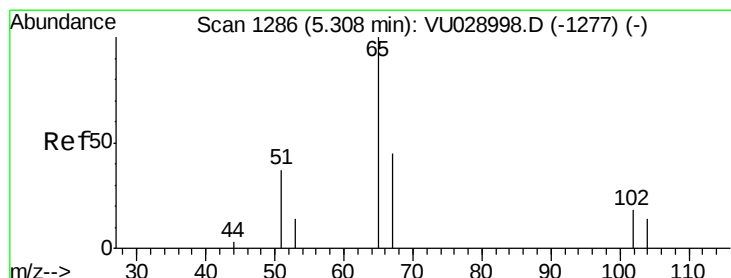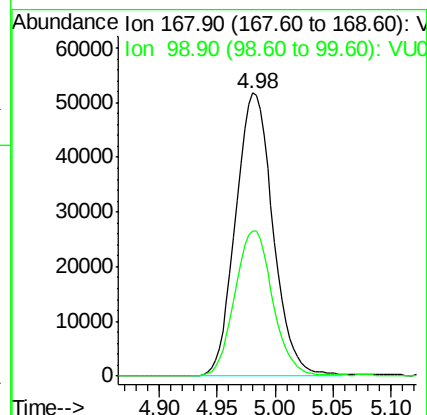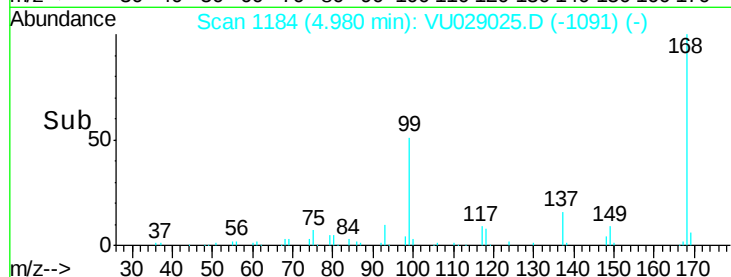

#33

1,2-Dichloroethane-d4

Concen: 52.234 ug/l

RT: 5.31 min Scan# 1285

Delta R.T. 0.00 min

Lab File: VU029025.D


Acq: 04 Jan 2019 14:15

Tgt Ion: 65 Resp: 74959

Ion Ratio Lower Upper

65 100

67 56.5 0.0 111.0


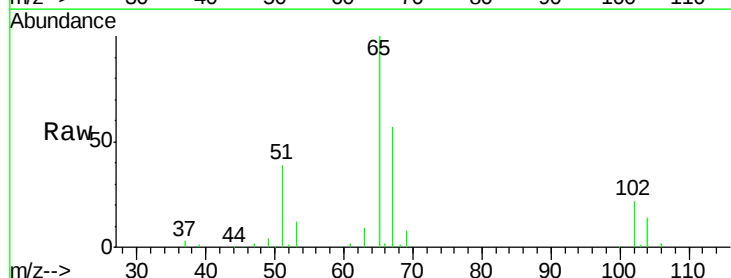



Abundance Ion 64.90 (64.60 to 65.60): VU028998.D (-1277) (-)

Ion 66.90 (66.60 to 67.60): VU028998.D (-1277) (-)

5.31

Time-->

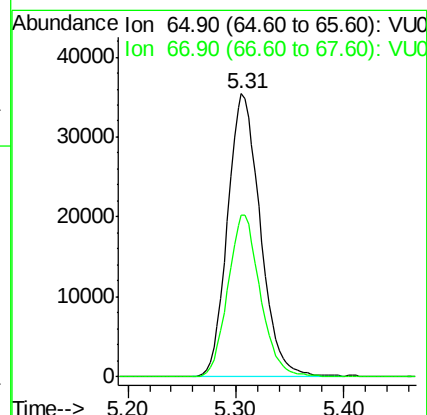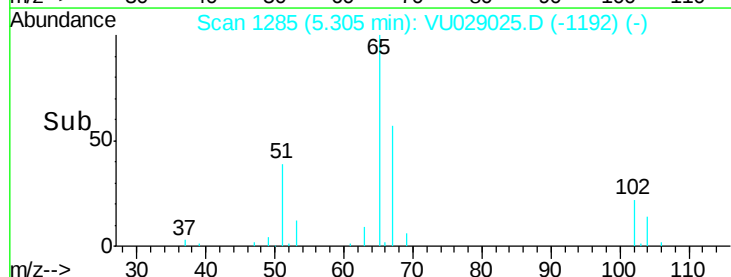

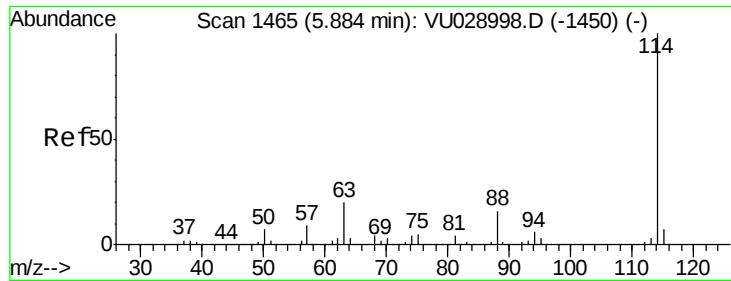

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.88 min Scan# 1465

Delta R.T. 0.00 min

Lab File: VU029025.D

Acq: 04 Jan 2019 14:15

Instrument :

MSVOA_U

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6


Tot Ion:114 Resp: 196156

Ion Ratio Lower Upper

114 100

63 21.4 0.0 40.2




88 16.1 0.0 30.4

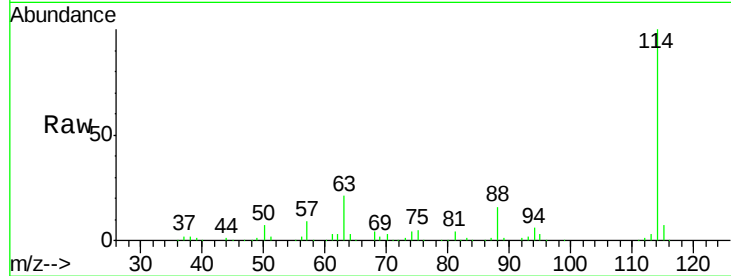

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

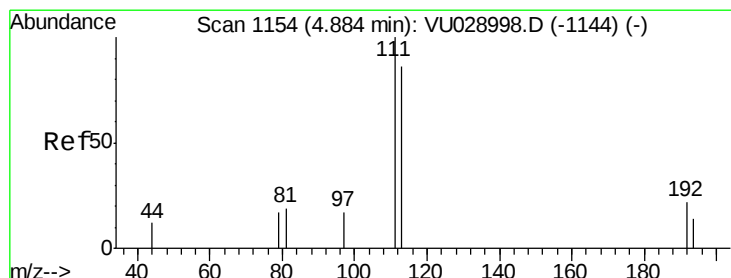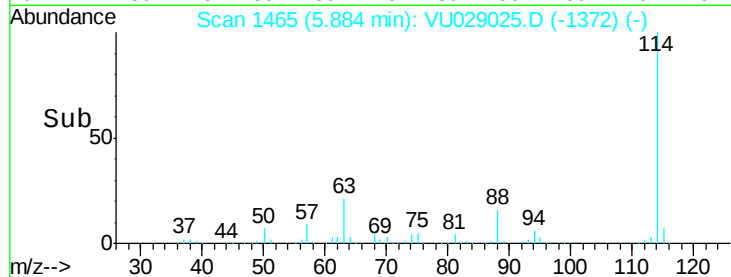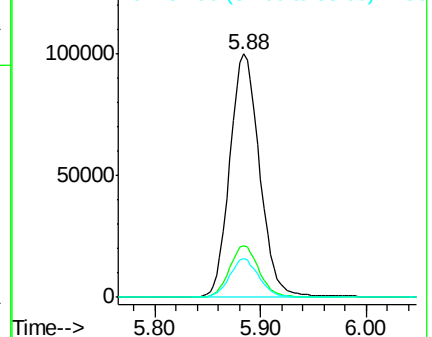

#35

Dibromofluoromethane

Concen: 51.478 ug/l

RT: 4.88 min Scan# 1153

Delta R.T. 0.00 min

Lab File: VU029025.D

Acq: 04 Jan 2019 14:15


Tgt Ion:113 Resp: 65456

Ion Ratio Lower Upper

113 100

111 104.6 81.4 122.2



192 21.4 16.8 25.2

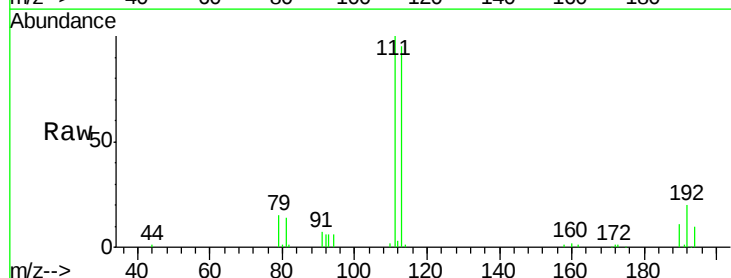


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

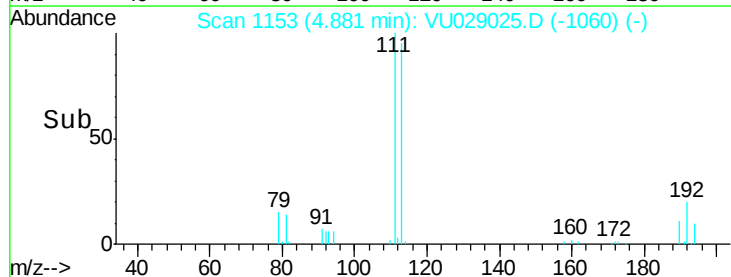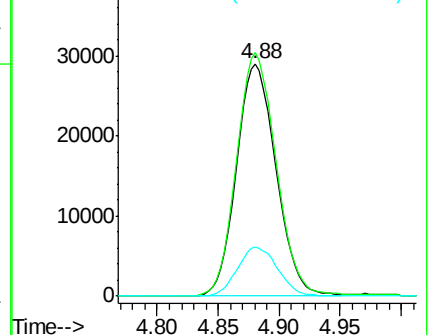


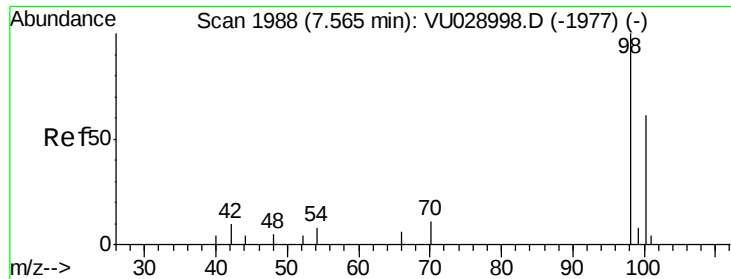


#50
Toluene-d8
Concen: 49.564 ug/l
RT: 7.56 min Scan# 1987
Delta R.T. 0.00 min
Lab File: VU029025.D
Acq: 04 Jan 2019 14:15

Instrument :
MSVOA_U
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6



Tot Ion: 98 Resp: 248804
Ion Ratio Lower Upper
98 100
100 64.0 51.6 77.4

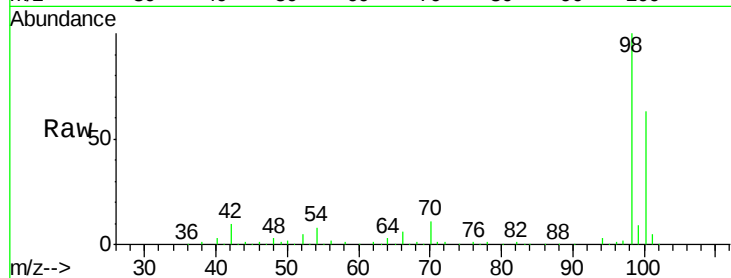

Abundance Ion 98.00 (97.70 to 98.70): VU028998.D (-1977) (-)
Ion 100.00 (99.70 to 100.70): VU028998.D (-1977) (-)

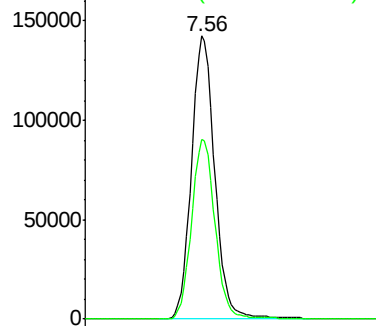


Time-->

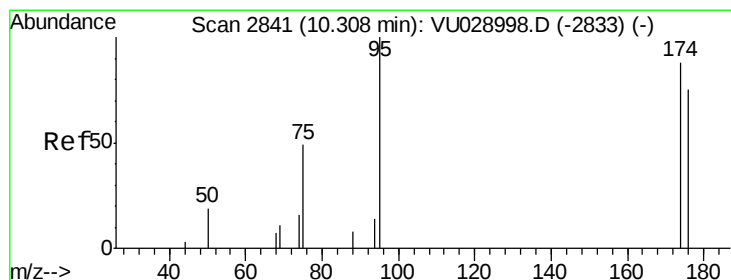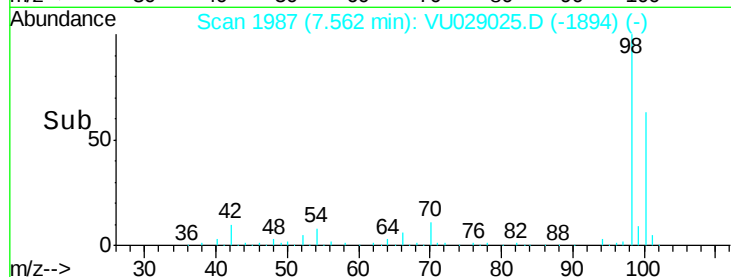


#62
4-Bromofluorobenzene
Concen: 42.827 ug/l
RT: 10.30 min Scan# 2840
Delta R.T. 0.00 min
Lab File: VU029025.D
Acq: 04 Jan 2019 14:15


Tgt Ion: 95 Resp: 77263
Ion Ratio Lower Upper
95 100
174 86.7 0.0 170.6
176 82.6 0.0 165.0

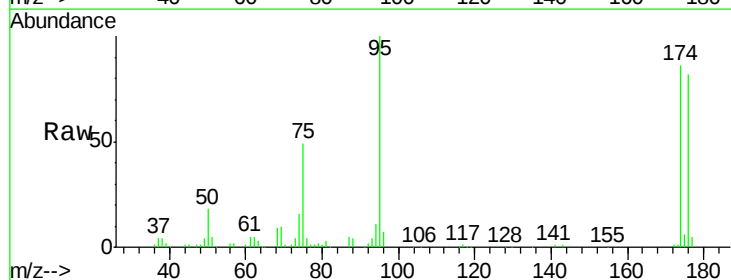


Abundance Ion 94.90 (94.60 to 95.60): VU028998.D (-2833) (-)
Ion 173.80 (173.50 to 174.50): VU028998.D (-2833) (-)
Ion 175.80 (175.50 to 176.50): VU028998.D (-2833) (-)

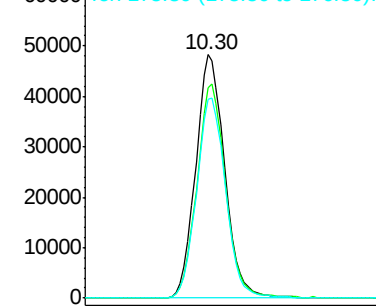

Time-->

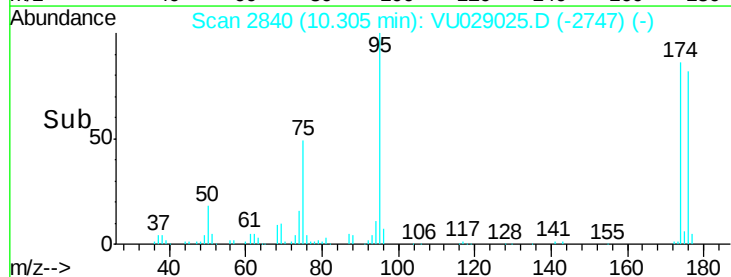


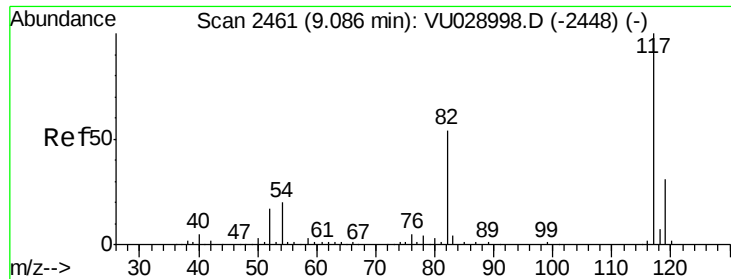


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. 0.00 min
Lab File: VU029025.D
Acq: 04 Jan 2019 14:15

Instrument :
MSVOA_U
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6



Tot Ion:117 Resp: 181114
Ion Ratio Lower Upper
117 100
82 56.2 43.9 65.9
119 31.8 26.0 39.0

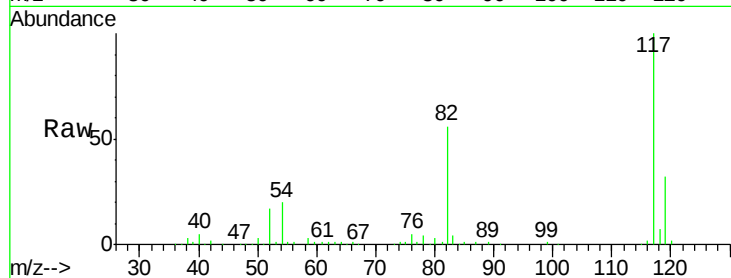

Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

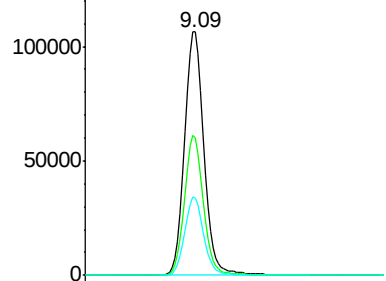


Time-->

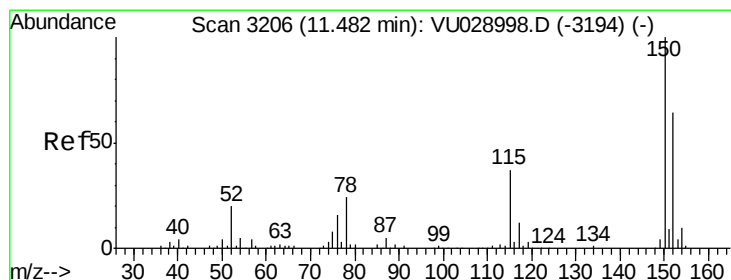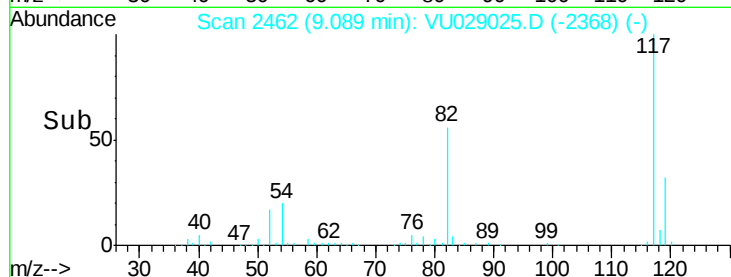


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3206
Delta R.T. 0.00 min
Lab File: VU029025.D
Acq: 04 Jan 2019 14:15

Tgt Ion:152 Resp: 70748
Ion Ratio Lower Upper
152 100
115 56.6 40.1 120.3
150 158.3 0.0 345.2

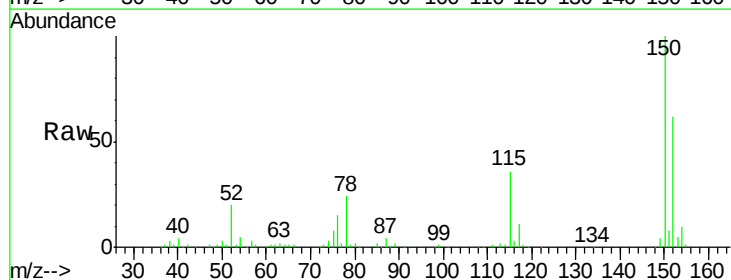

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

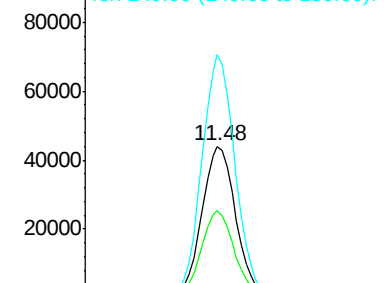

Time-->

