

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010519\
 Data File : VU029026.D
 Acq On : 04 Jan 2019 14:39
 Operator : MD/SY
 Sample : K1056-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Jan 05 04:09:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 04 02:22:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	112667	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	190638	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	166993	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	60692	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.30	65	73275	52.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.22%	
35) Dibromofluoromethane	4.88	113	64662	52.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.66%	
50) Toluene-d8	7.56	98	237792	48.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.48%	
62) 4-Bromofluorobenzene	10.30	95	70237	40.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	80.12%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010519\
Data File : VU029026.D
Acq On : 04 Jan 2019 14:39
Operator : MD/SY
Sample : K1056-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Jan 05 04:09:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Fri Jan 04 02:22:53 2019
Response via : Initial Calibration

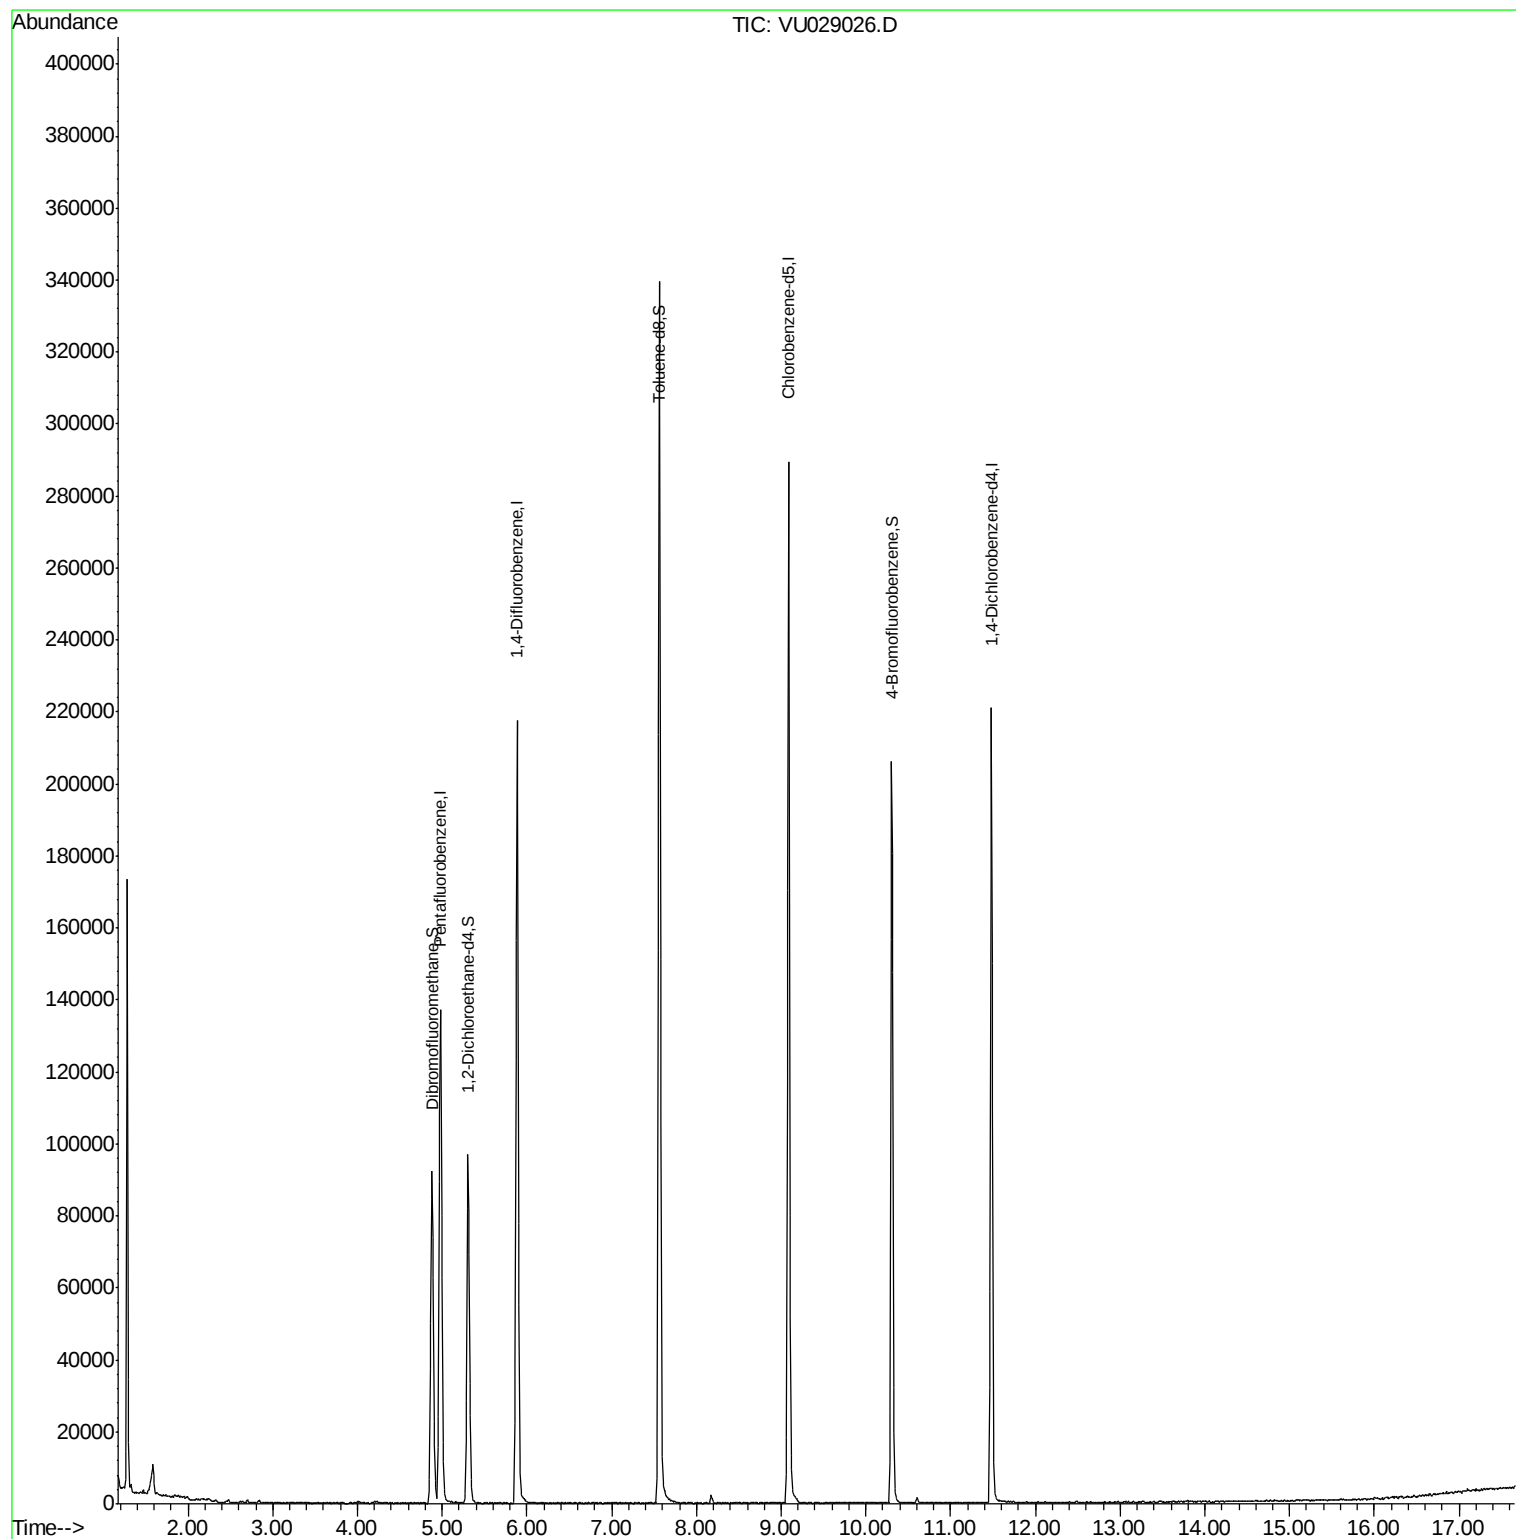

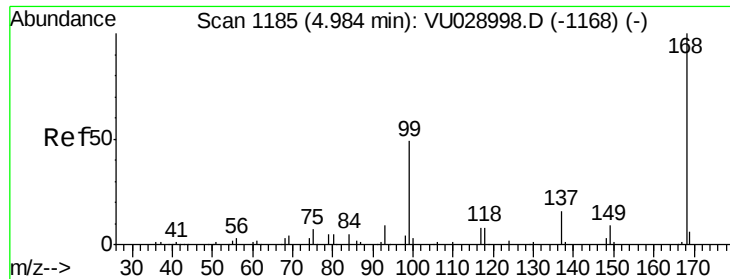

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1184

Delta R.T. 0.00 min

Lab File: VU029026.D

Acq: 04 Jan 2019 14:39

Instrument :

MSVOA_U

ClientSampleId :


STORAGE-BLANK-WATER-REF-5

Tot Ion:168 Resp: 112667

Ion Ratio Lower Upper

168 100

99 51.4 42.0 63.0

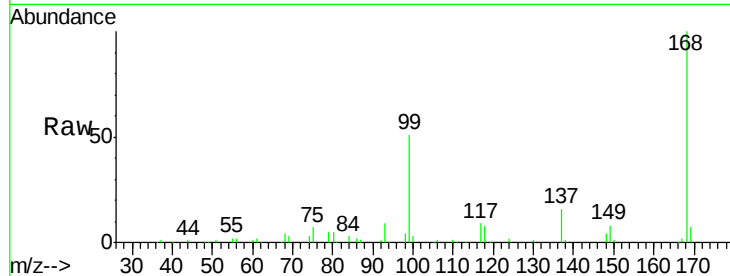

Abundance Ion 167.90 (167.60 to 168.60): VU028998.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028998.D (-1168) (-)

4.98

50000

40000

30000



20000

10000

0

4.90 4.95 5.00 5.05

Time-->

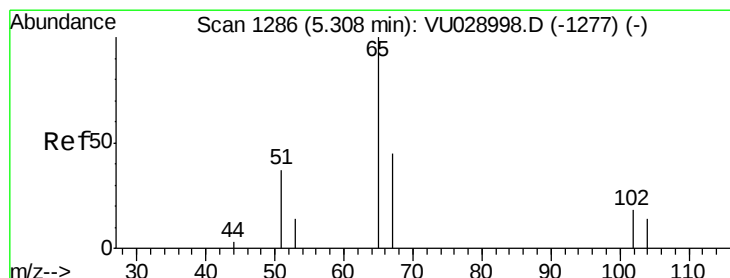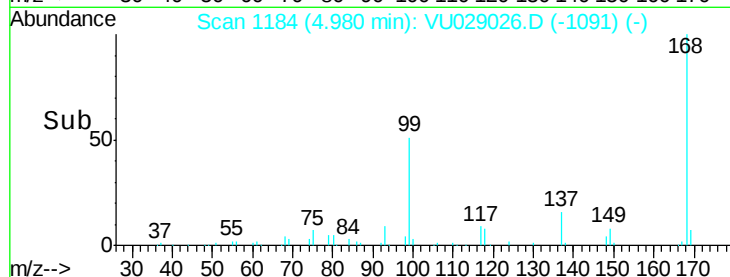

#33

1,2-Dichloroethane-d4

Concen: 52.610 ug/l

RT: 5.30 min Scan# 1285

Delta R.T. 0.00 min

Lab File: VU029026.D


Acq: 04 Jan 2019 14:39

Tgt Ion: 65 Resp: 73275

Ion Ratio Lower Upper

65 100

67 55.4 0.0 111.0

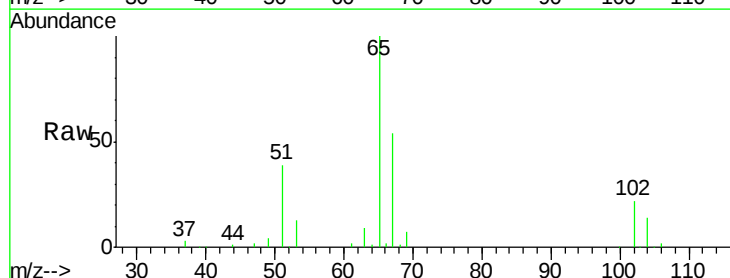

Abundance Ion 64.90 (64.60 to 65.60): VU028998.D (-1277) (-)

Ion 66.90 (66.60 to 67.60): VU028998.D (-1277) (-)

5.30

40000

30000


20000


10000

0

5.25 5.30 5.35 5.40

Time-->

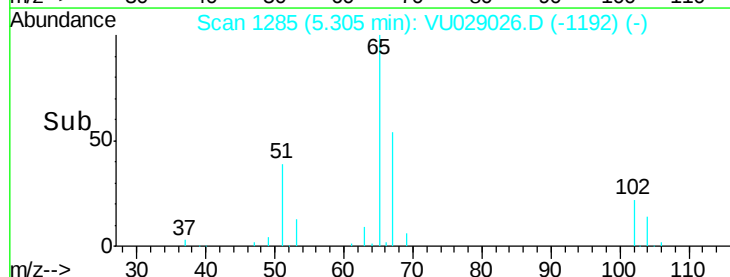


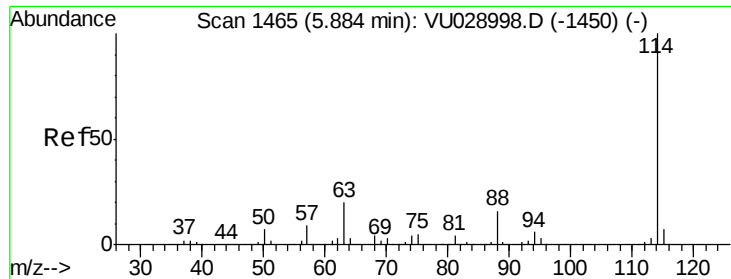




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. 0.00 min
 Lab File: VU029026.D
 Acq: 04 Jan 2019 14:39

Instrument :
 MSVOA_U
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Tot Ion:114 Resp: 190638
 Ion Ratio Lower Upper
 114 100
 63 20.5 0.0 40.2
 88 16.4 0.0 30.4

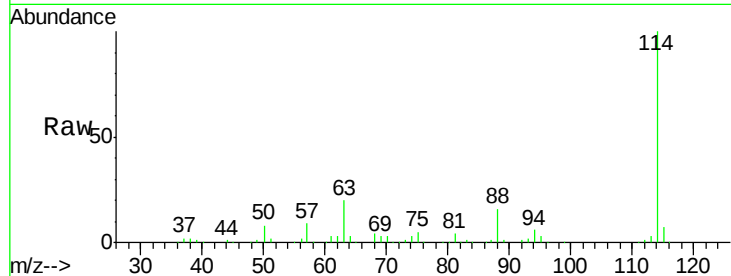


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

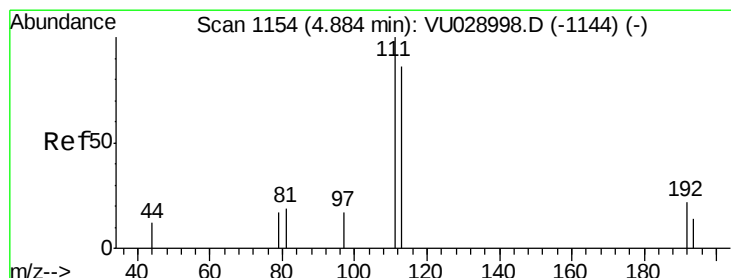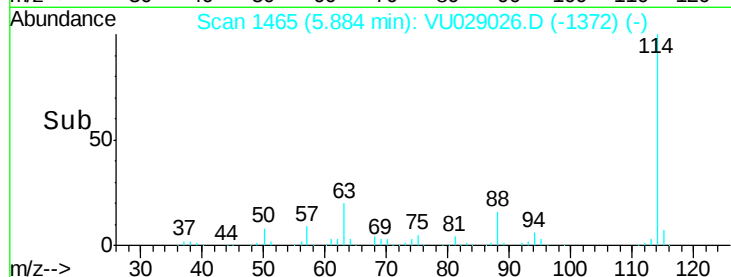
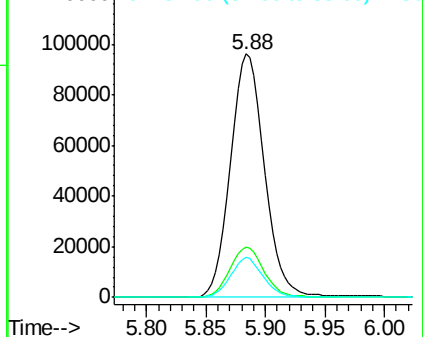



#35
 Dibromofluoromethane
 Concen: 52.325 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. 0.00 min
 Lab File: VU029026.D
 Acq: 04 Jan 2019 14:39

Tgt Ion:113 Resp: 64662
 Ion Ratio Lower Upper
 113 100
 111 103.1 81.4 122.2
 192 21.5 16.8 25.2

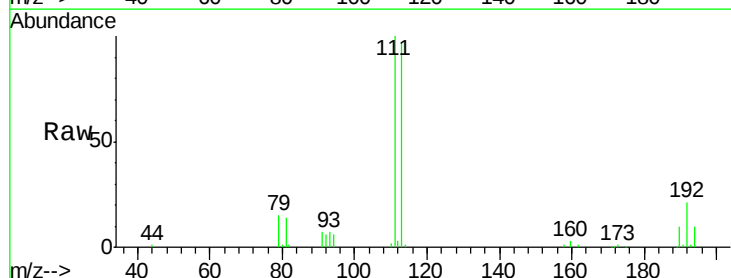

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

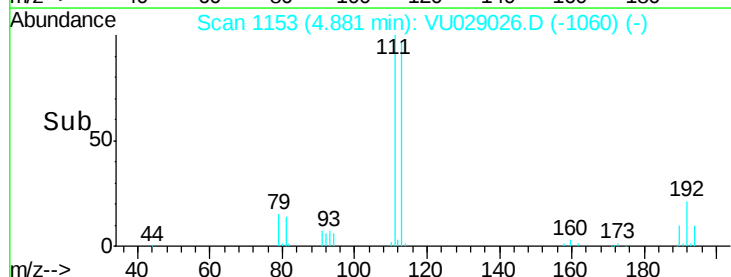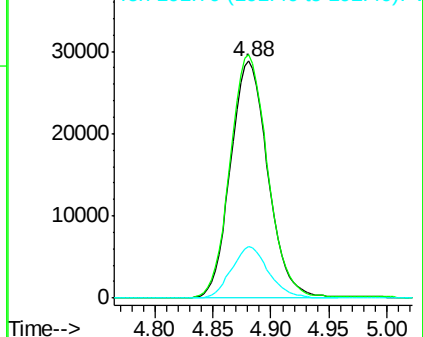

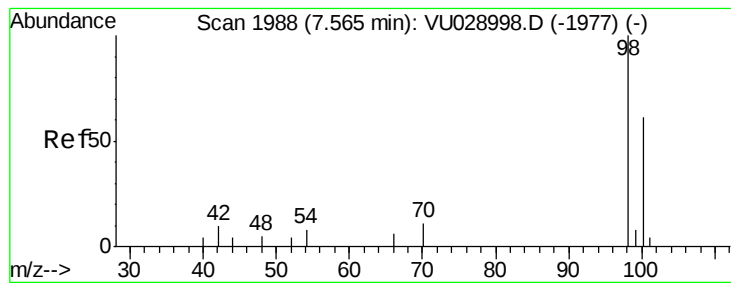

#50

Toluene-d8

Concen: 48.741 ug/l

RT: 7.56 min Scan# 1987

Delta R.T. 0.00 min

Lab File: VU029026.D

Acq: 04 Jan 2019 14:39

Instrument :

MSVOA_U

ClientSampleId :


STORAGE-BLANK-WATER-REF-5

Tot Ion: 98 Resp: 237792

Ion Ratio Lower Upper

98 100

100 63.9 51.6 77.4

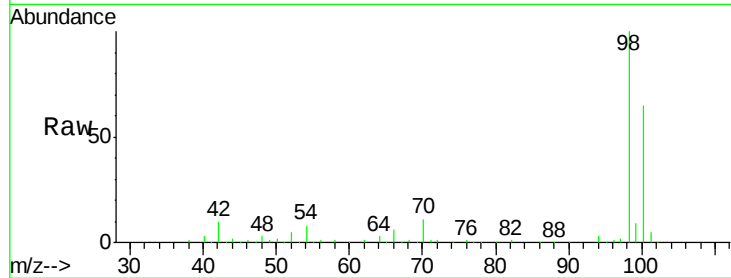

Abundance Ion 98.00 (97.70 to 98.70): VU028998.D (-1977) (-)

Ion 100.00 (99.70 to 100.70): VU028998.D (-1977) (-)

7.56



150000

100000

50000

0

Time-->

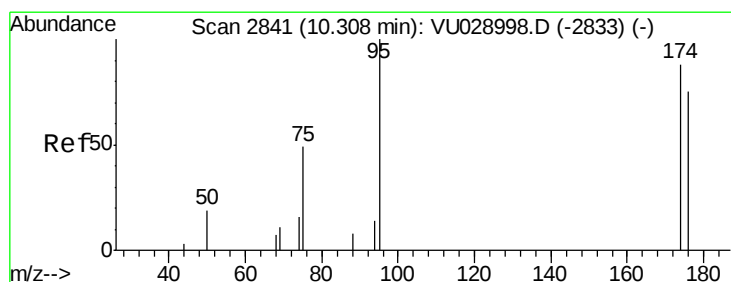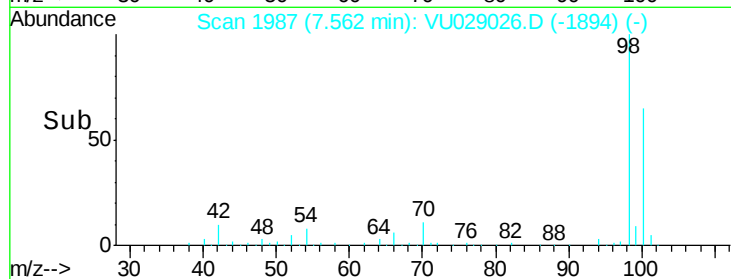

#62

4-Bromofluorobenzene

Concen: 40.060 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. 0.00 min

Lab File: VU029026.D

Acq: 04 Jan 2019 14:39


Tgt Ion: 95 Resp: 70237

Ion Ratio Lower Upper

95 100

174 85.6 0.0 170.6

176 81.5 0.0 165.0

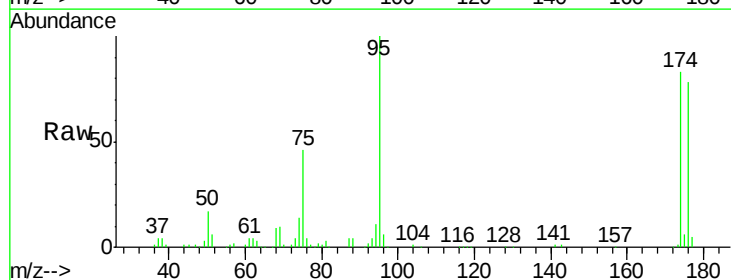

Abundance Ion 94.90 (94.60 to 95.60): VU028998.D (-2833) (-)

Ion 173.80 (173.50 to 174.50): VU028998.D (-2833) (-)

Ion 175.80 (175.50 to 176.50): VU028998.D (-2833) (-)

10.30

60000

50000

40000


30000


20000

10000

0

Time-->

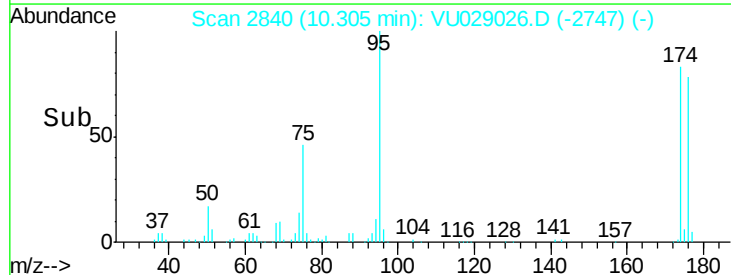


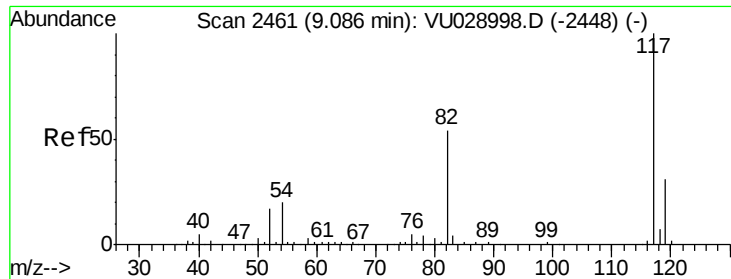




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2461
Delta R.T. 0.00 min
Lab File: VU029026.D
Acq: 04 Jan 2019 14:39

Instrument :
MSVOA_U
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tot Ion:117 Resp: 166993
Ion Ratio Lower Upper
117 100
82 57.1 43.9 65.9
119 32.2 26.0 39.0

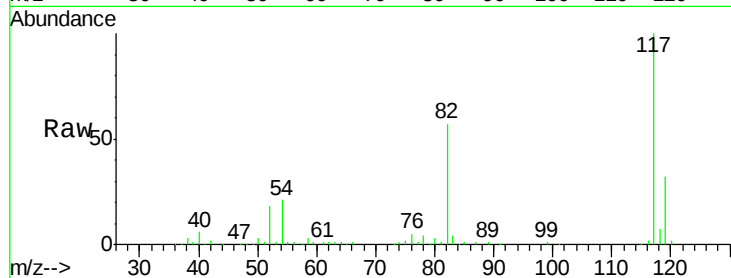


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

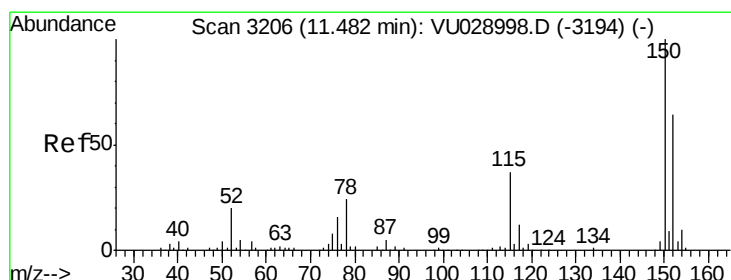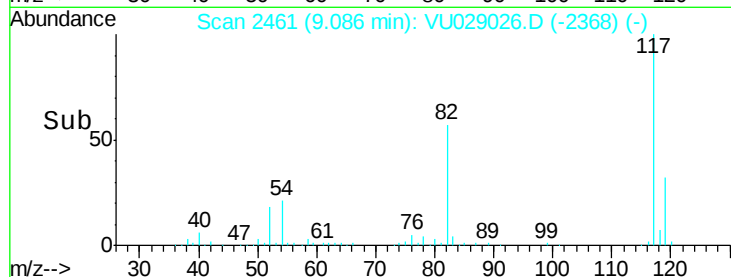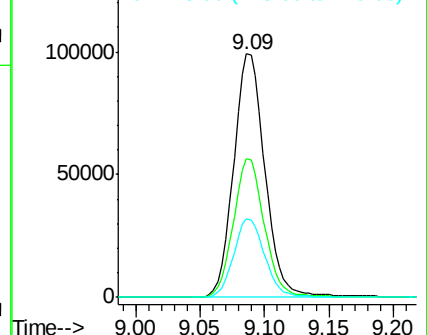

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3206
Delta R.T. 0.00 min
Lab File: VU029026.D
Acq: 04 Jan 2019 14:39

Tgt Ion:152 Resp: 60692
Ion Ratio Lower Upper
152 100
115 57.1 40.1 120.3
150 157.0 0.0 345.2

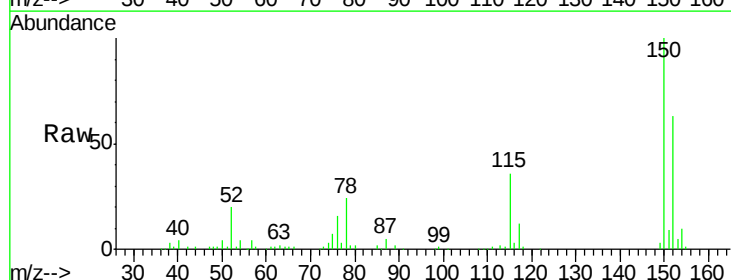

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

