


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010519\
 Data File : VU029021.D
 Acq On : 04 Jan 2019 12:26
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Title : SW846 8260
 Last Update : Fri Jan 04 02:22:53 2019

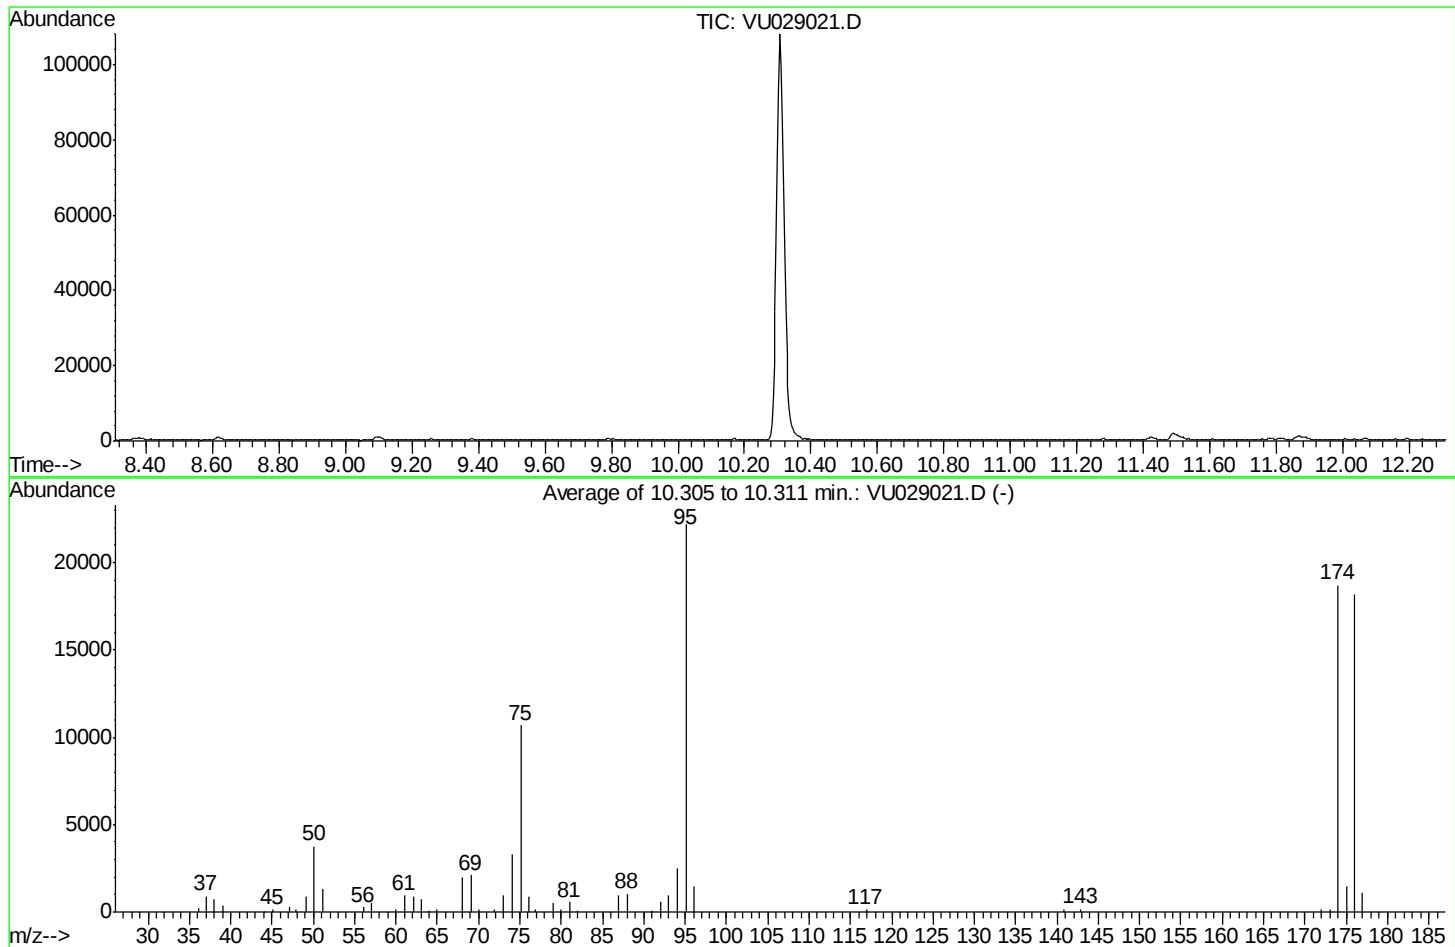

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	3769	PASS
75	95	30	60	48.2	10693	PASS
95	95	100	100	100.0	22194	PASS
96	95	5	9	6.6	1463	PASS
173	174	0.00	2	0.8	151	PASS
174	95	50	100	84.2	18693	PASS
175	174	5	9	7.8	1452	PASS
176	174	95	101	97.1	18152	PASS
177	176	5	9	6.2	1118	PASS