

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010522\
 Data File : VU046664.D
 Acq On : 05 Jan 2022 15:50
 Operator : SY/MD
 Sample : VU0105MBL01
 Misc : 5.00g/5.0mL/100uL/15.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Quant Time: Jan 06 03:03:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 06 02:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	196132	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	187679	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	92599	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	71851	41.981	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.960%		
7) Chloroethane-d5	1.919	69	54895	43.176	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.360%		
11) 1,1-Dichloroethene-d2	2.575	63	94903	32.602	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.200%		
21) 2-Butanone-d5	4.645	46	105928	84.565	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.560%		
24) Chloroform-d	5.070	84	123204	40.835	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.660%		
26) 1,2-Dichloroethane-d4	5.706	65	82964	43.357	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.720%		
32) Benzene-d6	5.732	84	256510	43.795	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.600%		
36) 1,2-Dichloropropane-d6	6.694	67	75906	42.475	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.940%		
41) Toluene-d8	7.902	98	228117	43.567	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.140%		
43) trans-1,3-Dichloroprop...	8.182	79	38322	44.511	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.020%		
47) 2-Hexanone-d5	8.639	63	84227	88.717	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.720%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	114084	41.219	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.440%		
66) 1,2-Dichlorobenzene-d4	12.195	152	89436	46.676	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.360%		
Target Compounds						Qvalue
14) Carbon disulfide	2.800	76	2253	0.583	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010522\
Data File : VU046664.D
Acq On : 05 Jan 2022 15:50
Operator : SY/MD
Sample : VU0105MBL01
Misc : 5.00g/5.0mL/100uL/15.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055


Quant Time: Jan 06 03:03:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 06 02:54:34 2022
Response via : Initial Calibration

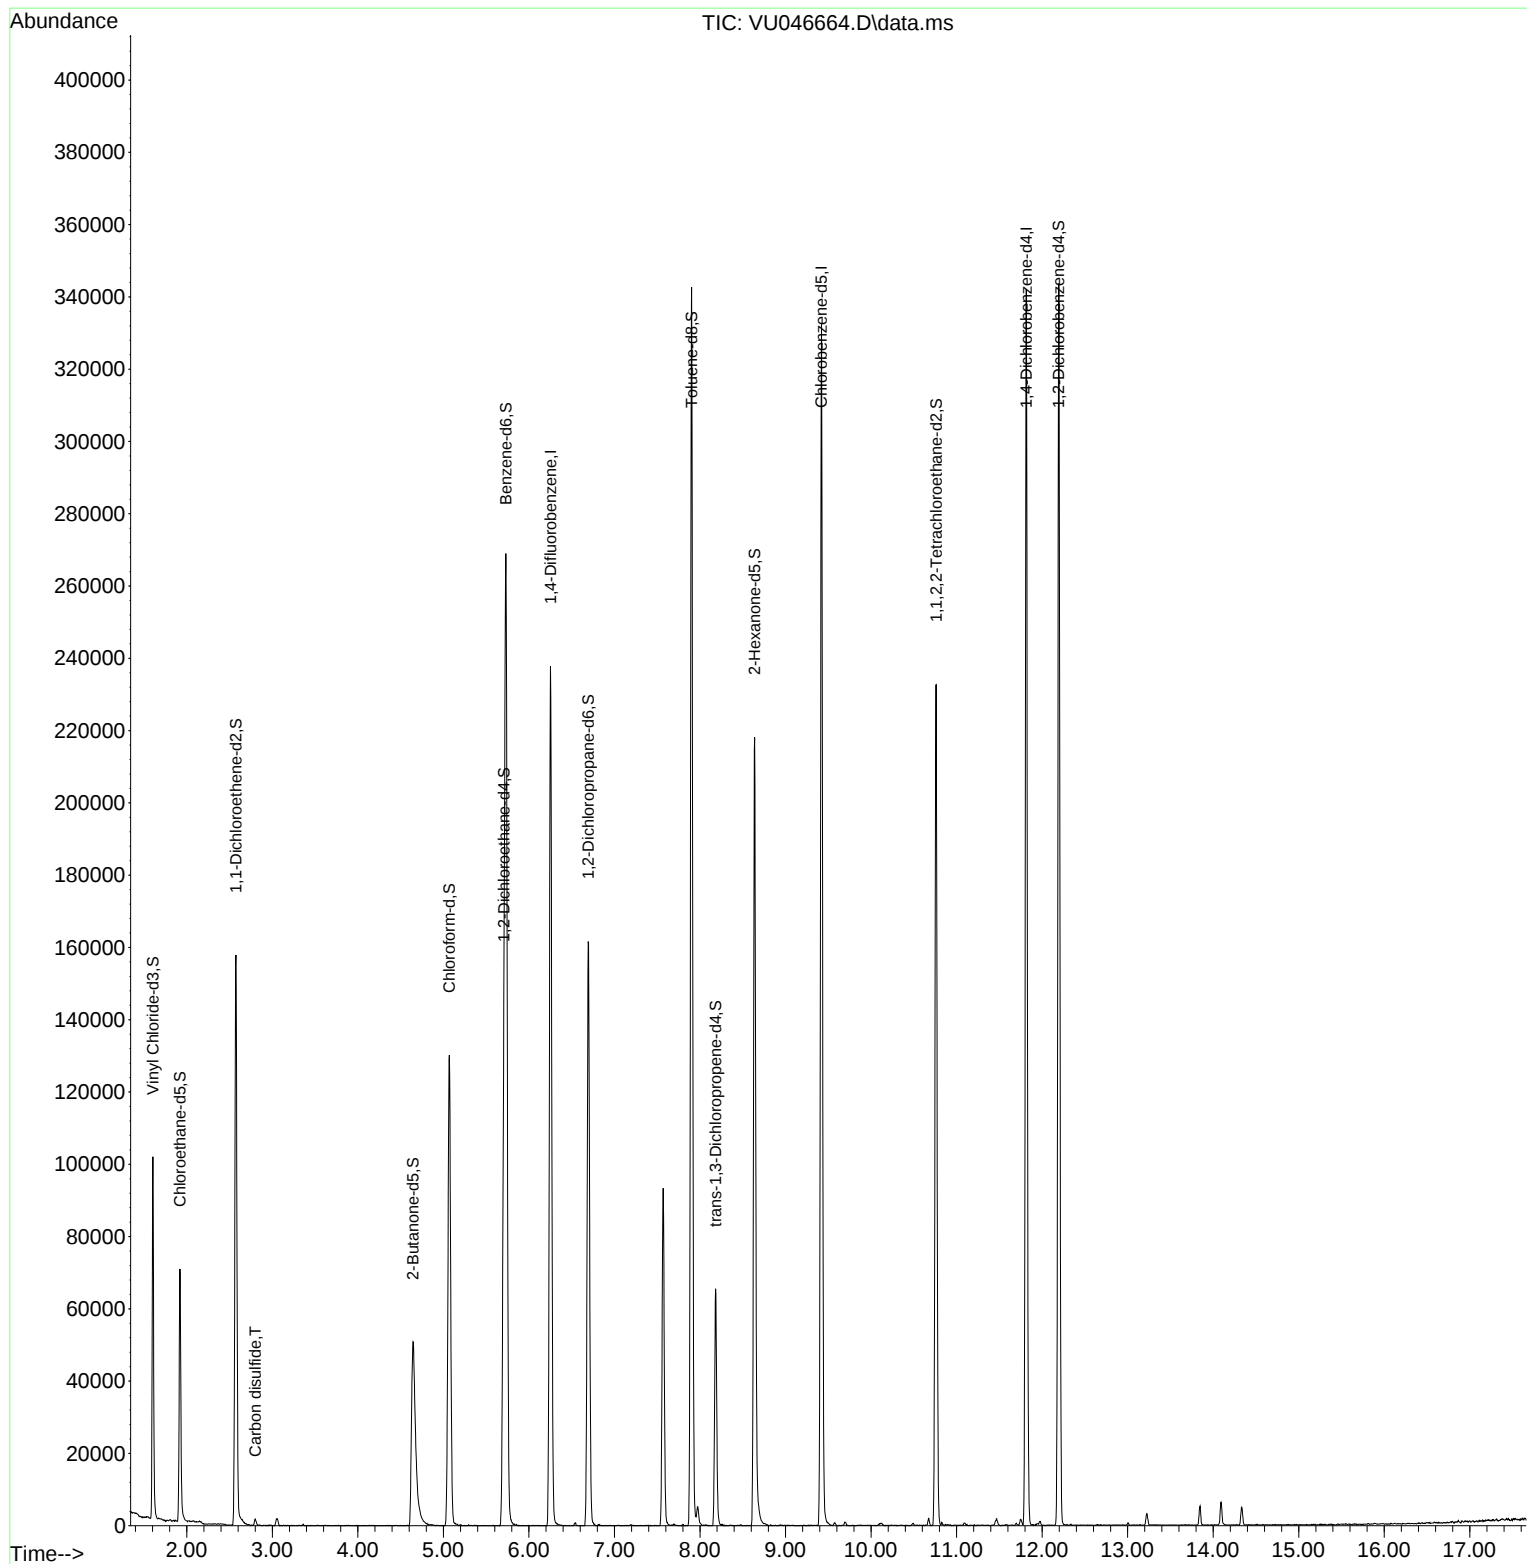

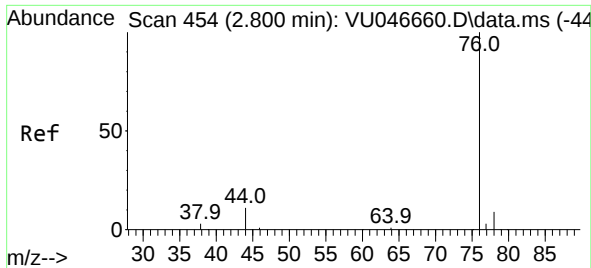

#14
Carbon disulfide
Concen: 0.583 ug/L
RT: 2.800 min Scan# 41
Delta R.T. -0.000 min
Lab File: VU046664.D
Acq: 05 Jan 2022 15:50

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

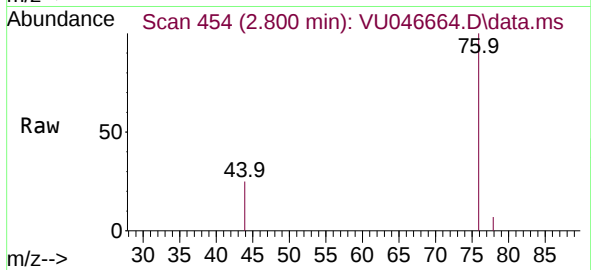

Tgt Ion: 76 Resp: 2253
Ion Ratio Lower Upper
76 100
78 7.1 7.1 10.7

