

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010522\
 Data File : VU046675.D
 Acq On : 05 Jan 2022 20:14
 Operator : SY/MD
 Sample : N1009-03
 Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGLF9

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 01/07/2022
 Supervised By :Semsettin Yesilyurt 01/11/2022

Quant Time: Jan 06 03:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 06 02:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	49404	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	50117	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.822	152	25253	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	125845	291.908	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 583.820%#			
7) Chloroethane-d5	1.919	69	95168m	297.154	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 594.300%#			
11) 1,1-Dichloroethene-d2	2.552	63	140740	191.944	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery = 383.880%#			
21) 2-Butanone-d5	4.671	46	168252	533.242	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery = 533.240%#			
24) Chloroform-d	5.067	84	222204	292.377	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 584.760%#			
26) 1,2-Dichloroethane-d4	5.703	65	151351	314.012	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 628.020%#			
32) Benzene-d6	5.726	84	459296	293.662	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 587.320%#			
36) 1,2-Dichloropropane-d6	6.694	67	140634	294.697	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 589.400%#			
41) Toluene-d8	7.899	98	430734	308.061	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 616.120%#			
43) trans-1,3-Dichloroprop...	8.186	79	74813	325.404	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 650.800%#			
47) 2-Hexanone-d5	8.687	63	159450	628.941	ug/L	0.05
Spiked Amount 100.000	Range 45 - 130		Recovery = 628.940%#			
56) 1,1,2,2-Tetrachloroeth...	10.774	84	215112	291.050	ug/L	0.02
Spiked Amount 50.000	Range 65 - 120		Recovery = 582.100%#			
66) 1,2-Dichlorobenzene-d4	12.201	152	172390	329.905	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 659.800%#			
Target Compounds						Qvalue
16) Methylene chloride	3.047	84	986	2.446	ug/L	91
42) Toluene	7.973	91	6495	4.131	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010522\
Data File : VU046675.D
Acq On : 05 Jan 2022 20:14
Operator : SY/MD
Sample : N1009-03
Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BGLF9

Quant Time: Jan 06 03:05:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 06 02:54:34 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 01/07/2022
Supervised By :Semsettin Yesilyurt 01/11/2022

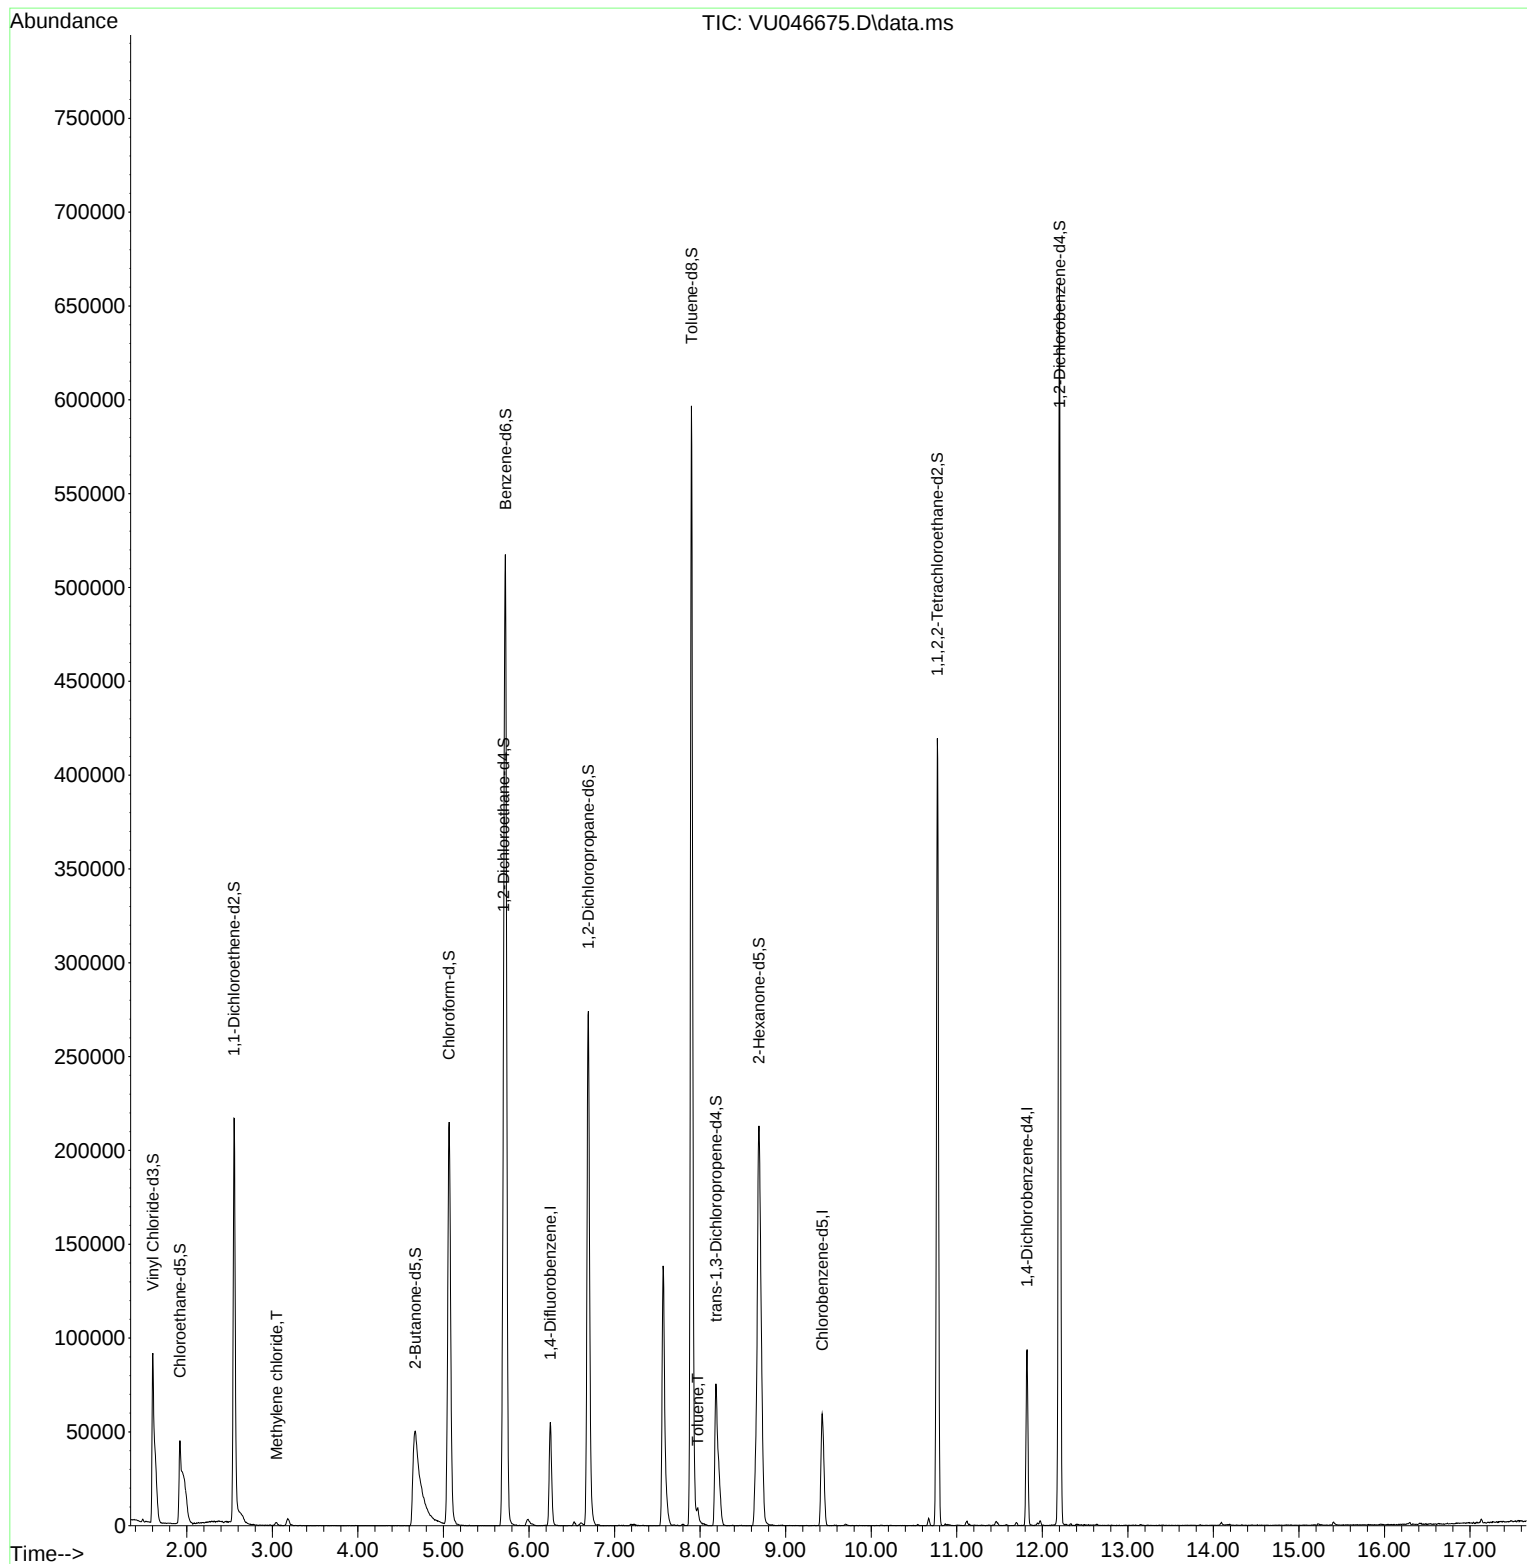

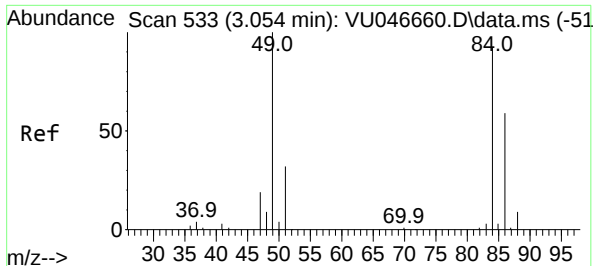

#16
Methylene chloride
Concen: 2.446 ug/L
RT: 3.047 min Scan# 51
Delta R.T. -0.006 min
Lab File: VU046675.D
Acq: 05 Jan 2022 20:14




Instrument :
MSVOA_U
ClientSampleId :
BGLF9

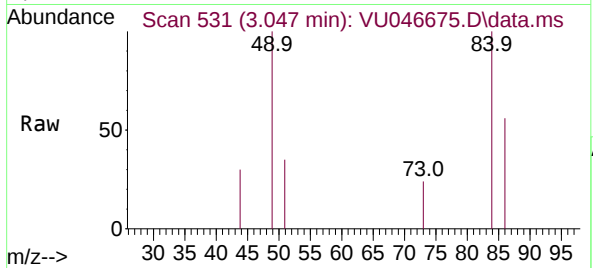

Tgt Ion: 84 Resp: 980
Ion Ratio Lower Upper
84 100
86 56.0 44.7 82.9
49 99.8 75.9 141.1

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 01/07/2022
Supervised By :Semsettin Yesilyurt 01/11/2022

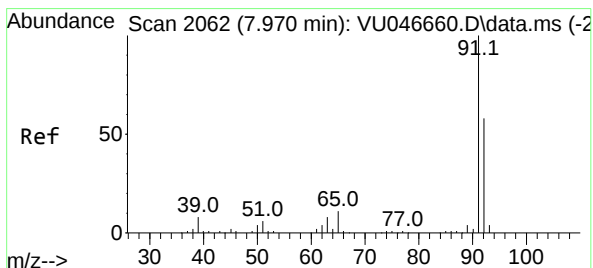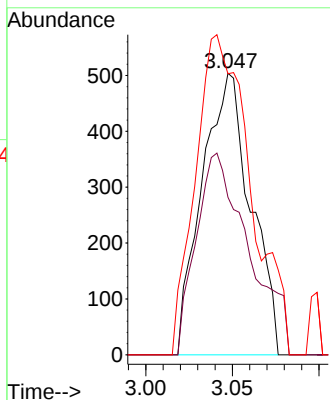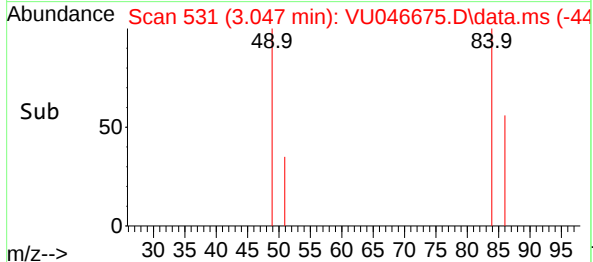

#42
Toluene
Concen: 4.131 ug/L
RT: 7.973 min Scan# 2063
Delta R.T. 0.003 min
Lab File: VU046675.D
Acq: 05 Jan 2022 20:14

Tgt Ion: 91 Resp: 6495
Ion Ratio Lower Upper
91 100
92 60.4 40.4 75.0

