

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010621\
 Data File : VU041855.D
 Acq On : 06 Jan 2021 10:15
 Operator : SY/MD
 Sample : VU0106WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 07 00:42:17 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jan 07 00:41:32 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.23	114	6453	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.36	117	5997	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.74	152	2996	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.60	65	3157	0.49	ug/L	0.00
Spiked Amount 0.500	Range	40 - 130	Recovery	=	98.00%	
4) 1,2-Dichloroethane-d4	5.68	65	3540	0.40	ug/L	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	80.00%	
7) 1,2-Dichloropropane-d6	6.64	67	3922	0.55	ug/L	0.00
Spiked Amount 0.500	Range	60 - 140	Recovery	=	110.00%	
8) Toluene-d8	7.85	98	6984	0.52	ug/L	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	104.00%	
10) 1,1,2,2-Tetrachloroethane-	10.68	84	4391	0.59	ug/L	0.00
Spiked Amount 0.500	Range	65 - 120	Recovery	=	118.00%	
Target Compounds						
13) 1,2-Dibromo-3-chloropropan	12.89	75	11	0.011	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU010621\
Data File : VU041855.D
Acq On : 06 Jan 2021 10:15
Operator : SY/MD
Sample : VU0106WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 07 00:42:17 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jan 07 00:41:32 2021
Response via : Initial Calibration

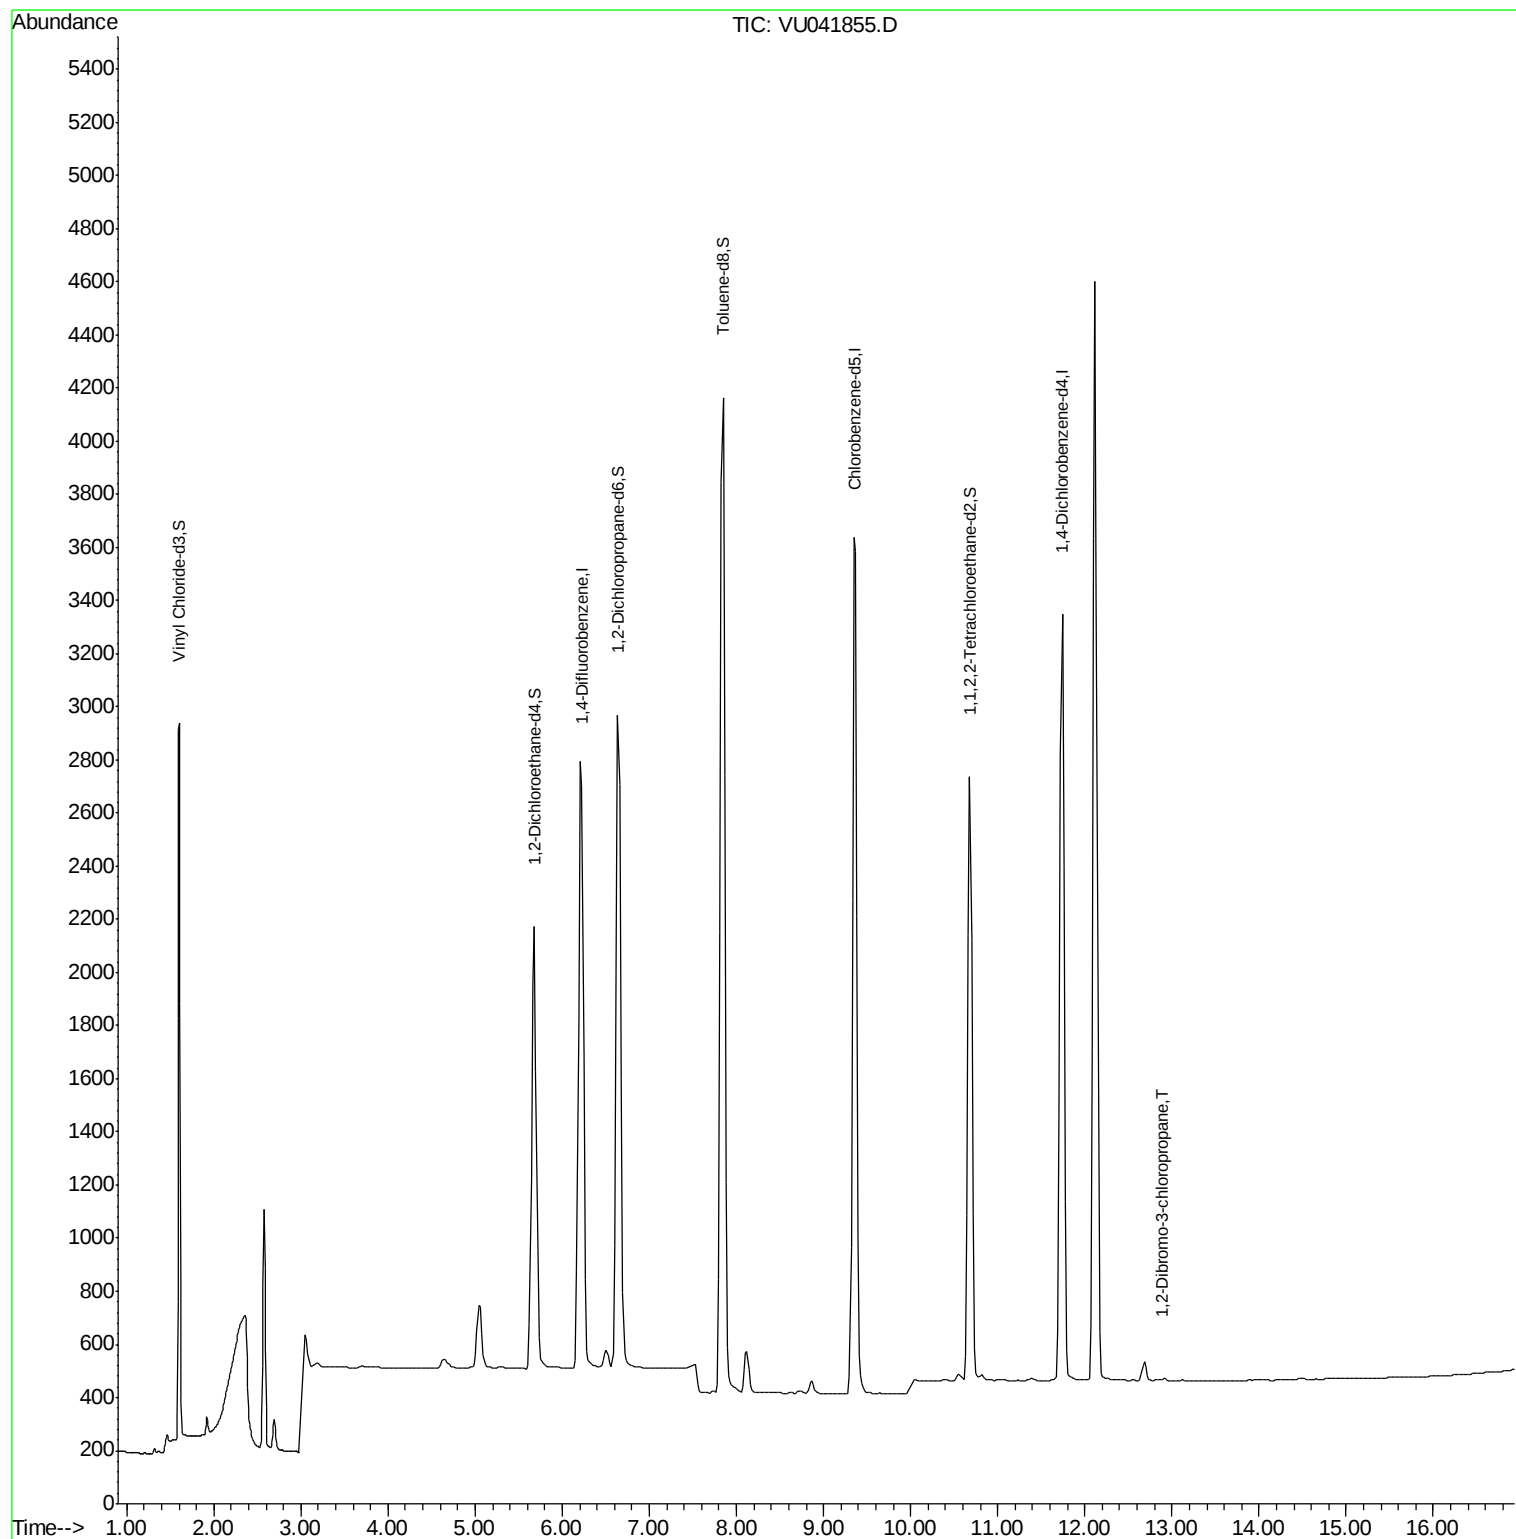

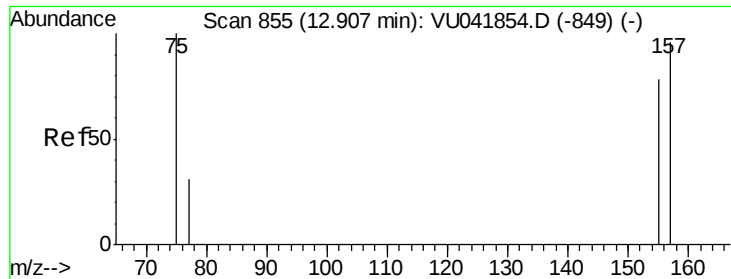

#13

1,2-Dibromo-3-chloropropane

Concen: 0.011 ug/L

RT: 12.89 min Scan# 854

Delta R.T. -0.02 min


Lab File: VU041855.D

Acq: 06 Jan 2021 10:15

Instrument :

MSVOA_U

ClientSampleId :

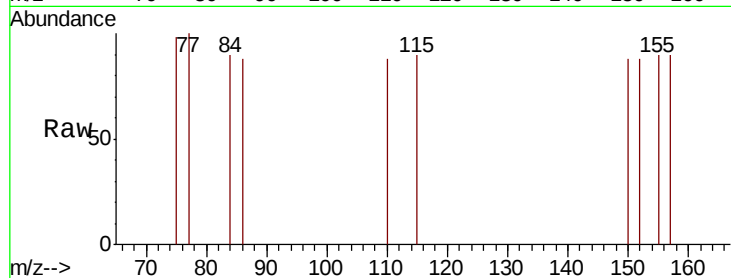


Tot Ion: 75 Resp: 11

Ion Ratio Lower Upper

75 100

157 92.0 72.2 108.2

155 92.0 68.3 102.5

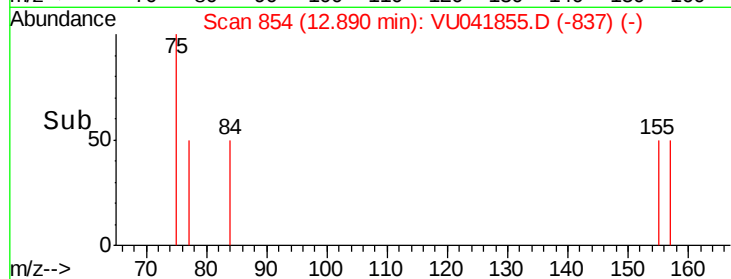

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 157.00 (156.70 to 157.70): V

Ion 155.00 (154.70 to 155.70): V

