


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU010621\
 Data File : VU041853.D
 Acq On : 06 Jan 2021 09:08
 Operator : SY/MD
 Sample : BFB34
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB34

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jan 07 14:13:56 2021

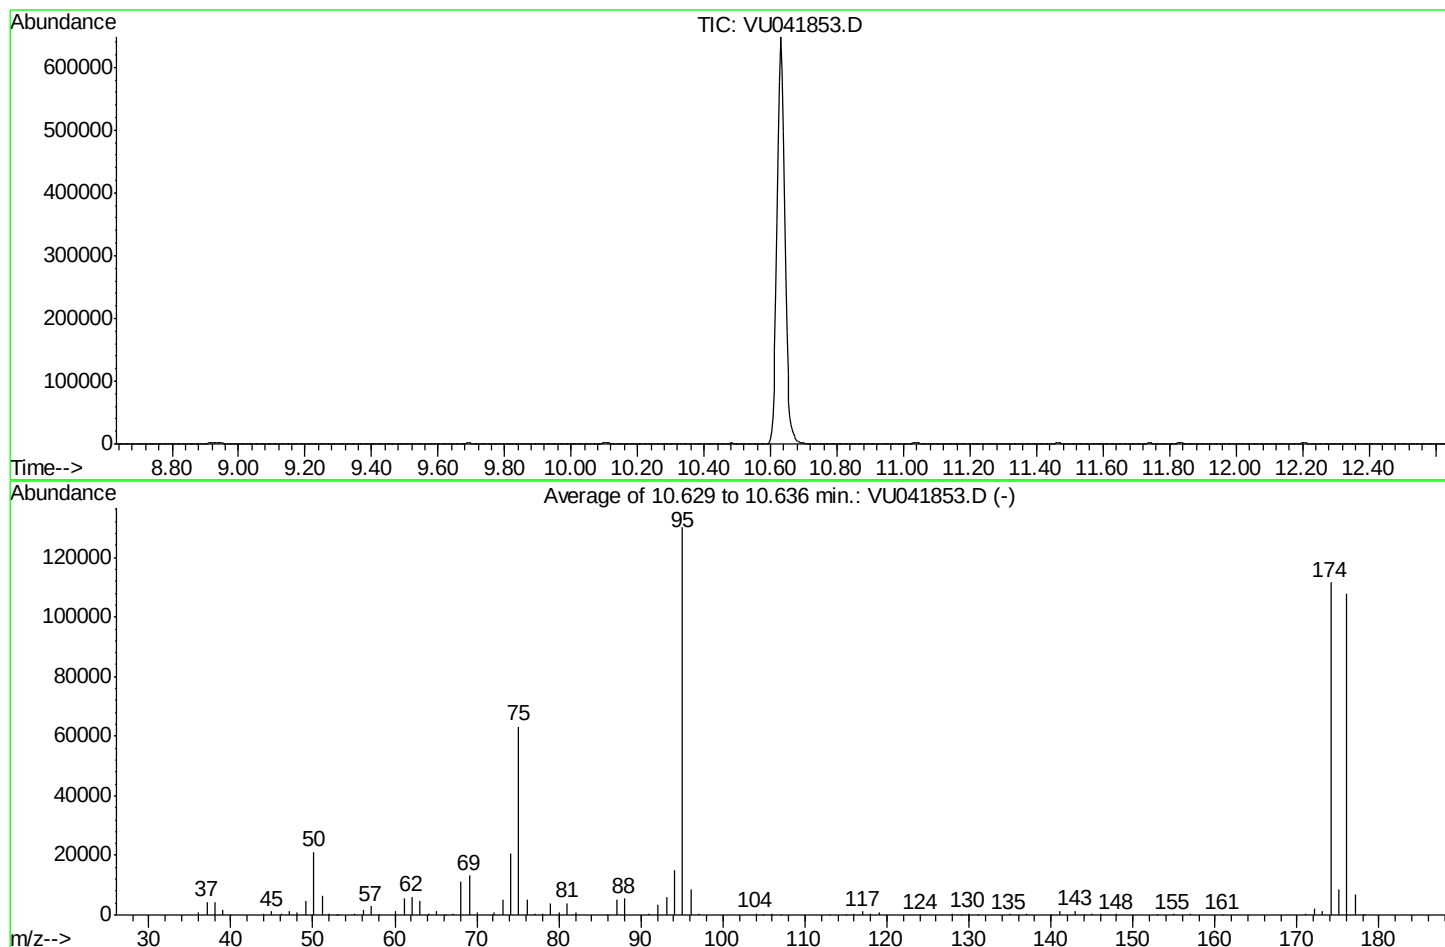

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	21184	PASS
75	95	30	80	48.6	63288	PASS
95	95	100	100	100.0	130104	PASS
96	95	5	9	6.5	8452	PASS
173	174	0.00	2	1.1	1175	PASS
174	95	50	120	85.8	111640	PASS
175	174	5	9	7.7	8571	PASS
176	174	95	101	96.8	108018	PASS
177	176	5	9	6.3	6846	PASS

m/z	Abundance
36.10	836.0
37.10	4338.0
38.00	3862.0
39.00	1698.0
40.10	169.0
44.00	591.0
45.00	1039.0
46.10	204.0
47.10	1161.0
48.10	768.0
49.10	4090.0
50.10	19928.0
51.10	5960.0
52.00	296.0
53.10	153.0
55.00	355.0
56.10	1541.0
57.10	2712.0
58.10	120.0
60.00	1054.0
61.10	5308.0
62.10	5844.0
63.10	4191.0
64.10	502.0
65.10	1181.0
67.00	282.0
68.10	10581.0
69.10	12197.0
70.10	668.0
72.10	765.0
73.10	4729.0
74.10	18864.0
75.10	60216.0
76.10	4980.0
77.00	477.0
77.90	453.0
79.00	3385.0
80.00	895.0
81.00	3669.0
82.00	1055.0
87.00	4592.0
88.00	5276.0
91.00	348.0
92.10	3253.0
93.10	5729.0
94.10	14134.0
95.10	123368.0
96.10	7631.0
97.00	219.0
104.00	518.0
104.90	142.0
106.00	425.0
107.00	152.0
112.90	126.0
114.90	131.0
116.00	468.0
117.00	1030.0
118.00	389.0
119.00	694.0
128.00	361.0
129.00	260.0
129.90	519.0
131.00	189.0
134.90	192.0
137.00	231.0
141.00	1170.0
143.00	1368.0
144.00	125.0
145.00	390.0
146.00	220.0
148.00	268.0
155.00	292.0
157.00	231.0
161.00	205.0
171.00	262.0
172.10	1860.0
174.10	107192.0
175.10	8174.0
176.10	104904.0
177.10	6330.0
178.20	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	885.0
37.10	4525.0
38.10	4483.0
39.00	1790.0
39.90	114.0
44.10	614.0
45.00	1098.0
46.10	276.0
47.00	1076.0
48.00	647.0
49.10	4909.0
50.10	21824.0
51.10	6790.0
52.00	335.0
52.90	105.0
55.00	481.0
56.10	1672.0
57.10	3001.0
58.00	195.0
60.00	1251.0
61.10	5896.0
62.10	6284.0
63.10	5121.0
64.10	724.0
65.00	1274.0
66.10	124.0
67.10	300.0
68.10	11897.0
69.10	14029.0
70.00	862.0
72.10	914.0
73.10	5454.0
74.10	21504.0
75.10	64280.0
76.10	5399.0
77.10	506.0
78.00	525.0
79.00	3955.0
80.00	1015.0
81.00	4109.0
82.00	922.0
85.80	126.0
87.00	5394.0
88.00	5567.0
91.00	408.0
92.10	3851.0
93.10	5895.0
94.10	15415.0
95.10	132608.0
96.10	8906.0
97.10	254.0
104.00	531.0
104.90	166.0
105.90	424.0
107.00	157.0
113.10	115.0
115.00	101.0
116.00	550.0
117.10	1211.0
118.00	465.0
119.00	774.0
124.10	109.0
128.00	385.0
129.10	172.0
130.00	538.0
131.10	130.0
134.90	278.0
137.00	222.0
140.00	103.0
141.10	983.0
143.00	1540.0
144.10	112.0
145.00	613.0
146.00	263.0
148.00	360.0
152.90	140.0
154.90	407.0
157.00	272.0
160.90	129.0
171.00	299.0
172.10	1978.0
173.10	1678.0
174.10	112600.0
175.10	8724.0
176.10	107928.0
177.10	7132.0
178.00	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.10	854.0
37.10	4676.0
38.10	4468.0
39.00	1795.0
40.00	120.0
44.00	631.0
45.00	1158.0
46.10	263.0
47.00	1131.0
48.10	730.0
49.10	4812.0
50.10	21800.0
51.10	6780.0
52.00	317.0
53.10	131.0
55.00	463.0
56.10	1708.0
57.10	3001.0
58.10	184.0
60.00	1225.0
61.10	5952.0
62.10	6412.0
63.10	4705.0
64.10	617.0
65.00	1256.0
66.10	110.0
67.00	320.0
68.10	11607.0
69.10	13719.0
70.10	746.0
72.10	913.0
73.10	5322.0
74.10	21096.0
75.10	65368.0
76.10	5369.0
77.20	464.0
77.90	468.0
79.00	3831.0
80.00	931.0
81.00	4056.0
82.00	1044.0
87.00	5308.0
88.00	5653.0
91.00	412.0
92.10	3726.0
93.10	6066.0
94.10	15639.0
95.10	134336.0
96.10	8821.0
97.00	250.0
104.00	540.0
104.90	160.0
106.00	457.0
107.00	157.0
113.00	126.0
115.00	108.0
116.00	533.0
117.10	1186.0
118.00	416.0
119.00	786.0
128.00	371.0
129.10	235.0
130.00	588.0
131.10	163.0
134.90	259.0
137.00	255.0
141.00	1146.0
143.00	1477.0
144.10	133.0
145.00	528.0
146.00	249.0
148.00	315.0
154.90	367.0
157.00	263.0
161.00	184.0
171.00	339.0
172.10	2030.0
173.10	1847.0
174.10	115128.0
175.10	8815.0
176.10	111224.0
177.10	7077.0
178.20	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

Scan 2875 (10.584 min): VU041853.D
BFB34

m/z	Abundance
39.90	129.0
44.00	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.10	854.0
37.10	4676.0
38.10	4468.0
39.00	1795.0
40.00	120.0
44.00	631.0
45.00	1158.0
46.10	263.0
47.00	1131.0
48.10	730.0
49.10	4812.0
50.10	21800.0
51.10	6780.0
52.00	317.0
53.10	131.0
55.00	463.0
56.10	1708.0
57.10	3001.0
58.10	184.0
60.00	1225.0
61.10	5952.0
62.10	6412.0
63.10	4705.0
64.10	617.0
65.00	1256.0
66.10	110.0
67.00	320.0
68.10	11607.0
69.10	13719.0
70.10	746.0
72.10	913.0
73.10	5322.0
74.10	21096.0
75.10	65368.0
76.10	5369.0
77.20	464.0
77.90	468.0
79.00	3831.0
80.00	931.0
81.00	4056.0
82.00	1044.0
87.00	5308.0
88.00	5653.0
91.00	412.0
92.10	3726.0
93.10	6066.0
94.10	15639.0
95.10	134336.0
96.10	8821.0
97.00	250.0
104.00	540.0
104.90	160.0
106.00	457.0
107.00	157.0
113.00	126.0
115.00	108.0
116.00	533.0
117.10	1186.0
118.00	416.0
119.00	786.0
128.00	371.0
129.10	235.0
130.00	588.0
131.10	163.0
134.90	259.0
137.00	255.0
141.00	1146.0
143.00	1477.0
144.10	133.0
145.00	528.0
146.00	249.0
148.00	315.0
154.90	367.0
157.00	263.0
161.00	184.0
171.00	339.0
172.10	2030.0
173.10	1847.0
174.10	115128.0
175.10	8815.0
176.10	111224.0
177.10	7077.0
178.20	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	885.0
37.10	4525.0
38.10	4483.0
39.00	1790.0
39.90	114.0
44.10	614.0
45.00	1098.0
46.10	276.0
47.00	1076.0
48.00	647.0
49.10	4909.0
50.10	21824.0
51.10	6790.0
52.00	335.0
52.90	105.0
55.00	481.0
56.10	1672.0
57.10	3001.0
58.00	195.0
60.00	1251.0
61.10	5896.0
62.10	6284.0
63.10	5121.0
64.10	724.0
65.00	1274.0
66.10	124.0
67.10	300.0
68.10	11897.0
69.10	14029.0
70.00	862.0
72.10	914.0
73.10	5454.0
74.10	21504.0
75.10	64280.0
76.10	5399.0
77.10	506.0
78.00	525.0
79.00	3955.0
80.00	1015.0
81.00	4109.0
82.00	922.0
85.80	126.0
87.00	5394.0
88.00	5567.0
91.00	408.0
92.10	3851.0
93.10	5895.0
94.10	15415.0
95.10	132608.0
96.10	8906.0
97.10	254.0
104.00	531.0
104.90	166.0
105.90	424.0
107.00	157.0
113.10	115.0
115.00	101.0
116.00	550.0
117.10	1211.0
118.00	465.0
119.00	774.0
124.10	109.0
128.00	385.0
129.10	172.0
130.00	538.0
131.10	130.0
134.90	278.0
137.00	222.0
140.00	103.0
141.10	983.0
143.00	1540.0
144.10	112.0
145.00	613.0
146.00	263.0
148.00	360.0
152.90	140.0
154.90	407.0
157.00	272.0
160.90	129.0
171.00	299.0
172.10	1978.0
173.10	1678.0
174.10	112600.0
175.10	8724.0
176.10	107928.0
177.10	7132.0
178.00	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

Scan 2875 (10.584 min): VU041853.D
BFB34

m/z	Abundance
39.90	129.0
44.00	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34