

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
 Data File : VU046682.D
 Acq On : 06 Jan 2022 13:26
 Operator : SY/MD
 Sample : N1027-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Quant Time: Jan 07 03:15:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 07 03:14:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	72126	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	77284	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	38467	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	28367	4.993	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.800%
7) Chloroethane-d5	1.919	69	22690	5.072	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.400%
11) 1,1-Dichloroethene-d2	2.571	65	12002	5.010	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.200%
20) 2-Butanone-d5	4.652	46	96656	58.654	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.300%
24) Chloroform-d	5.066	84	53608	5.150	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.706	65	32968	5.540	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
32) Benzene-d6	5.732	84	106484	4.943	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
36) 1,2-Dichloropropane-d6	6.693	67	33488	5.173	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.902	98	89156	4.560	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	8.182	79	14298	4.775	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.600%
46) 2-Hexanone-d5	8.639	63	87944	50.029	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.060%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	35459	5.337	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	36919	5.210	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.200%
Target Compounds						
					Qvalue	
3) Chloromethane	1.523	50	1344	0.141	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
Data File : VU046682.D
Acq On : 06 Jan 2022 13:26
Operator : SY/MD
Sample : N1027-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Time: Jan 07 03:15:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 07 03:14:07 2022
Response via : Initial Calibration

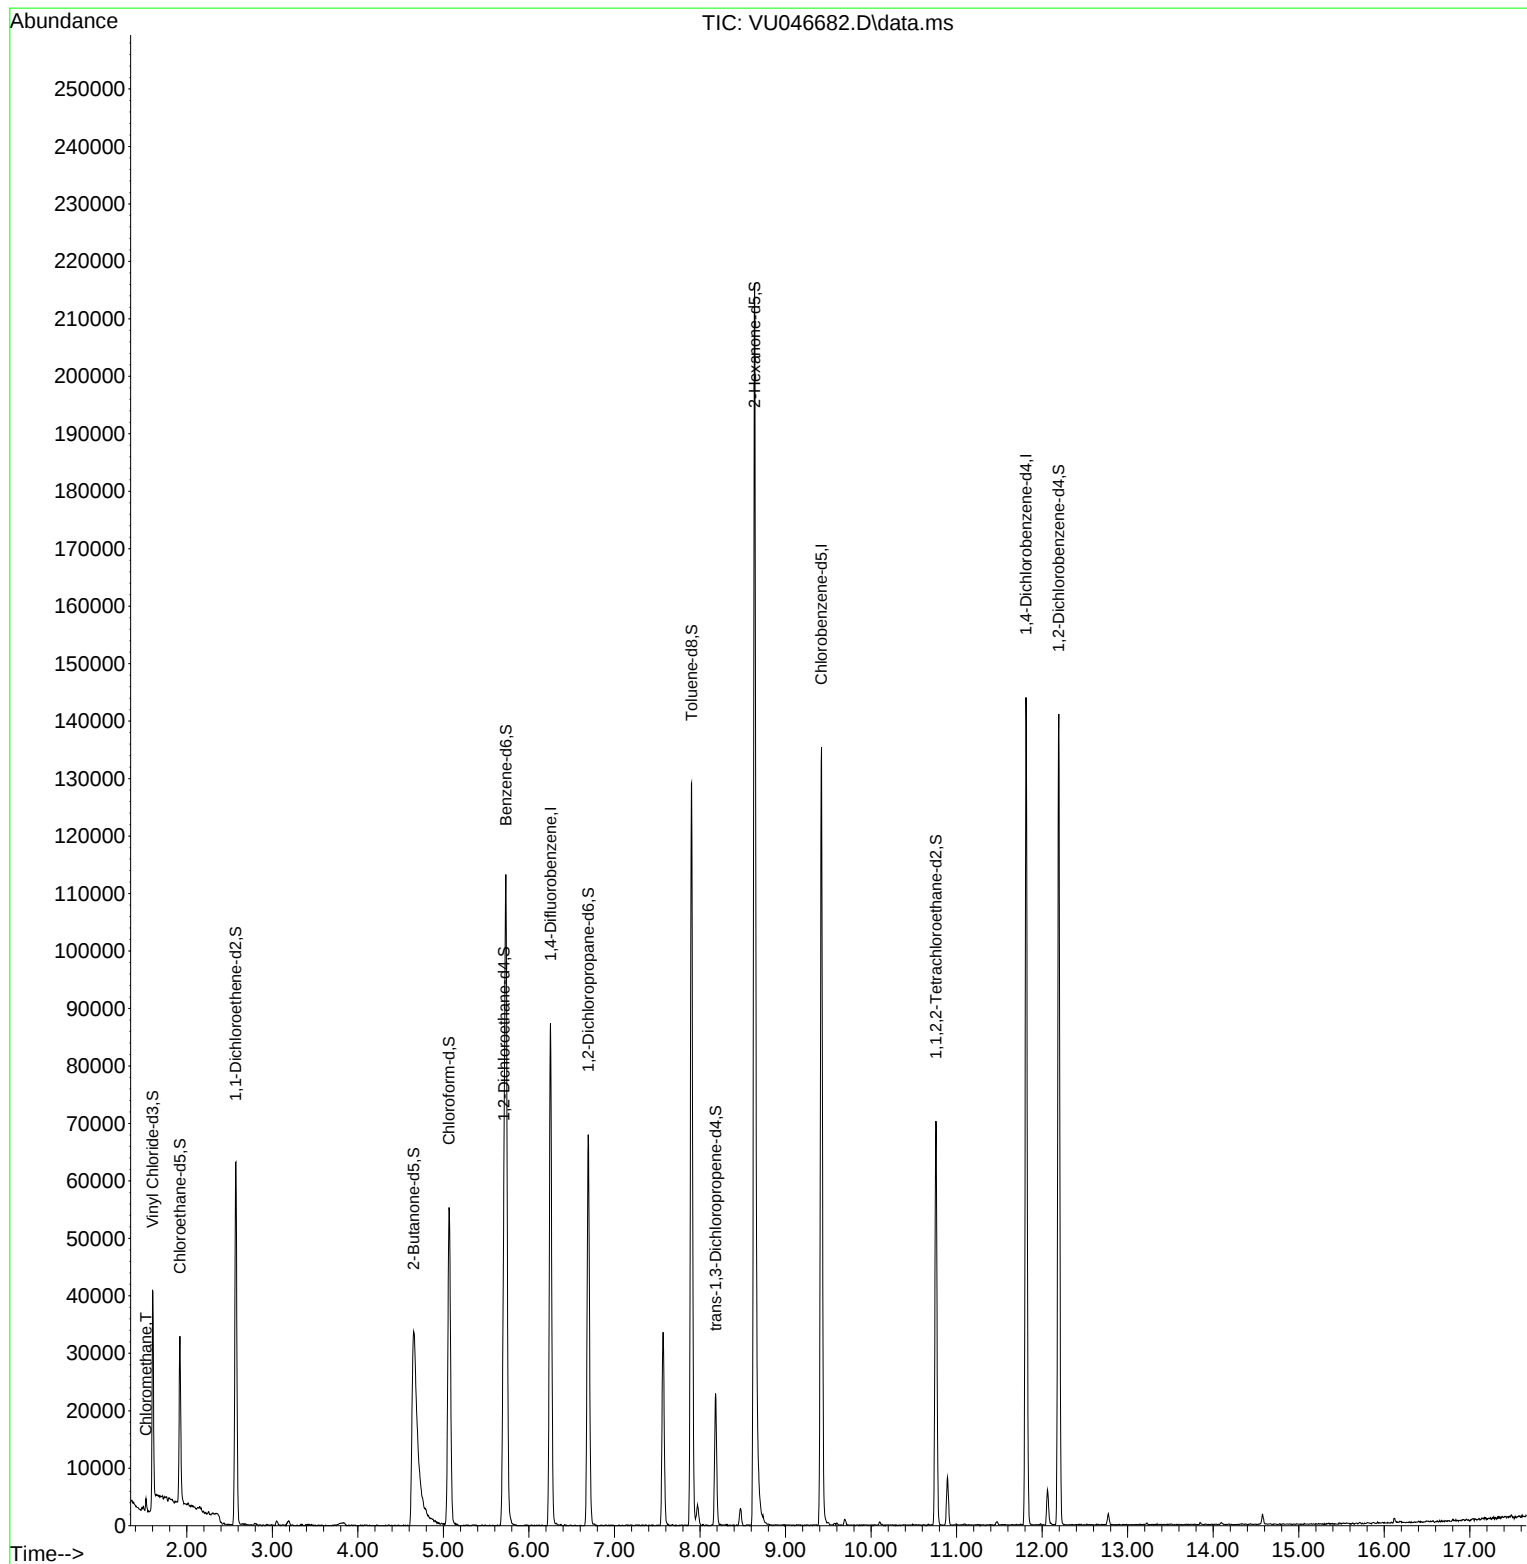

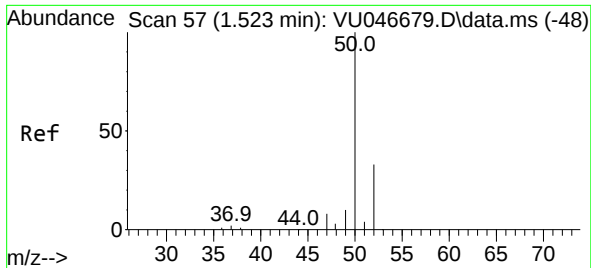

#3
 Chloromethane
 Concen: 0.141 ug/L
 RT: 1.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VU046682.D
 Acq: 06 Jan 2022 13:26

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Tgt Ion: 50 Resp: 1344
 Ion Ratio Lower Upper
 50 100
 52 38.3 23.0 42.8

