

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
 Data File : VU046690.D
 Acq On : 06 Jan 2022 17:06
 Operator : SY/MD
 Sample : N1027-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Jan 07 03:16:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 07 03:14:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	77249	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	82369	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	41252	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	26790	4.403	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.000%	
7) Chloroethane-d5	1.919	69	21930	4.577	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.600%	
11) 1,1-Dichloroethene-d2	2.572	65	11829	4.610	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	92.200%	
20) 2-Butanone-d5	4.658	46	93341	52.886	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.780%	
24) Chloroform-d	5.067	84	53309	4.781	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
26) 1,2-Dichloroethane-d4	5.706	65	32327	5.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.400%	
32) Benzene-d6	5.732	84	103654	4.514	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
36) 1,2-Dichloropropane-d6	6.694	67	33186	4.810	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.200%	
41) Toluene-d8	7.903	98	86441	4.148	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.000%	
43) trans-1,3-Dichloroprop...	8.182	79	13537	4.242	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.639	63	85299	45.528	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.060%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	33790	4.772	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	12.195	152	36548	4.810	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds						Qvalue
3) Chloromethane	1.523	50	1724	0.169	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
Data File : VU046690.D
Acq On : 06 Jan 2022 17:06
Operator : SY/MD
Sample : N1027-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Jan 07 03:16:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 07 03:14:07 2022
Response via : Initial Calibration

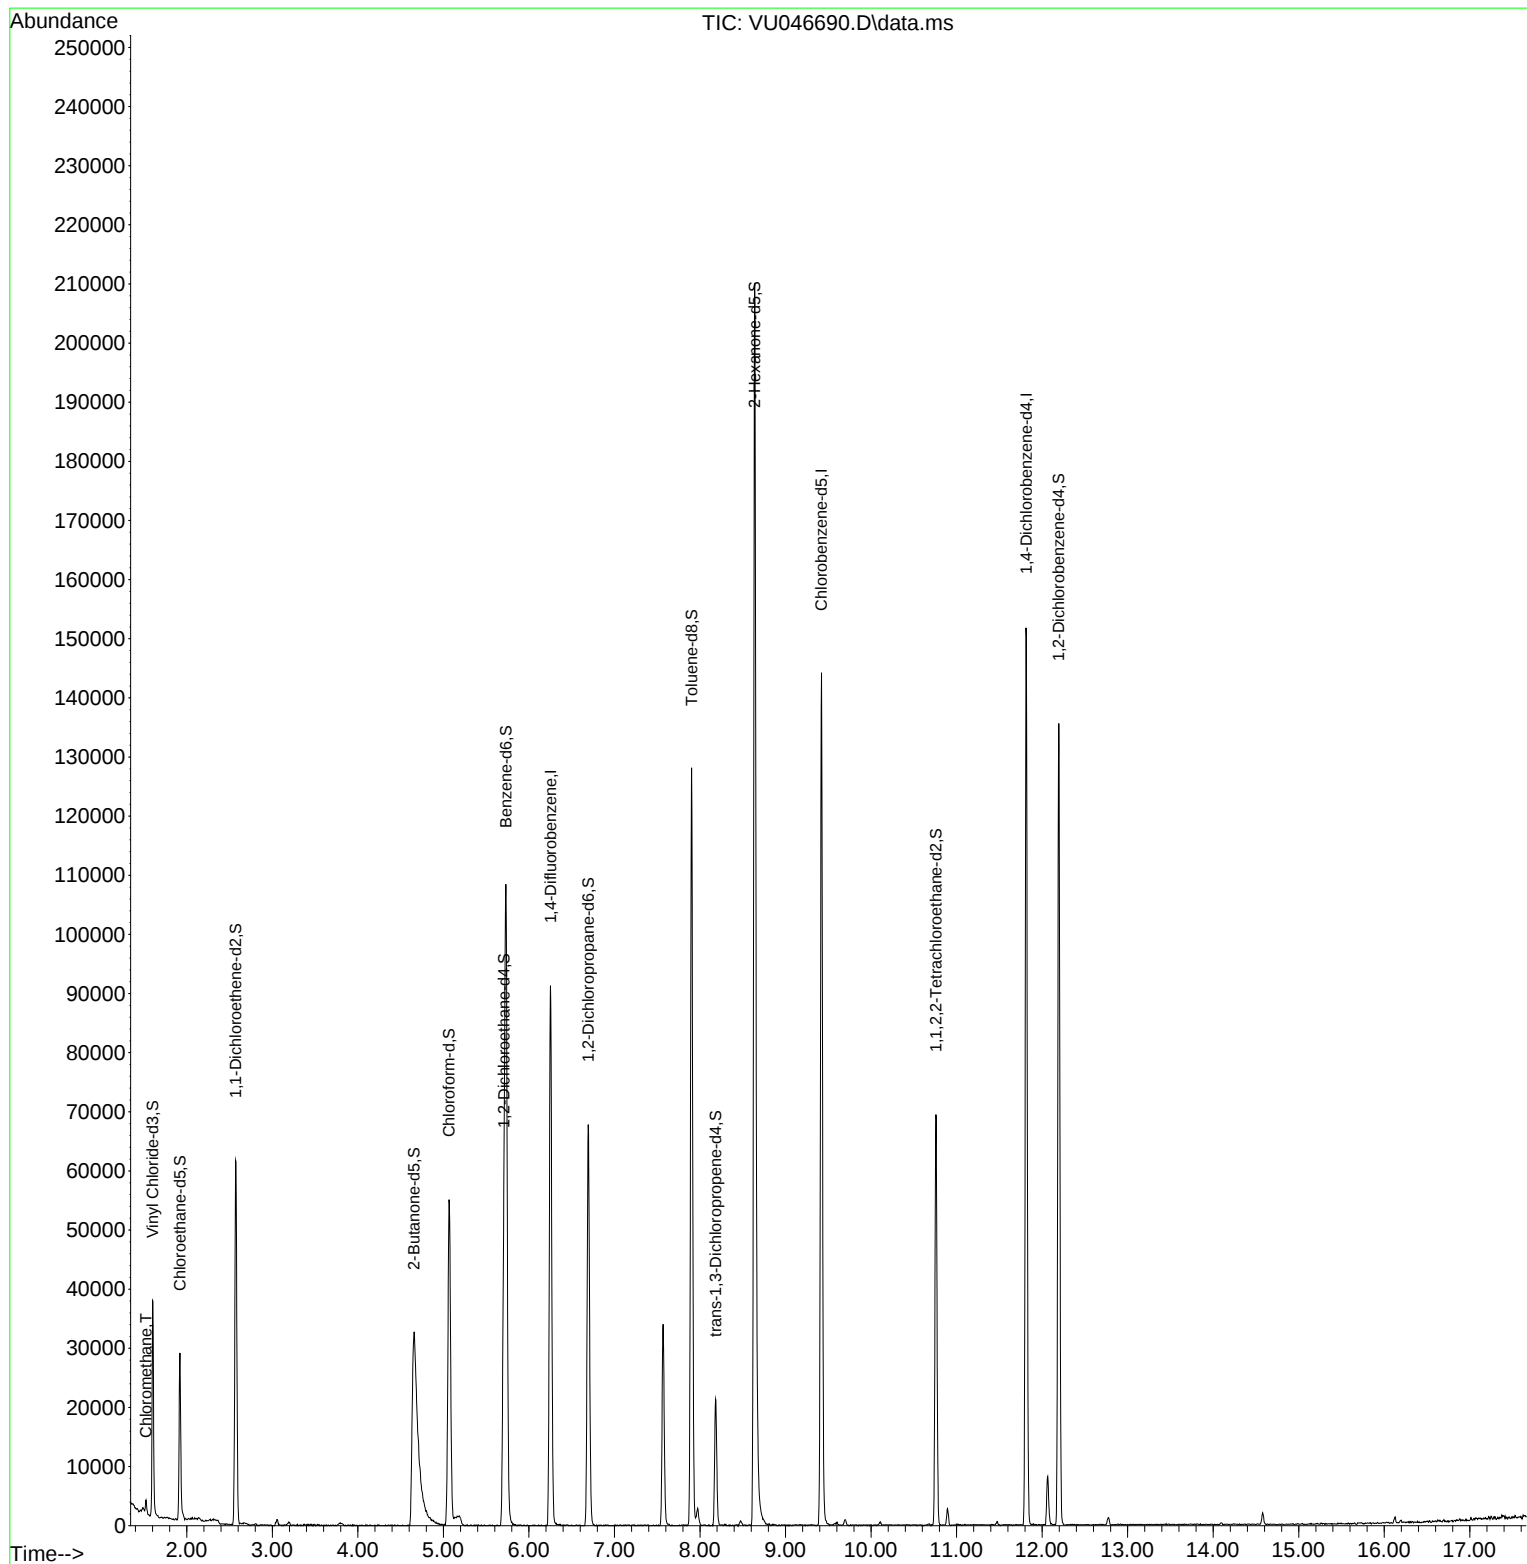

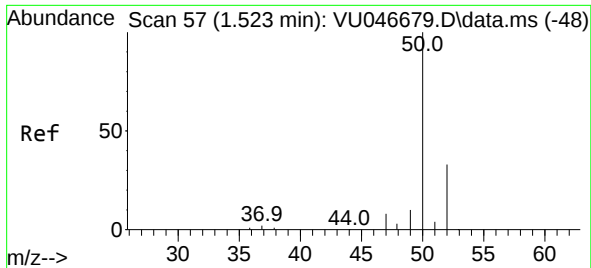

#3
 Chloromethane
 Concen: 0.169 ug/L
 RT: 1.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VU046690.D
 Acq: 06 Jan 2022 17:06

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Tgt Ion: 50 Resp: 1724
 Ion Ratio Lower Upper
 50 100
 52 33.9 23.0 42.8

