

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
 Data File : VU046682.D
 Acq On : 06 Jan 2022 13:26
 Operator : SY/MD
 Sample : N1027-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J36

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	91	rBV	38164	46585	11.42%	1.789%
2	1.919	172	180	195	rVB	29218	39033	9.57%	1.499%
3	2.575	371	384	400	rBV	63070	102019	25.00%	3.918%
4	4.652	1015	1030	1069	rBV	33767	151378	37.10%	5.813%
5	5.067	1144	1159	1180	rBV	55184	121681	29.82%	4.673%
6	5.729	1345	1365	1393	rBV3	113215	294907	72.27%	11.325%
7	6.253	1515	1528	1547	rBV2	87447	163431	40.05%	6.276%
8	6.693	1651	1665	1682	rBV	68060	131900	32.32%	5.065%
9	7.568	1926	1937	1953	rBV2	33671	60501	14.83%	2.323%
10	7.902	2028	2041	2055	rBV	129233	225368	55.23%	8.654%
11	7.970	2055	2062	2074	rVB2	3557	6362	1.56%	0.244%
12	8.182	2117	2128	2142	rBV	22849	37895	9.29%	1.455%
13	8.472	2209	2218	2229	rBB3	3009	5154	1.26%	0.198%
14	8.639	2257	2270	2297	rBV	216161	408049	100.00%	15.669%
15	9.420	2500	2513	2533	rBV	135513	224243	54.95%	8.611%
16	10.758	2917	2929	2944	rVB	70272	113893	27.91%	4.374%
17	10.893	2961	2971	2983	rVB2	8335	13310	3.26%	0.511%
18	11.812	3246	3257	3273	rBV	143935	225478	55.26%	8.659%
19	12.063	3326	3335	3345	rBV3	6145	9978	2.45%	0.383%
20	12.195	3364	3376	3394	rBV	141080	222952	54.64%	8.562%




Sum of corrected areas: 2604117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
Data File : VU046682.D
Acq On : 06 Jan 2022 13:26
Operator : SY/MD
Sample : N1027-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

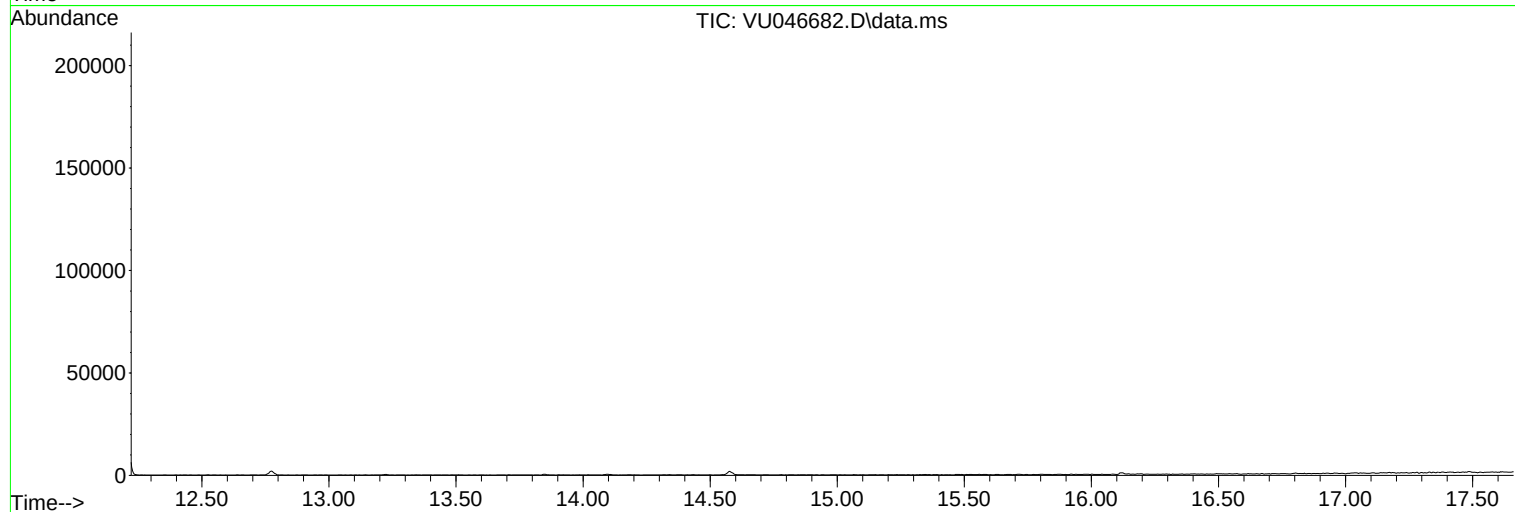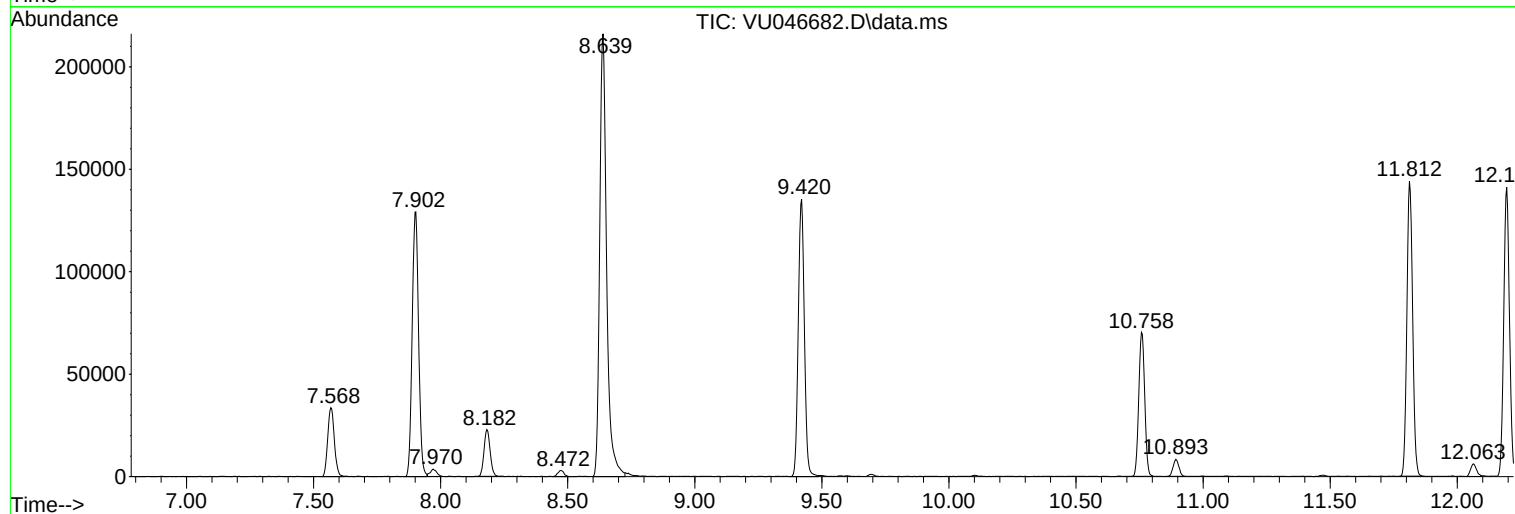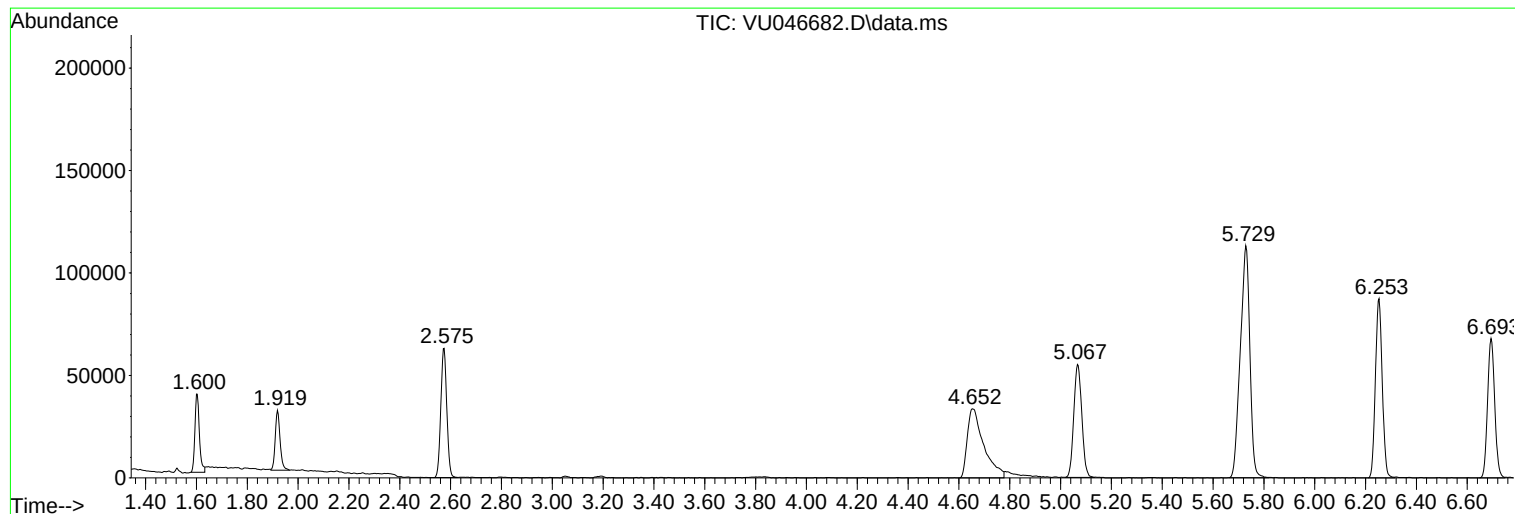

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
Data File : VU046682.D
Acq On : 06 Jan 2022 13:26
Operator : SY/MD
Sample : N1027-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
Data File : VU046682.D
Acq On : 06 Jan 2022 13:26
Operator : SY/MD
Sample : N1027-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc