
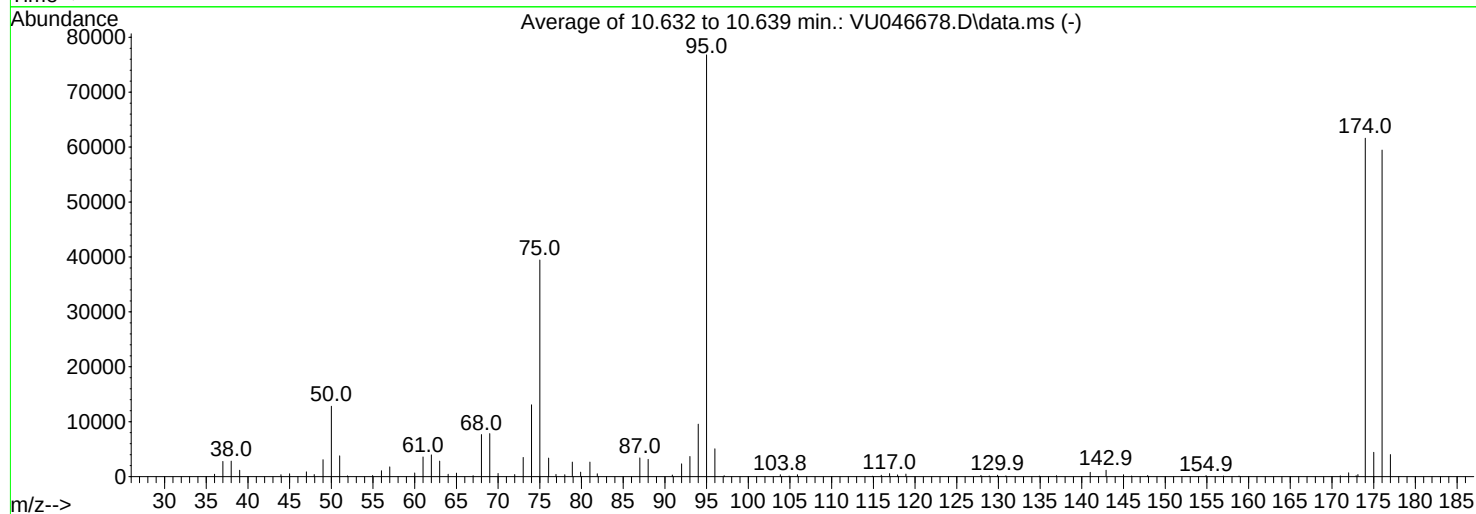


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010622\
Data File : VU046678.D
Acq On : 06 Jan 2022 10:58
Operator : SY/MD
Sample : BFB039
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB039

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jan 10 00:25:50 2022

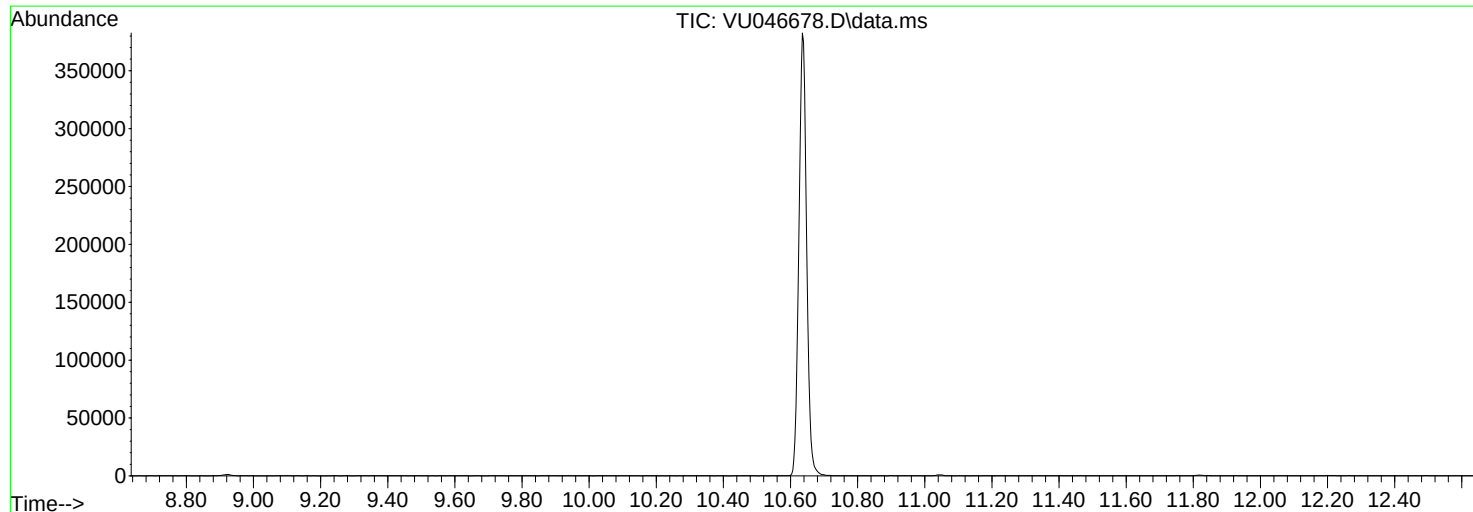

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	12823	PASS
75	95	30	80	51.4	39453	PASS
95	95	100	100	100.0	76797	PASS
96	95	5	9	6.6	5085	PASS
173	174	0.00	2	0.6	376	PASS
174	95	50	120	80.2	61619	PASS
175	174	5	9	7.2	4416	PASS
176	174	95	101	96.5	59467	PASS
177	176	5	9	6.8	4021	PASS

m/z	Abundance
43.80	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
36.00	425.0
37.00	2677.0
38.00	2741.0
39.00	1198.0
44.00	452.0
45.00	518.0
47.00	816.0
48.00	369.0
49.00	2976.0
50.00	12709.0
51.00	3765.0
52.00	165.0
55.00	203.0
56.00	1034.0
57.00	1721.0
60.00	672.0
61.00	3341.0
62.00	3967.0
63.00	2864.0
64.00	484.0
65.00	671.0
67.00	180.0
68.00	7370.0
69.00	7687.0
70.00	562.0
72.00	358.0
73.00	3337.0
74.00	12562.0
75.00	38080.0
76.10	3271.0
76.90	392.0
78.00	322.0
78.90	2526.0
79.90	770.0
81.00	2611.0
81.90	572.0
87.00	3139.0
88.00	3013.0
90.90	260.0
92.00	2165.0
93.00	3651.0
94.00	8871.0
95.00	73464.0
96.00	4894.0
97.10	209.0
103.90	356.0
104.90	115.0
105.90	290.0
115.90	259.0
116.90	503.0
117.90	312.0
118.90	441.0
127.90	227.0
128.90	120.0
129.90	273.0
130.90	126.0
134.90	100.0
137.00	149.0
141.00	751.0
142.90	1062.0
145.00	343.0
146.00	123.0
147.90	179.0
154.90	174.0
157.00	118.0
158.80	123.0
171.00	133.0
172.00	686.0
172.90	508.0
174.00	58008.0
175.00	4220.0
176.00	55424.0
177.00	3910.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
36.00	468.0
37.00	2823.0
38.00	2919.0
39.00	1194.0
44.00	447.0
45.00	553.0
47.00	923.0
48.00	377.0
49.00	3219.0
50.00	13193.0
51.00	3880.0
51.90	159.0
54.90	221.0
56.00	1119.0
57.00	1826.0
60.00	692.0
61.00	3732.0
62.00	4146.0
63.00	2921.0
64.00	456.0
65.00	672.0
67.00	185.0
68.00	7967.0
69.00	8084.0
70.00	622.0
72.00	408.0
73.00	3590.0
74.00	13489.0
75.00	40896.0
76.00	3487.0
76.90	424.0
78.00	389.0
78.90	2748.0
79.90	829.0
81.00	2741.0
81.90	518.0
87.00	3551.0
88.00	3278.0
90.90	325.0
92.00	2457.0
93.00	3811.0
94.00	9923.0
95.00	79248.0
96.00	5254.0
97.10	188.0
103.80	360.0
104.90	135.0
105.90	354.0
114.90	114.0
116.00	256.0
117.00	596.0
117.90	358.0
118.90	459.0
127.90	253.0
128.90	167.0
129.90	269.0
130.90	148.0
134.90	125.0
137.00	177.0
141.00	810.0
142.90	1214.0
145.00	344.0
146.00	126.0
147.90	232.0
154.90	219.0
157.00	149.0
158.80	119.0
171.00	141.0
172.00	694.0
173.10	566.0
174.00	63744.0
175.00	4513.0
176.00	61352.0
177.00	4212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
36.00	462.0
37.00	2834.0
38.00	2816.0
39.00	1078.0
44.00	431.0
45.00	543.0
47.00	927.0
47.90	384.0
49.00	3097.0
50.00	12568.0
51.00	3731.0
51.90	153.0
54.90	185.0
56.00	1110.0
57.00	1813.0
60.00	670.0
61.00	3701.0
62.00	3784.0
63.00	2735.0
64.00	390.0
65.00	597.0
67.00	167.0
68.00	7683.0
69.00	7730.0
70.00	567.0
72.00	420.0
73.00	3564.0
74.00	13200.0
75.00	39384.0
76.00	3371.0
77.00	430.0
78.00	354.0
78.90	2724.0
79.90	816.0
81.00	2649.0
81.90	474.0
87.00	3545.0
88.00	3161.0
90.90	329.0
92.00	2414.0
93.00	3558.0
94.00	9855.0
95.00	77680.0
96.00	5108.0
97.10	151.0
103.80	330.0
104.90	137.0
105.90	383.0
114.90	120.0
116.00	259.0
116.90	585.0
117.90	327.0
118.90	471.0
127.90	269.0
128.90	174.0
129.90	222.0
130.90	135.0
134.90	158.0
136.90	169.0
141.00	788.0
142.90	1214.0
145.00	338.0
145.90	119.0
147.90	237.0
154.90	223.0
157.00	137.0
158.90	103.0
171.00	138.0
172.00	686.0
173.10	563.0
174.00	63104.0
175.00	4515.0
176.00	61624.0
177.00	3942.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039