

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052627.D
 Acq On : 06 Jan 2023 14:55
 Operator : JC/MD
 Sample : 01036-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLE1

Quant Time: Jan 07 01:36:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jan 07 00:30:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	326430	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	315215	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	140597	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	176261	47.938	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.880%
7) Chloroethane-d5	1.909	69	132109	45.923	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.840%
11) 1,1-Dichloroethene-d2	2.565	63	226169	37.406	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.820%
21) 2-Butanone-d5	4.623	46	239312	102.847	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.850%
24) Chloroform-d	5.060	84	269197	46.578	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.160%
26) 1,2-Dichloroethane-d4	5.697	65	184354	48.527	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.060%
32) Benzene-d6	5.722	84	559892	51.357	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.720%
36) 1,2-Dichloropropane-d6	6.687	67	196302	51.250	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.500%
41) Toluene-d8	7.896	98	448861	48.557	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.120%
43) trans-1,3-Dichloroprop...	8.176	79	79811	47.955	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.920%
47) 2-Hexanone-d5	8.632	63	148170	109.784	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.780%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	253683	50.277	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.560%
66) 1,2-Dichlorobenzene-d4	12.188	152	152476	56.483	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.960%
Target Compounds						
					Qvalue	
13) Acetone	2.633	43	6847	2.903	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052627.D
Acq On : 06 Jan 2023 14:55
Operator : JC/MD
Sample : 01036-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLE1

Quant Time: Jan 07 01:36:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jan 07 00:30:36 2023
Response via : Initial Calibration

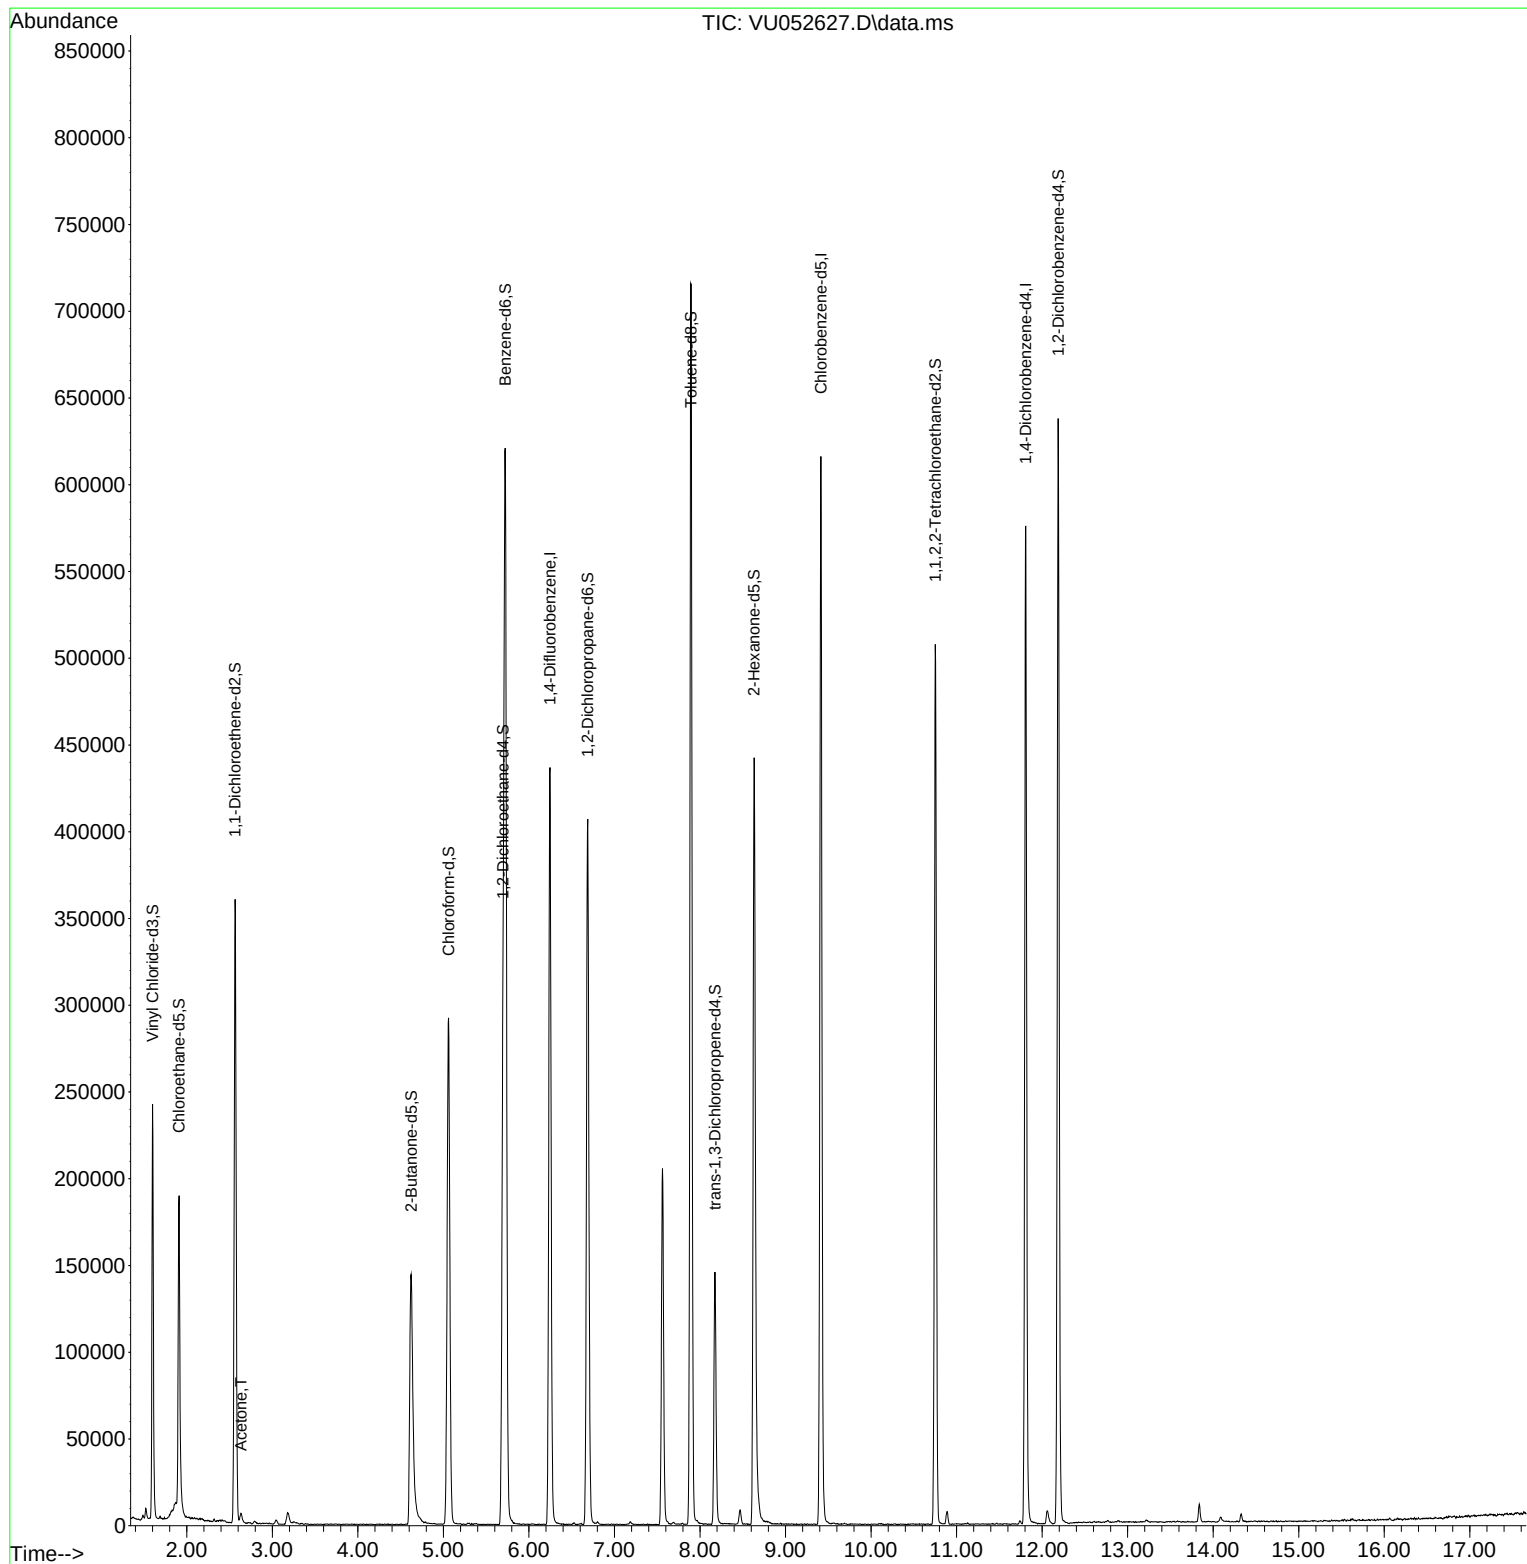

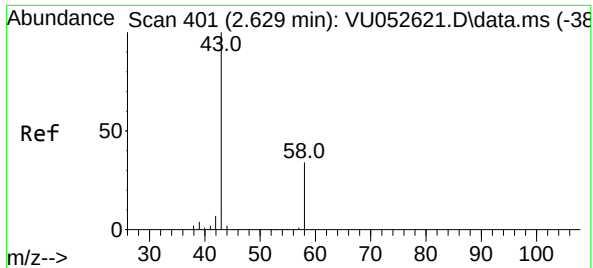

#13

Acetone

Concen: 2.903 ug/L

RT: 2.633 min Scan# 40

Delta R.T. 0.004 min

Lab File: VU052627.D


Acq: 06 Jan 2023 14:55

Instrument :

MSVOA_U

ClientSampleId :

COLE1

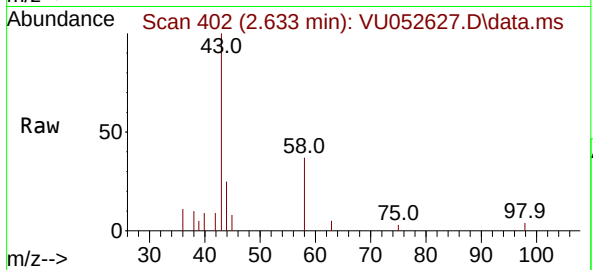

Tgt Ion: 43 Resp: 6847

Ion Ratio Lower Upper

43 100

58 30.8 0.0 64.4

