

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052625.D
 Acq On : 06 Jan 2023 13:58
 Operator : JC/MD
 Sample : VU0106WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK035

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M

Title : VOC Analysis

Signal : TIC: VU052625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	41	47	53	rBV	25429	27249	1.59%	0.224%
2	1.601	73	81	96	rVB	244093	288970	16.90%	2.376%
3	1.909	169	177	210	rVB	187186	291297	17.03%	2.395%
4	2.565	368	381	395	rBV	363206	586248	34.28%	4.820%
5	2.790	442	451	463	rBV2	2565	4847	0.28%	0.040%
6	2.884	477	480	483	rVB3	299	213	0.01%	0.002%
7	2.941	494	498	501	rBV3	419	409	0.02%	0.003%
8	3.009	515	519	521	rBV3	412	367	0.02%	0.003%
9	3.048	521	531	545	rVB4	3621	6954	0.41%	0.057%
10	3.218	582	584	589	rVB2	468	365	0.02%	0.003%
11	3.269	597	600	605	rBV2	259	282	0.02%	0.002%
12	3.353	620	626	634	rVB7	1085	1465	0.09%	0.012%
13	3.449	650	656	658	rBV	551	493	0.03%	0.004%
14	3.562	686	691	692	rBV2	270	259	0.02%	0.002%
15	3.903	789	797	803	rVB3	369	631	0.04%	0.005%
16	3.935	803	807	811	rBV3	489	483	0.03%	0.004%
17	4.189	880	886	889	rVB2	347	404	0.02%	0.003%
18	4.231	895	899	907	rVB2	317	352	0.02%	0.003%
19	4.273	907	912	916	rBV3	355	434	0.03%	0.004%
20	4.546	994	997	1001	rVB	331	248	0.01%	0.002%
21	4.623	1008	1021	1065	rBV	143676	400890	23.44%	3.296%
22	4.964	1124	1127	1130	rVB3	412	251	0.01%	0.002%
23	4.986	1130	1134	1135	rBV2	340	253	0.01%	0.002%
24	5.057	1140	1156	1178	rBV	295617	648079	37.89%	5.328%
25	5.205	1199	1202	1205	rVB2	480	399	0.02%	0.003%
26	5.247	1212	1215	1218	rVB	310	197	0.01%	0.002%
27	5.279	1222	1225	1226	rBV	844	555	0.03%	0.005%
28	5.372	1249	1254	1257	rBV3	679	669	0.04%	0.006%
29	5.494	1288	1292	1296	rVB	457	315	0.02%	0.003%
30	5.520	1296	1300	1302	rVB3	275	210	0.01%	0.002%
31	5.536	1302	1305	1309	rBV	404	415	0.02%	0.003%
32	5.610	1325	1328	1332	rVB2	295	197	0.01%	0.002%
33	5.642	1332	1338	1341	rBV2	233	252	0.01%	0.002%
34	5.723	1341	1363	1394	rBV2	634065	1710331	100.00%	14.062%
35	5.932	1422	1428	1430	rBV3	232	254	0.01%	0.002%
36	5.983	1441	1444	1448	rVB3	663	409	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052625.D
 Acq On : 06 Jan 2023 13:58
 Operator : JC/MD
 Sample : VU0106WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK035

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	6.022	1453	1456	1458	rBV2	321	218	0.01%	0.002%
38	6.041	1458	1462	1465	rBV3	522	322	0.02%	0.003%
39	6.112	1478	1484	1485	rBV	373	290	0.02%	0.002%
40	6.244	1509	1525	1546	rBV	430199	815909	47.70%	6.708%
41	6.420	1577	1580	1585	rVB3	339	347	0.02%	0.003%
42	6.530	1609	1614	1622	rVB5	1661	2545	0.15%	0.021%
43	6.600	1632	1636	1639	rBV3	360	275	0.02%	0.002%
44	6.617	1639	1641	1645	rVB3	467	237	0.01%	0.002%
45	6.687	1648	1663	1686	rBV	414740	801191	46.84%	6.587%
46	6.800	1693	1698	1701	rBV4	1152	1109	0.06%	0.009%
47	6.867	1716	1719	1723	rBV2	312	250	0.01%	0.002%
48	7.192	1811	1820	1826	rBV5	1511	2548	0.15%	0.021%
49	7.282	1847	1848	1853	rVB	346	197	0.01%	0.002%
50	7.346	1864	1868	1874	rVB3	470	443	0.03%	0.004%
51	7.382	1874	1879	1880	rBV	347	292	0.02%	0.002%
52	7.456	1898	1902	1905	rVB2	333	240	0.01%	0.002%
53	7.562	1922	1935	1955	rBV	208547	367970	21.51%	3.025%
54	7.684	1968	1973	1974	rBV3	823	627	0.04%	0.005%
55	7.793	2004	2007	2016	rVB3	1188	1336	0.08%	0.011%
56	7.829	2016	2018	2023	rVB3	365	222	0.01%	0.002%
57	7.893	2023	2038	2056	rBV	722355	1239575	72.48%	10.191%
58	8.018	2073	2077	2078	rBV2	479	308	0.02%	0.003%
59	8.176	2114	2126	2145	rBV	145862	250692	14.66%	2.061%
60	8.285	2157	2160	2164	rVB4	512	407	0.02%	0.003%
61	8.321	2166	2171	2175	rBV5	371	443	0.03%	0.004%
62	8.549	2238	2242	2247	rBV4	1029	846	0.05%	0.007%
63	8.636	2256	2269	2304	rBV2	436805	879746	51.44%	7.233%
64	8.829	2327	2329	2336	rVB4	1115	1063	0.06%	0.009%
65	8.858	2336	2338	2342	rVB4	567	368	0.02%	0.003%
66	8.999	2379	2382	2388	rVB3	314	238	0.01%	0.002%
67	9.079	2403	2407	2410	rBV2	345	286	0.02%	0.002%
68	9.292	2466	2473	2476	rBV3	479	685	0.04%	0.006%
69	9.414	2497	2511	2532	rBV	613147	1007771	58.92%	8.286%
70	9.565	2551	2558	2569	rVB5	1377	1929	0.11%	0.016%
71	9.632	2575	2579	2586	rBV3	251	325	0.02%	0.003%
72	9.690	2590	2597	2605	rVB5	1228	2040	0.12%	0.017%
73	9.816	2629	2636	2641	rBV3	366	522	0.03%	0.004%
74	9.858	2646	2649	2653	rVB2	431	304	0.02%	0.002%
75	9.880	2653	2656	2661	rBV2	360	332	0.02%	0.003%
76	9.928	2666	2671	2673	rBV2	230	221	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052625.D
 Acq On : 06 Jan 2023 13:58
 Operator : JC/MD
 Sample : VU0106WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK035

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	9.960	2678	2681	2686	rVB2	276	228	0.01%	0.002%
78	9.993	2686	2691	2696	rVB3	412	414	0.02%	0.003%
79	10.034	2697	2704	2706	rBV2	327	436	0.03%	0.004%
80	10.063	2711	2713	2717	rVB2	303	217	0.01%	0.002%
81	10.108	2717	2727	2736	rBV5	2028	4139	0.24%	0.034%
82	10.276	2776	2779	2782	rBV2	340	274	0.02%	0.002%
83	10.324	2790	2794	2796	rBV2	330	234	0.01%	0.002%
84	10.346	2798	2801	2802	rBV	415	214	0.01%	0.002%
85	10.372	2807	2809	2812	rVB2	393	237	0.01%	0.002%
86	10.417	2819	2823	2825	rBV2	445	343	0.02%	0.003%
87	10.546	2858	2863	2868	rBV2	641	789	0.05%	0.006%
88	10.755	2914	2928	2944	rBV	502999	817274	47.78%	6.719%
89	10.938	2980	2985	2988	rVB2	332	263	0.02%	0.002%
90	11.025	3009	3012	3017	rVV2	249	309	0.02%	0.003%
91	11.086	3024	3031	3038	rVB3	990	1212	0.07%	0.010%
92	11.378	3119	3122	3127	rVB2	445	340	0.02%	0.003%
93	11.629	3196	3200	3201	rBV2	297	237	0.01%	0.002%
94	11.745	3229	3236	3243	rVB5	2535	3520	0.21%	0.029%
95	11.809	3243	3256	3286	rBV	573114	901267	52.70%	7.410%
96	12.189	3360	3374	3396	rBV	653119	1034980	60.51%	8.509%
97	13.218	3689	3694	3703	rVB5	3624	4955	0.29%	0.041%
98	13.838	3881	3887	3896	rVB4	5465	7925	0.46%	0.065%
99	14.086	3957	3964	3974	rVB2	8122	12297	0.72%	0.101%
100	14.324	4031	4038	4049	rBV4	6496	10468	0.61%	0.086%




Sum of corrected areas: 12162887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052625.D
Acq On : 06 Jan 2023 13:58
Operator : JC/MD
Sample : VU0106WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK035

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

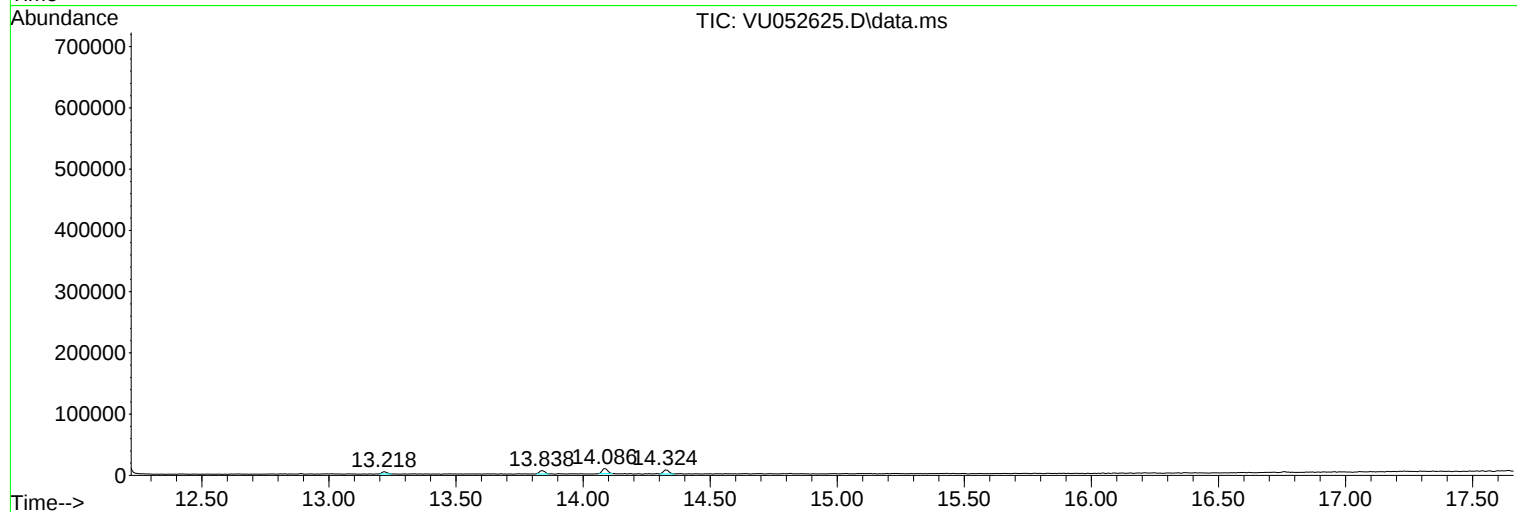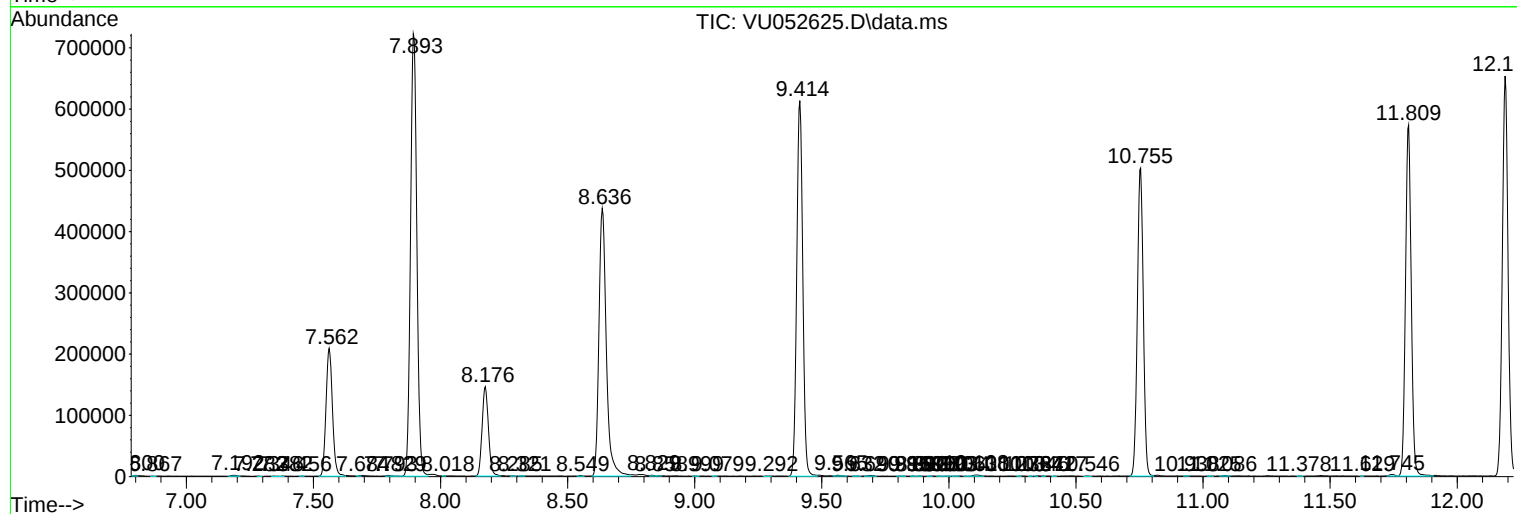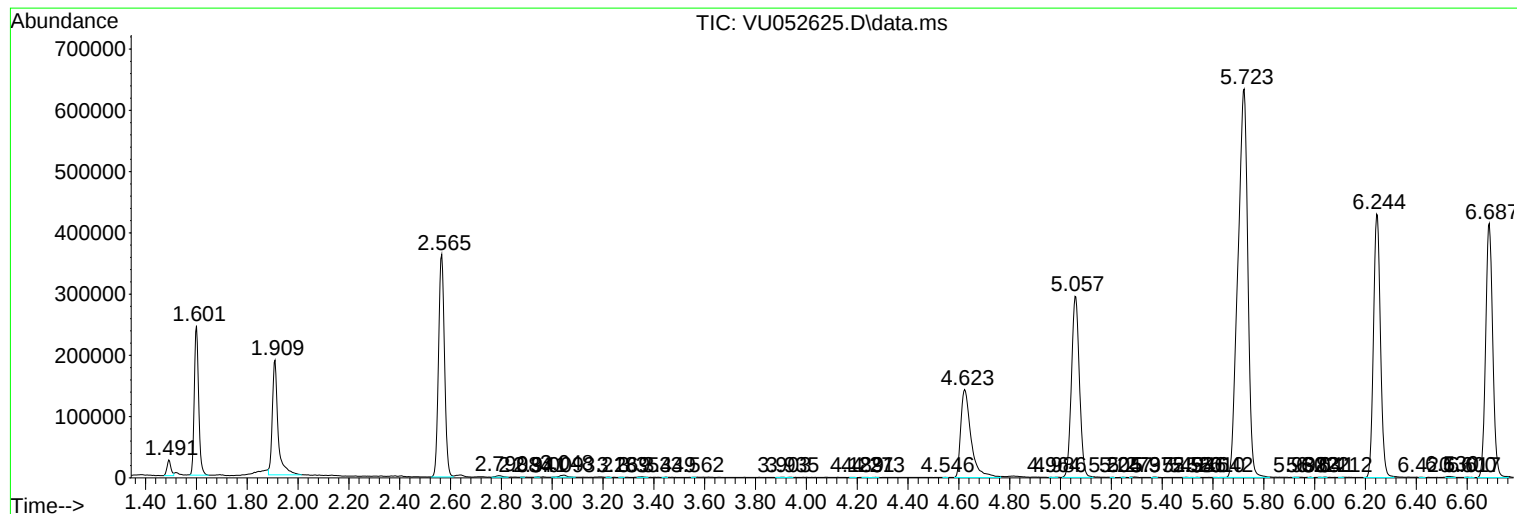

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052625.D
Acq On : 06 Jan 2023 13:58
Operator : JC/MD
Sample : VU0106WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK035

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052625.D
Acq On : 06 Jan 2023 13:58
Operator : JC/MD
Sample : VU0106WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK035

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------