

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052626.D
 Acq On : 06 Jan 2023 14:33
 Operator : JC/MD
 Sample : 01036-03 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLEO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	41	47	55	rBV	27719	29063	0.58%	0.141%
2	1.600	73	81	95	rVB	242179	279501	5.61%	1.356%
3	1.912	170	178	196	rVB	177772	248965	5.00%	1.208%
4	2.568	369	382	396	rBV	350806	572128	11.48%	2.776%
5	2.726	424	431	437	rVB5	721	1209	0.02%	0.006%
6	2.752	437	439	442	rVB2	391	216	0.00%	0.001%
7	2.793	446	452	463	rVB3	1632	2924	0.06%	0.014%
8	3.047	521	531	546	rVB2	5468	10804	0.22%	0.052%
9	3.179	569	572	585	rVB3	933	1764	0.04%	0.009%
10	3.231	585	588	591	rBV2	332	292	0.01%	0.001%
11	3.359	625	628	633	rVV4	664	709	0.01%	0.003%
12	3.491	665	669	673	rBV	357	406	0.01%	0.002%
13	3.549	683	687	691	rVB2	282	243	0.00%	0.001%
14	3.607	702	705	710	rBV3	362	357	0.01%	0.002%
15	3.690	728	731	734	rBV2	235	196	0.00%	0.001%
16	3.764	752	754	760	rVB2	302	331	0.01%	0.002%
17	3.796	760	764	767	rBV3	403	353	0.01%	0.002%
18	3.816	767	770	774	rVB2	319	246	0.00%	0.001%
19	3.841	774	778	783	rBV2	293	288	0.01%	0.001%
20	3.896	792	795	800	rVV2	215	224	0.00%	0.001%
21	4.096	850	857	861	rBV3	257	372	0.01%	0.002%
22	4.349	932	936	940	rBV	238	249	0.00%	0.001%
23	4.372	940	943	947	rVB2	380	260	0.01%	0.001%
24	4.530	984	992	995	rBV3	1026	1104	0.02%	0.005%
25	4.546	995	997	1003	rVB4	616	422	0.01%	0.002%
26	4.620	1003	1020	1044	rBV	143307	365703	7.34%	1.774%
27	4.822	1071	1083	1096	rVB8	1503	3581	0.07%	0.017%
28	4.931	1114	1117	1121	rVB3	316	267	0.01%	0.001%
29	5.060	1141	1157	1186	rVV	287750	631994	12.68%	3.066%
30	5.224	1204	1208	1210	rVB3	436	352	0.01%	0.002%
31	5.282	1218	1226	1228	rBV3	539	612	0.01%	0.003%
32	5.346	1241	1246	1250	rBV2	162	201	0.00%	0.001%
33	5.372	1250	1254	1255	rBV3	679	486	0.01%	0.002%
34	5.465	1277	1283	1286	rBV2	271	226	0.00%	0.001%
35	5.520	1293	1300	1311	rVB4	1799	3244	0.07%	0.016%
36	5.575	1311	1317	1322	rVB3	352	421	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052626.D
 Acq On : 06 Jan 2023 14:33
 Operator : JC/MD
 Sample : 01036-03 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLEO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	5.603	1322	1326	1330	rBV3	338	328	0.01%	0.002%
38	5.626	1330	1333	1337	rBV3	289	223	0.00%	0.001%
39	5.722	1340	1363	1372	rBV2	612013	1657175	33.25%	8.039%
40	5.915	1421	1423	1424	rBV	470	230	0.00%	0.001%
41	5.999	1447	1449	1455	rBV3	247	207	0.00%	0.001%
42	6.086	1471	1476	1480	rBV	314	355	0.01%	0.002%
43	6.111	1480	1484	1488	rVV2	376	325	0.01%	0.002%
44	6.247	1512	1526	1548	rBV	449284	846507	16.98%	4.107%
45	6.407	1573	1576	1581	rVB2	357	300	0.01%	0.001%
46	6.501	1602	1605	1609	rVB2	320	253	0.01%	0.001%
47	6.533	1609	1615	1621	rBV6	1196	1695	0.03%	0.008%
48	6.687	1649	1663	1682	rBV	397437	767648	15.40%	3.724%
49	6.803	1694	1699	1706	rVB5	1238	1612	0.03%	0.008%
50	6.870	1715	1720	1723	rBV3	243	232	0.00%	0.001%
51	6.906	1728	1731	1733	rBV3	340	204	0.00%	0.001%
52	7.009	1759	1763	1766	rBV2	384	340	0.01%	0.002%
53	7.083	1784	1786	1793	rBV4	323	404	0.01%	0.002%
54	7.176	1801	1815	1817	rBV3	824	1284	0.03%	0.006%
55	7.192	1817	1820	1824	rVB5	1004	927	0.02%	0.004%
56	7.234	1827	1833	1835	rBV2	355	338	0.01%	0.002%
57	7.304	1847	1855	1857	rBV2	406	558	0.01%	0.003%
58	7.353	1867	1870	1875	rVB3	315	310	0.01%	0.002%
59	7.562	1922	1935	1957	rBV	193129	349358	7.01%	1.695%
60	7.896	2025	2039	2057	rBV	694317	1187436	23.83%	5.761%
61	8.124	2107	2110	2112	rBV	565	366	0.01%	0.002%
62	8.176	2114	2126	2148	rVV	137830	236554	4.75%	1.148%
63	8.459	2209	2214	2217	rVB3	436	374	0.01%	0.002%
64	8.555	2239	2244	2249	rVB5	1051	869	0.02%	0.004%
65	8.581	2249	2252	2255	rVB3	336	198	0.00%	0.001%
66	8.632	2255	2268	2297	rBV2	406004	778975	15.63%	3.779%
67	9.053	2396	2399	2403	rBV2	294	253	0.01%	0.001%
68	9.443	2499	2520	2543	rBV2	2456894	4983979	100.00%	24.179%
69	9.648	2582	2584	2587	rBV2	391	242	0.00%	0.001%
70	9.799	2629	2631	2636	rBV3	252	244	0.00%	0.001%
71	9.844	2641	2645	2647	rVB3	393	280	0.01%	0.001%
72	9.867	2647	2652	2654	rBV3	363	385	0.01%	0.002%
73	9.934	2670	2673	2675	rVB	382	229	0.00%	0.001%
74	9.960	2678	2681	2684	rVB3	358	216	0.00%	0.001%
75	9.983	2684	2688	2689	rBV2	315	243	0.00%	0.001%
76	10.037	2701	2705	2707	rBV2	319	217	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052626.D
 Acq On : 06 Jan 2023 14:33
 Operator : JC/MD
 Sample : 01036-03 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLEO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	10.076	2714	2717	2719	rVB2	390	207	0.00%	0.001%
78	10.108	2722	2727	2737	rVB6	1447	2411	0.05%	0.012%
79	10.182	2747	2750	2755	rBV3	294	279	0.01%	0.001%
80	10.217	2755	2761	2768	rVB3	535	784	0.02%	0.004%
81	10.250	2768	2771	2773	rBV	297	232	0.00%	0.001%
82	10.295	2778	2785	2787	rBV3	281	362	0.01%	0.002%
83	10.333	2792	2797	2806	rBV3	385	687	0.01%	0.003%
84	10.484	2837	2844	2846	rBV4	594	736	0.01%	0.004%
85	10.565	2864	2869	2871	rBV2	327	323	0.01%	0.002%
86	10.751	2914	2927	2945	rBV	454754	735338	14.75%	3.567%
87	10.893	2969	2971	2975	rBV4	343	215	0.00%	0.001%
88	10.992	2999	3002	3004	rBV	311	225	0.00%	0.001%
89	11.021	3009	3011	3017	rVB2	305	227	0.00%	0.001%
90	11.089	3026	3032	3038	rBV4	919	1286	0.03%	0.006%
91	11.124	3038	3043	3053	rVB5	848	1231	0.02%	0.006%
92	11.336	3106	3109	3111	rBV	404	255	0.01%	0.001%
93	11.610	3189	3194	3197	rBV2	474	518	0.01%	0.003%
94	11.696	3213	3221	3224	rBV2	578	768	0.02%	0.004%
95	11.741	3224	3235	3244	rVV	131019	200761	4.03%	0.974%
96	11.832	3244	3263	3301	rVB2	1224918	2811748	56.42%	13.641%
97	12.204	3361	3379	3407	rBV2	1645876	3433293	68.89%	16.656%
98	13.835	3874	3886	3902	rBV	218899	350311	7.03%	1.699%
99	14.085	3959	3964	3975	rVB4	5485	7960	0.16%	0.039%
100	14.327	4029	4039	4055	rBV2	51160	81484	1.63%	0.395%




Sum of corrected areas: 20613227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052626.D
Acq On : 06 Jan 2023 14:33
Operator : JC/MD
Sample : 01036-03 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLEO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

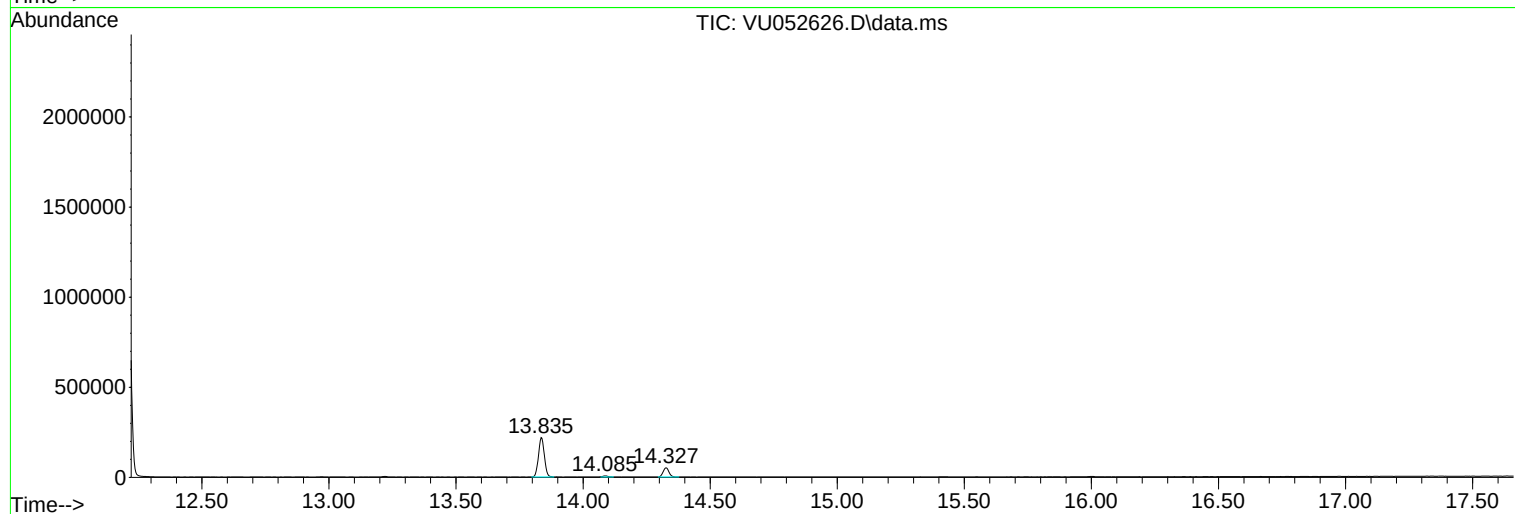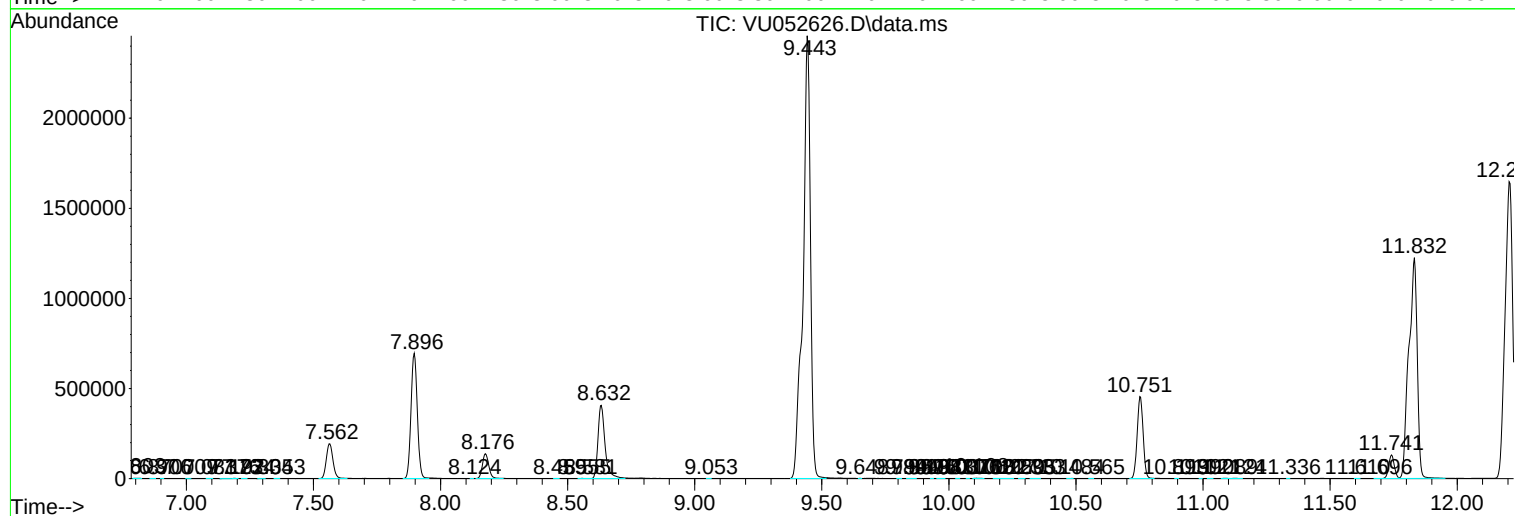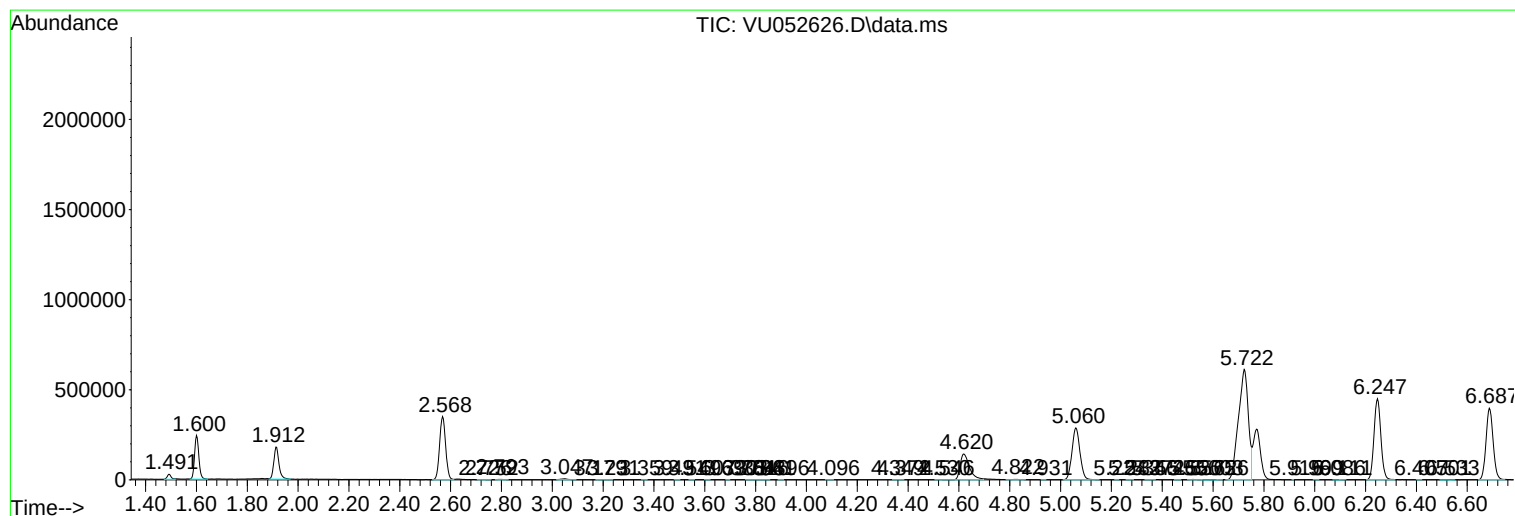

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052626.D
Acq On : 06 Jan 2023 14:33
Operator : JC/MD
Sample : 01036-03 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052626.D
Acq On : 06 Jan 2023 14:33
Operator : JC/MD
Sample : 01036-03 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------