

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052627.D
 Acq On : 06 Jan 2023 14:55
 Operator : JC/MD
 Sample : 01036-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	52	56	68	rVB2	5890	6629	0.39%	0.055%
2	1.600	73	81	99	rVB	238799	279005	16.50%	2.313%
3	1.909	169	177	200	rVB	185340	269040	15.91%	2.230%
4	2.565	368	381	395	rBV	359382	576908	34.11%	4.782%
5	2.633	396	402	420	rVB	5875	11540	0.68%	0.096%
6	2.713	424	427	428	rBV	462	241	0.01%	0.002%
7	2.790	443	451	454	rBV2	1562	1957	0.12%	0.016%
8	2.964	502	505	510	rBV3	473	351	0.02%	0.003%
9	3.044	521	530	540	rVB4	2447	4409	0.26%	0.037%
10	3.179	560	572	586	rBV	6725	15643	0.92%	0.130%
11	3.250	591	594	600	rVV5	674	827	0.05%	0.007%
12	3.334	615	620	621	rBV2	298	239	0.01%	0.002%
13	3.452	650	657	660	rBV3	257	283	0.02%	0.002%
14	3.829	768	774	778	rBV2	276	324	0.02%	0.003%
15	4.063	844	847	853	rBV	344	254	0.02%	0.002%
16	4.221	891	896	898	rBV2	325	280	0.02%	0.002%
17	4.311	919	924	929	rBV2	386	441	0.03%	0.004%
18	4.353	934	937	940	rVV	411	266	0.02%	0.002%
19	4.456	967	969	975	rVB2	281	245	0.01%	0.002%
20	4.623	1008	1021	1060	rBV	143954	392489	23.21%	3.253%
21	4.944	1116	1121	1124	rBV4	228	232	0.01%	0.002%
22	5.060	1140	1157	1183	rVV	291765	638263	37.74%	5.290%
23	5.231	1206	1210	1212	rBV2	466	355	0.02%	0.003%
24	5.285	1224	1227	1230	rBV	434	361	0.02%	0.003%
25	5.330	1238	1241	1244	rBV2	751	521	0.03%	0.004%
26	5.369	1248	1253	1255	rBV3	432	439	0.03%	0.004%
27	5.520	1297	1300	1304	rVB	326	269	0.02%	0.002%
28	5.542	1304	1307	1310	rBV3	263	229	0.01%	0.002%
29	5.722	1341	1363	1393	rBV2	620478	1691155	100.00%	14.017%
30	5.886	1411	1414	1417	rVB	409	255	0.02%	0.002%
31	5.925	1422	1426	1428	rBV3	350	290	0.02%	0.002%
32	5.938	1428	1430	1435	rVB2	520	409	0.02%	0.003%
33	6.121	1483	1487	1491	rVB2	537	528	0.03%	0.004%
34	6.147	1491	1495	1499	rBV3	348	350	0.02%	0.003%
35	6.247	1510	1526	1550	rBV	436557	827181	48.91%	6.856%
36	6.440	1583	1586	1589	rVB3	401	281	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052627.D
 Acq On : 06 Jan 2023 14:55
 Operator : JC/MD
 Sample : 01036-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	6.459	1589	1592	1594	rBV2	488	355	0.02%	0.003%
38	6.517	1604	1610	1611	rBV2	746	510	0.03%	0.004%
39	6.526	1611	1613	1621	rVB5	1025	976	0.06%	0.008%
40	6.597	1626	1635	1637	rBV3	491	673	0.04%	0.006%
41	6.610	1637	1639	1647	rVB4	584	417	0.02%	0.003%
42	6.687	1647	1663	1684	rBV	406596	788268	46.61%	6.534%
43	6.851	1712	1714	1718	rVB3	409	282	0.02%	0.002%
44	6.906	1729	1731	1734	rVV	294	240	0.01%	0.002%
45	6.928	1735	1738	1743	rVV3	365	337	0.02%	0.003%
46	6.964	1745	1749	1754	rVV2	404	421	0.02%	0.003%
47	6.993	1755	1758	1761	rVV2	283	253	0.01%	0.002%
48	7.028	1765	1769	1774	rBV3	275	321	0.02%	0.003%
49	7.157	1805	1809	1811	rVV	365	317	0.02%	0.003%
50	7.185	1811	1818	1827	rVV4	1573	2430	0.14%	0.020%
51	7.337	1862	1865	1870	rVV3	324	318	0.02%	0.003%
52	7.388	1877	1881	1884	rVV2	430	337	0.02%	0.003%
53	7.562	1921	1935	1959	rBV	205231	362776	21.45%	3.007%
54	7.684	1967	1973	1974	rBV2	851	724	0.04%	0.006%
55	7.793	2003	2007	2013	rVB4	735	763	0.05%	0.006%
56	7.893	2024	2038	2059	rBV	715183	1219354	72.10%	10.107%
57	8.050	2083	2087	2090	rBV2	395	379	0.02%	0.003%
58	8.118	2104	2108	2112	rVB3	386	348	0.02%	0.003%
59	8.176	2112	2126	2148	rBV	145498	247489	14.63%	2.051%
60	8.253	2148	2150	2155	rVB5	259	228	0.01%	0.002%
61	8.468	2208	2217	2228	rVB2	8312	14247	0.84%	0.118%
62	8.517	2228	2232	2236	rVB3	431	344	0.02%	0.003%
63	8.546	2236	2241	2244	rVB3	377	356	0.02%	0.003%
64	8.632	2256	2268	2303	rBV2	441818	850494	50.29%	7.049%
65	8.941	2361	2364	2368	rVB3	680	490	0.03%	0.004%
66	9.185	2432	2440	2442	rBV3	392	442	0.03%	0.004%
67	9.253	2458	2461	2466	rBV	400	376	0.02%	0.003%
68	9.336	2480	2487	2490	rBV3	335	426	0.03%	0.004%
69	9.414	2497	2511	2534	rBV	615473	1023151	60.50%	8.480%
70	9.542	2548	2551	2553	rBV2	441	278	0.02%	0.002%
71	9.690	2595	2597	2601	rVB4	488	253	0.01%	0.002%
72	9.877	2653	2655	2660	rVB3	377	236	0.01%	0.002%
73	9.967	2678	2683	2688	rBV3	313	291	0.02%	0.002%
74	10.005	2691	2695	2700	rBV2	354	295	0.02%	0.002%
75	10.195	2749	2754	2758	rBV3	418	395	0.02%	0.003%
76	10.237	2764	2767	2772	rBV2	269	237	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052627.D
 Acq On : 06 Jan 2023 14:55
 Operator : JC/MD
 Sample : 01036-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	10.269	2773	2777	2779	rBV2	263	234	0.01%	0.002%
78	10.346	2795	2801	2805	rBV3	453	486	0.03%	0.004%
79	10.433	2824	2828	2831	rBV2	520	342	0.02%	0.003%
80	10.452	2831	2834	2837	rBV2	315	286	0.02%	0.002%
81	10.613	2882	2884	2890	rVB2	306	270	0.02%	0.002%
82	10.668	2898	2901	2907	rVB	410	371	0.02%	0.003%
83	10.751	2914	2927	2954	rBV	507217	802208	47.44%	6.649%
84	10.889	2961	2970	2979	rVB2	7327	11507	0.68%	0.095%
85	10.954	2987	2990	2994	rBV2	400	297	0.02%	0.002%
86	11.131	3042	3045	3049	rVB2	814	634	0.04%	0.005%
87	11.166	3053	3056	3059	rBV2	280	229	0.01%	0.002%
88	11.423	3134	3136	3142	rVB2	450	357	0.02%	0.003%
89	11.471	3145	3151	3154	rBV3	604	531	0.03%	0.004%
90	11.555	3172	3177	3179	rBV2	478	432	0.03%	0.004%
91	11.661	3203	3210	3214	rVV3	477	665	0.04%	0.006%
92	11.738	3227	3234	3242	rBV5	1940	2698	0.16%	0.022%
93	11.809	3243	3256	3279	rBV	574876	926224	54.77%	7.677%
94	11.954	3299	3301	3304	rBV3	361	262	0.02%	0.002%
95	12.060	3325	3334	3353	rVB5	7570	15930	0.94%	0.132%
96	12.188	3361	3374	3392	rBV	636806	1035155	61.21%	8.580%
97	12.330	3414	3418	3423	rBV4	469	617	0.04%	0.005%
98	13.838	3879	3887	3900	rVB3	10325	15762	0.93%	0.131%
99	14.327	4033	4039	4046	rBV4	4195	5465	0.32%	0.045%
100	15.613	4436	4439	4441	rBV	1103	704	0.04%	0.006%




Sum of corrected areas: 12064982

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052627.D
Acq On : 06 Jan 2023 14:55
Operator : JC/MD
Sample : 01036-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

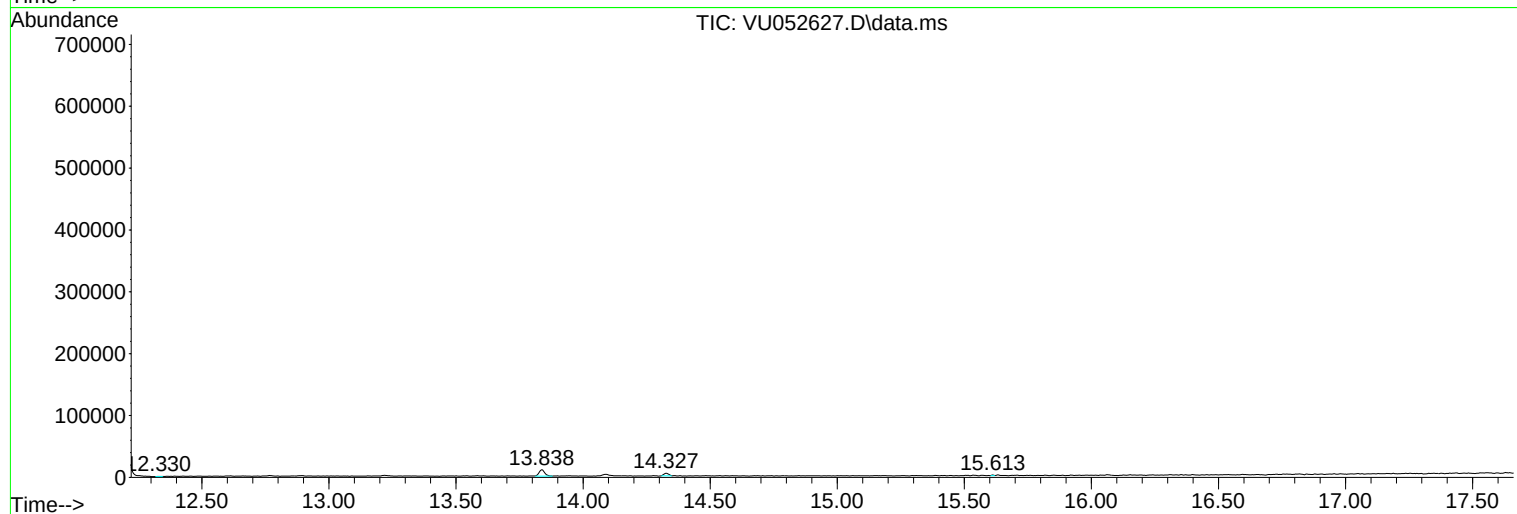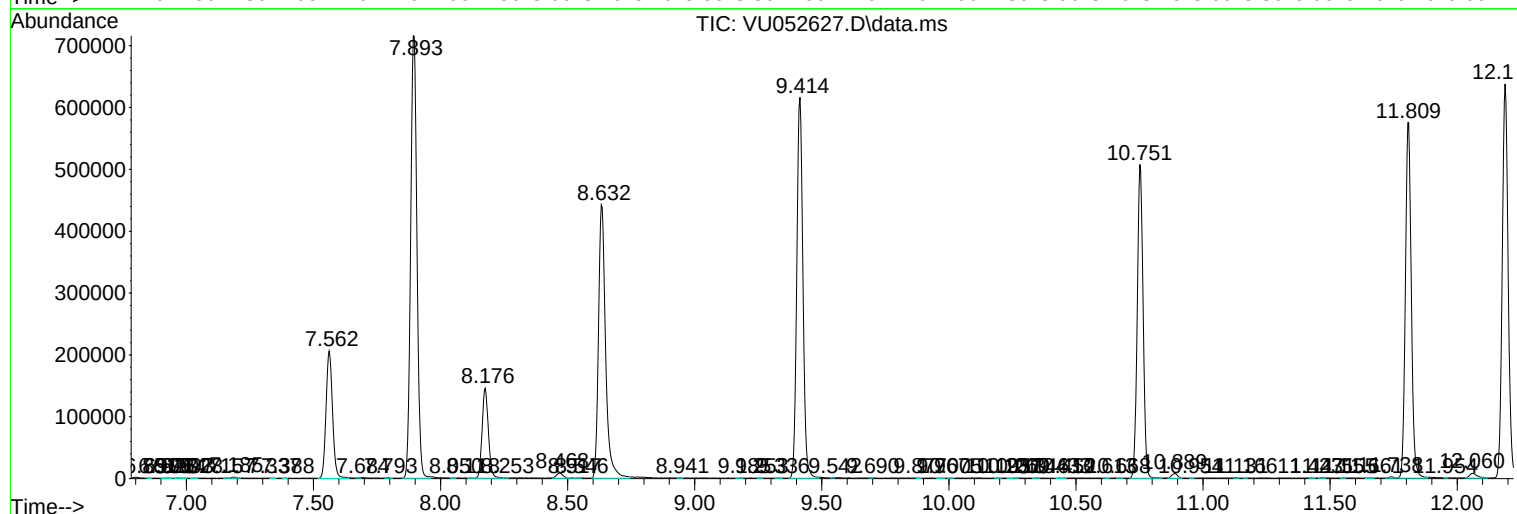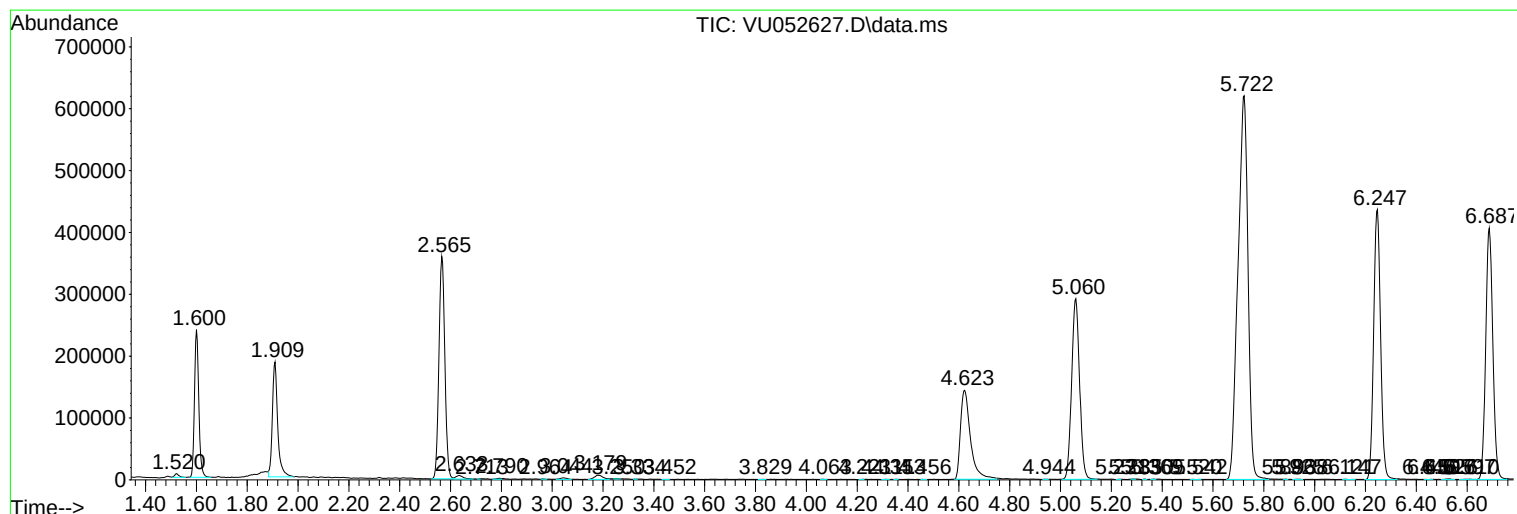

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052627.D
Acq On : 06 Jan 2023 14:55
Operator : JC/MD
Sample : 01036-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052627.D
Acq On : 06 Jan 2023 14:55
Operator : JC/MD
Sample : 01036-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------