

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052628.D
 Acq On : 06 Jan 2023 15:18
 Operator : JC/MD
 Sample : 01036-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	51	56	63	rBV	5665	6649	0.41%	0.057%
2	1.601	73	81	100	rVB	220688	259336	16.09%	2.237%
3	1.906	168	176	197	rVB	176762	251320	15.59%	2.168%
4	2.565	368	381	397	rBV	339357	547150	33.95%	4.720%
5	2.713	424	427	428	rBV3	703	421	0.03%	0.004%
6	2.790	445	451	460	rBV4	1187	1849	0.11%	0.016%
7	2.871	473	476	478	rBV2	495	214	0.01%	0.002%
8	3.047	522	531	540	rVB4	2317	4091	0.25%	0.035%
9	3.183	557	573	587	rBV2	32050	75963	4.71%	0.655%
10	3.379	630	634	639	rBV3	196	232	0.01%	0.002%
11	3.420	644	647	653	rVB	333	254	0.02%	0.002%
12	3.501	669	672	676	rBV	230	199	0.01%	0.002%
13	3.536	676	683	686	rBV3	471	546	0.03%	0.005%
14	3.662	719	722	724	rBV2	305	217	0.01%	0.002%
15	3.732	740	744	750	rBV2	418	583	0.04%	0.005%
16	3.768	751	755	759	rVV3	208	221	0.01%	0.002%
17	3.822	768	772	775	rBV3	250	252	0.02%	0.002%
18	3.967	815	817	822	rVB2	331	210	0.01%	0.002%
19	3.996	822	826	828	rBV2	331	198	0.01%	0.002%
20	4.028	834	836	840	rBV2	293	282	0.02%	0.002%
21	4.112	858	862	865	rVB2	461	304	0.02%	0.003%
22	4.366	937	941	945	rBV3	345	315	0.02%	0.003%
23	4.472	971	974	977	rBV	285	203	0.01%	0.002%
24	4.623	1004	1021	1051	rBV	146901	400647	24.86%	3.456%
25	4.861	1092	1095	1101	rVB3	494	409	0.03%	0.004%
26	4.948	1119	1122	1126	rBV4	430	385	0.02%	0.003%
27	5.057	1139	1156	1182	rBV	281888	616150	38.23%	5.315%
28	5.211	1200	1204	1209	rVB3	523	568	0.04%	0.005%
29	5.237	1209	1212	1213	rBV	421	220	0.01%	0.002%
30	5.276	1220	1224	1226	rBV2	652	459	0.03%	0.004%
31	5.317	1234	1237	1240	rVB2	511	342	0.02%	0.003%
32	5.337	1240	1243	1247	rBV2	418	283	0.02%	0.002%
33	5.382	1250	1257	1261	rVB4	752	854	0.05%	0.007%
34	5.600	1322	1325	1330	rVV2	313	275	0.02%	0.002%
35	5.636	1334	1336	1340	rVV2	259	223	0.01%	0.002%
36	5.719	1340	1362	1399	rVV2	591883	1611604	100.00%	13.901%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052628.D
 Acq On : 06 Jan 2023 15:18
 Operator : JC/MD
 Sample : 01036-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

37	5.871	1404	1409	1411	rBV3	372	331	0.02%	0.003%
38	5.906	1418	1420	1423	rVB2	401	217	0.01%	0.002%
39	5.941	1428	1431	1434	rBV2	358	329	0.02%	0.003%
40	6.044	1455	1463	1468	rBV4	556	766	0.05%	0.007%
41	6.121	1480	1487	1491	rBV2	326	353	0.02%	0.003%
42	6.247	1508	1526	1549	rBV	435403	819470	50.85%	7.069%
43	6.356	1556	1560	1564	rBV3	422	333	0.02%	0.003%
44	6.417	1576	1579	1583	rVB2	329	223	0.01%	0.002%
45	6.526	1605	1613	1619	rBV6	1053	1470	0.09%	0.013%
46	6.600	1632	1636	1639	rVB3	439	330	0.02%	0.003%
47	6.687	1647	1663	1688	rBV	387703	755318	46.87%	6.515%
48	7.006	1758	1762	1765	rVB3	402	376	0.02%	0.003%
49	7.182	1809	1817	1825	rBV5	1701	2901	0.18%	0.025%
50	7.314	1848	1858	1866	rVB2	422	738	0.05%	0.006%
51	7.440	1893	1897	1899	rBV3	280	210	0.01%	0.002%
52	7.562	1918	1935	1959	rBV	194175	343618	21.32%	2.964%
53	7.681	1966	1972	1974	rBV4	639	611	0.04%	0.005%
54	7.822	2014	2016	2019	rBV3	291	201	0.01%	0.002%
55	7.893	2024	2038	2058	rBV	674996	1160700	72.02%	10.012%
56	8.083	2095	2097	2101	rVB3	491	302	0.02%	0.003%
57	8.176	2111	2126	2145	rBV	138480	235337	14.60%	2.030%
58	8.298	2162	2164	2170	rBV	290	246	0.02%	0.002%
59	8.468	2208	2217	2226	rBV2	3069	4938	0.31%	0.043%
60	8.565	2244	2247	2249	rVB	365	218	0.01%	0.002%
61	8.587	2249	2254	2255	rBV2	325	247	0.02%	0.002%
62	8.636	2255	2269	2308	rBV2	416774	801959	49.76%	6.918%
63	8.864	2334	2340	2344	rBV2	683	743	0.05%	0.006%
64	8.960	2366	2370	2373	rBV2	380	324	0.02%	0.003%
65	9.015	2384	2387	2389	rBV2	379	247	0.02%	0.002%
66	9.153	2428	2430	2435	rVB	466	309	0.02%	0.003%
67	9.192	2435	2442	2445	rBV	179	195	0.01%	0.002%
68	9.259	2460	2463	2466	rBV	384	304	0.02%	0.003%
69	9.288	2469	2472	2475	rBV2	318	234	0.01%	0.002%
70	9.359	2490	2494	2497	rBV	264	208	0.01%	0.002%
71	9.414	2497	2511	2530	rBV	602396	996499	61.83%	8.596%
72	9.784	2624	2626	2630	rVB3	323	207	0.01%	0.002%
73	9.854	2646	2648	2655	rVB2	296	270	0.02%	0.002%
74	9.973	2682	2685	2688	rBV2	230	203	0.01%	0.002%
75	10.021	2695	2700	2704	rBV3	268	301	0.02%	0.003%
76	10.140	2733	2737	2741	rVB3	296	246	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
 Data File : VU052628.D
 Acq On : 06 Jan 2023 15:18
 Operator : JC/MD
 Sample : 01036-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
 Title : VOC Analysis

77	10.176	2742	2748	2750	rBV3	367	365	0.02%	0.003%
78	10.256	2769	2773	2777	rBV2	290	267	0.02%	0.002%
79	10.317	2787	2792	2796	rBV3	368	428	0.03%	0.004%
80	10.423	2821	2825	2828	rVB2	292	234	0.01%	0.002%
81	10.446	2828	2832	2838	rBV3	372	529	0.03%	0.005%
82	10.475	2838	2841	2845	rBV3	279	292	0.02%	0.003%
83	10.536	2856	2860	2865	rBV2	272	275	0.02%	0.002%
84	10.571	2869	2871	2874	rBV3	447	330	0.02%	0.003%
85	10.626	2886	2888	2891	rBV	243	199	0.01%	0.002%
86	10.751	2913	2927	2946	rBV	478099	775007	48.09%	6.685%
87	10.886	2960	2969	2978	rVB2	3225	4531	0.28%	0.039%
88	11.128	3042	3044	3051	rVB3	641	722	0.04%	0.006%
89	11.195	3061	3065	3069	rVV2	375	422	0.03%	0.004%
90	11.214	3069	3071	3076	rVB	537	396	0.02%	0.003%
91	11.327	3101	3106	3107	rBV2	219	210	0.01%	0.002%
92	11.436	3138	3140	3144	rVB	367	208	0.01%	0.002%
93	11.472	3147	3151	3157	rVV3	540	529	0.03%	0.005%
94	11.713	3222	3226	3230	rBV2	438	410	0.03%	0.004%
95	11.742	3230	3235	3242	rVB5	1427	1718	0.11%	0.015%
96	11.809	3242	3256	3289	rBV	556450	900420	55.87%	7.767%
97	12.063	3324	3335	3350	rBV5	6401	13302	0.83%	0.115%
98	12.189	3361	3374	3394	rBV	608953	973573	60.41%	8.398%
99	12.369	3427	3430	3435	rBV3	701	681	0.04%	0.006%
100	14.330	4033	4040	4048	rVB5	1642	2557	0.16%	0.022%


Sum of corrected areas: 11593065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052628.D
Acq On : 06 Jan 2023 15:18
Operator : JC/MD
Sample : 01036-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

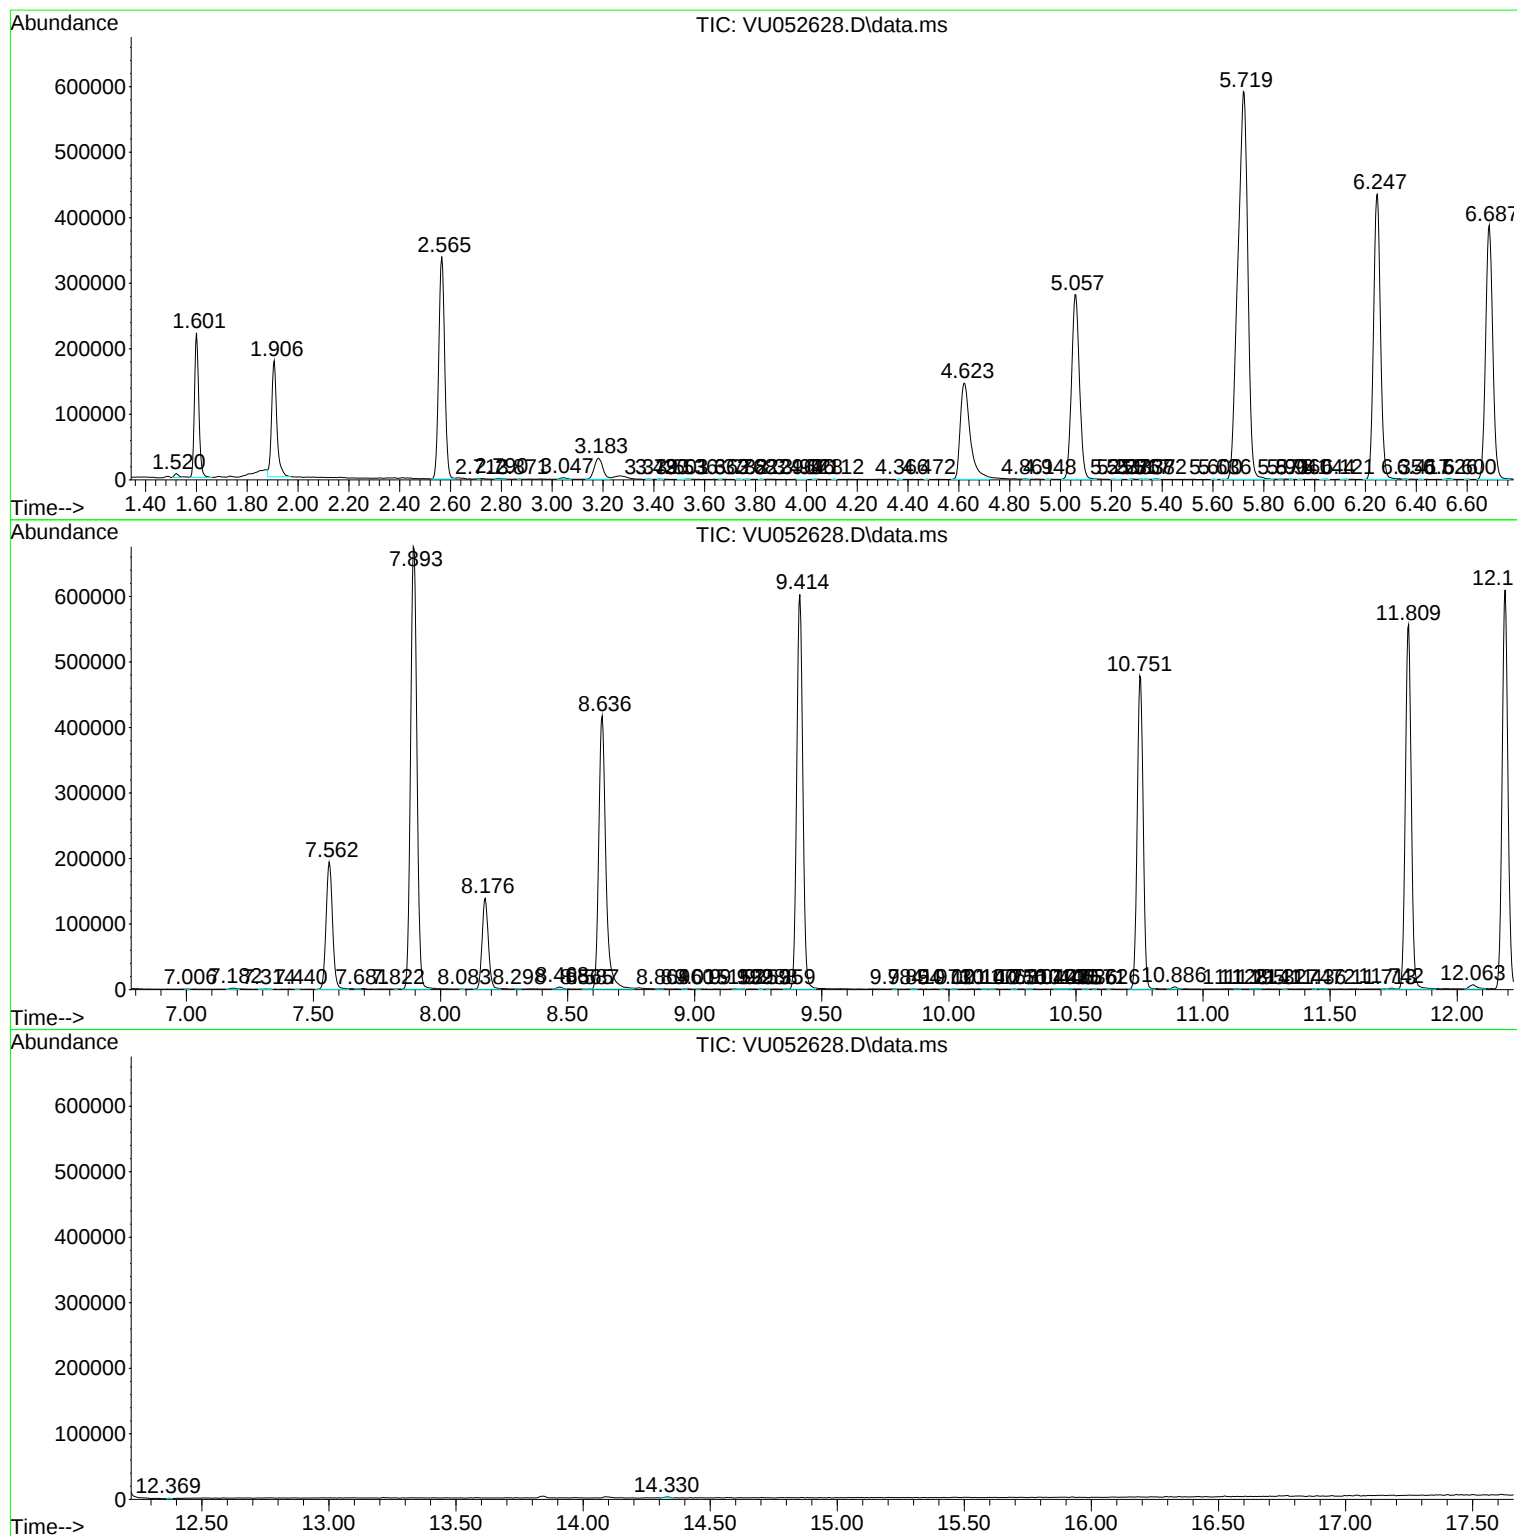

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052628.D
Acq On : 06 Jan 2023 15:18
Operator : JC/MD
Sample : 01036-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010623\
Data File : VU052628.D
Acq On : 06 Jan 2023 15:18
Operator : JC/MD
Sample : 01036-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------